

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
 Data File : BN030804.D
 Acq On : 10 Apr 2024 00:29
 Operator : MA/JU
 Sample : P2013-21
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0MC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030804.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	40	rBV	29473	41861	0.57%	0.069%
2	3.599	101	104	127	rBV	141510	262309	3.57%	0.432%
3	3.911	153	157	162	rBV2	9102	12636	0.17%	0.021%
4	6.852	650	657	672	rVB	188721	321171	4.37%	0.529%
5	7.022	679	686	696	rBV	744580	1172045	15.95%	1.930%
6	7.211	711	718	729	rBV	698648	1106632	15.06%	1.822%
7	7.681	790	798	807	rBV	613578	989510	13.46%	1.629%
8	8.381	910	917	929	rBV	617090	972934	13.24%	1.602%
9	8.834	985	994	1008	rBV	919837	1476598	20.09%	2.431%
10	9.240	1058	1063	1067	rVB3	8086	13879	0.19%	0.023%
11	9.552	1109	1116	1130	rBV	698087	1125974	15.32%	1.854%
12	10.081	1199	1206	1224	rBV	1087744	1827638	24.87%	3.009%
13	10.463	1263	1271	1281	rBV	942089	1599554	21.76%	2.633%
14	10.605	1287	1295	1312	rBV	963542	1678886	22.84%	2.764%
15	12.057	1534	1542	1550	rVB	20476	34566	0.47%	0.057%
16	13.222	1734	1740	1746	rBV2	16120	25507	0.35%	0.042%
17	13.740	1821	1828	1841	rBV	2379314	3347556	45.55%	5.511%
18	14.016	1864	1875	1896	rBV2	2696213	4074683	55.44%	6.708%
19	14.322	1920	1927	1940	rBV	1651619	2401555	32.68%	3.954%
20	14.534	1955	1963	1978	rBV	118601	278029	3.78%	0.458%
21	14.740	1994	1998	2005	rVB9	6212	13302	0.18%	0.022%
22	15.322	2089	2097	2110	rBV	3577491	5249767	71.43%	8.643%
23	15.434	2110	2116	2134	rVV	942314	1404098	19.10%	2.312%
24	15.557	2134	2137	2147	rVB4	18933	33943	0.46%	0.056%
25	16.098	2225	2229	2235	rBV3	10853	17728	0.24%	0.029%
26	16.745	2336	2339	2344	rVB6	5564	8097	0.11%	0.013%
27	16.998	2379	2382	2386	rVB5	8651	10640	0.14%	0.018%
28	17.069	2388	2394	2404	rVV	2114746	3031551	41.25%	4.991%
29	17.169	2405	2411	2424	rVV2	4152971	6021735	81.93%	9.914%
30	17.745	2505	2509	2515	rVB6	16137	24176	0.33%	0.040%
31	17.969	2543	2547	2554	rBV	74665	101143	1.38%	0.167%
32	18.404	2619	2621	2625	rVB5	5580	7390	0.10%	0.012%
33	19.033	2723	2728	2732	rBV2	58002	77378	1.05%	0.127%
34	19.104	2735	2740	2744	rBV	49807	74020	1.01%	0.122%
35	19.257	2762	2766	2771	rBV2	59098	80881	1.10%	0.133%
36	19.469	2796	2802	2811	rBV	5197271	7349765	100.00%	12.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030804.D
Acq On : 10 Apr 2024 00:29
Operator : MA/JU
Sample : P2013-21
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	21.304	3109	3114	3125	rBV2	2400389	3482060	47.38%	5.733%
38	24.039	3570	3579	3592	rBV2	3126151	7345825	99.95%	12.094%
39	24.239	3604	3613	3627	rBV2	1420329	3642208	49.56%	5.996%




Sum of corrected areas: 60739230

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030804.D
Acq On : 10 Apr 2024 00:29
Operator : MA/JU
Sample : P2013-21
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

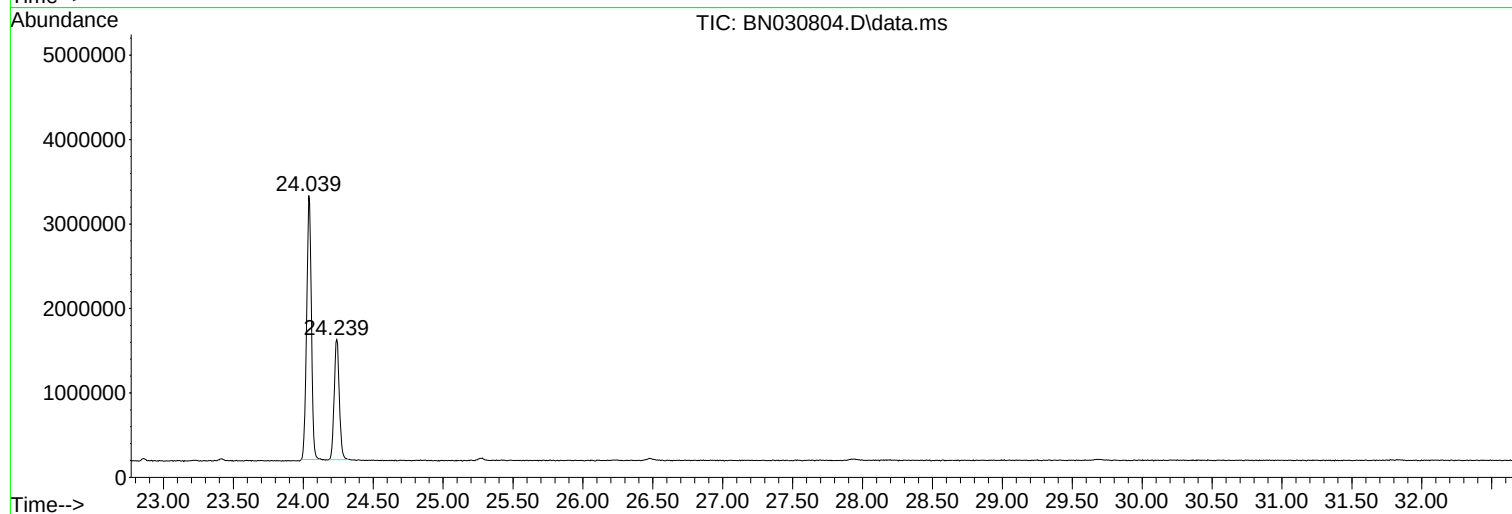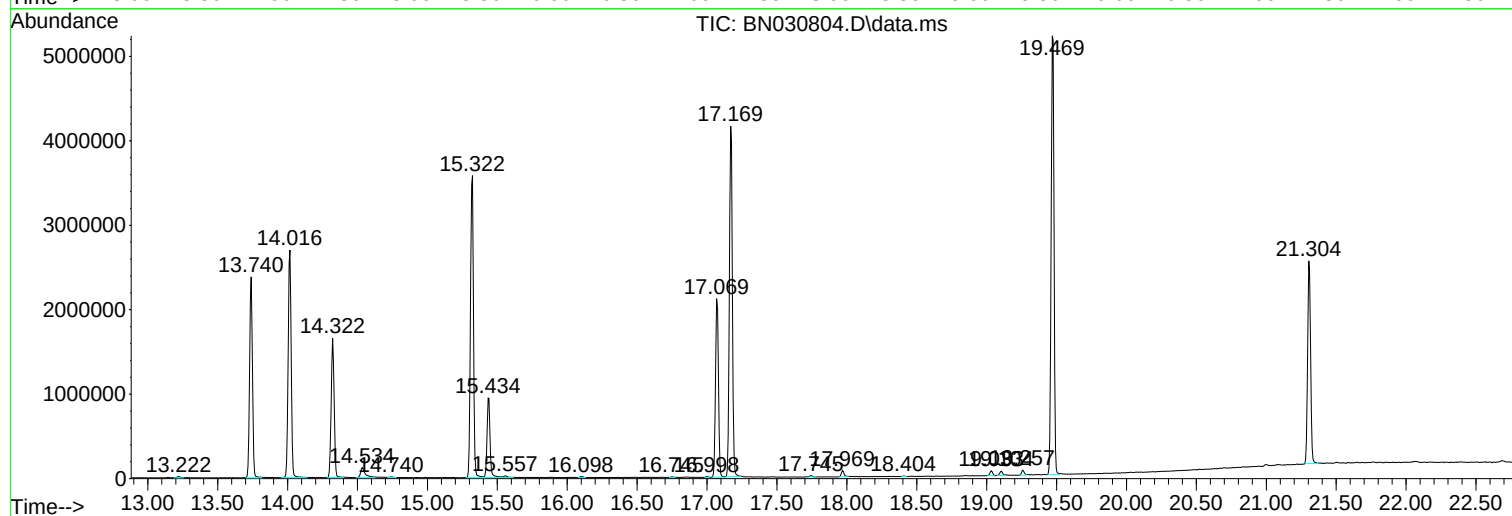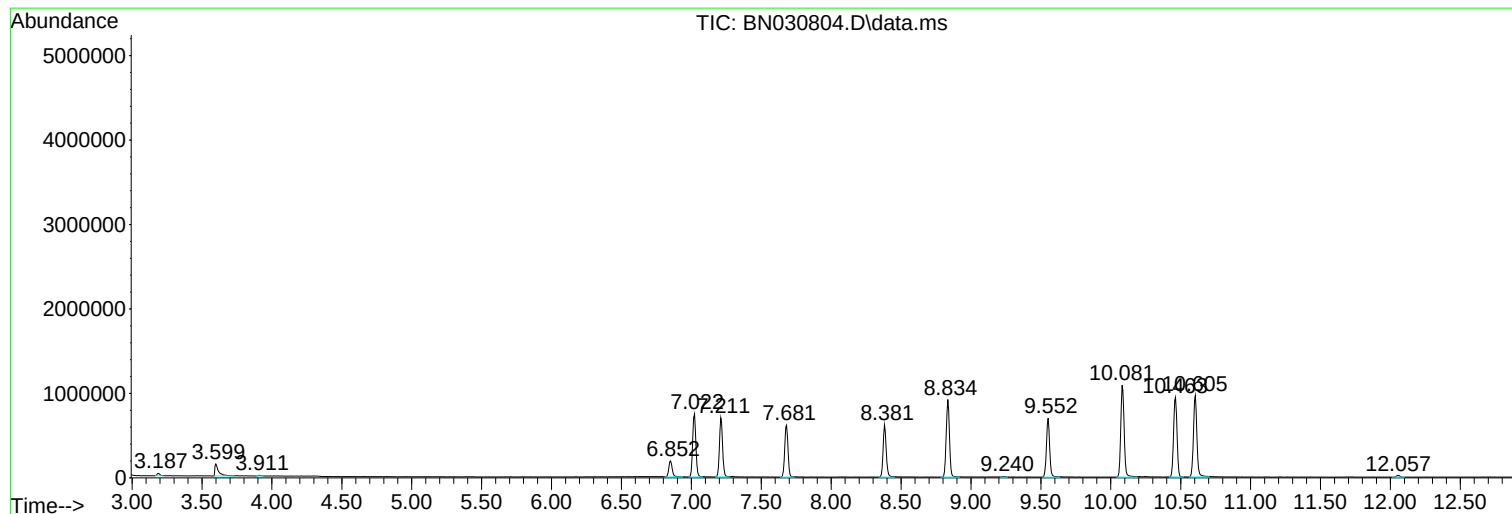

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030804.D
Acq On : 10 Apr 2024 00:29
Operator : MA/JU
Sample : P2013-21
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030804.D
Acq On : 10 Apr 2024 00:29
Operator : MA/JU
Sample : P2013-21
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc