

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
 Data File : BN030805.D
 Acq On : 10 Apr 2024 01:09
 Operator : MA/JU
 Sample : P2013-22
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0MC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	45	rVB	31698	55418	0.74%	0.092%
2	3.599	101	104	121	rBV	223458	407029	5.46%	0.676%
3	3.911	154	157	161	rVB3	7903	10334	0.14%	0.017%
4	6.852	650	657	667	rBV	202807	327061	4.39%	0.543%
5	7.022	680	686	699	rVB	734338	1160066	15.57%	1.926%
6	7.210	712	718	731	rBV	697881	1109496	14.89%	1.842%
7	7.681	790	798	805	rBV	580236	925285	12.42%	1.536%
8	8.381	910	917	930	rBV	633202	1007508	13.52%	1.673%
9	8.834	987	994	1003	rBV	912893	1449274	19.45%	2.406%
10	9.240	1058	1063	1066	rVB4	8721	13949	0.19%	0.023%
11	9.552	1108	1116	1136	rBV	684179	1116036	14.98%	1.853%
12	10.081	1198	1206	1225	rBV	1090213	1808234	24.26%	3.002%
13	10.463	1264	1271	1280	rBV	890406	1481795	19.88%	2.460%
14	10.604	1287	1295	1309	rBV	1050926	1772931	23.79%	2.943%
15	12.057	1537	1542	1550	rVB3	19864	33529	0.45%	0.056%
16	13.145	1722	1727	1734	rVB8	5087	9394	0.13%	0.016%
17	13.216	1734	1739	1748	rBV3	14608	28204	0.38%	0.047%
18	13.740	1817	1828	1842	rBV	2407289	3345845	44.90%	5.554%
19	14.016	1866	1875	1890	rBV	2661724	3989334	53.53%	6.623%
20	14.322	1920	1927	1937	rBV	1509095	2223416	29.84%	3.691%
21	14.534	1957	1963	1976	rBV	128404	286448	3.84%	0.476%
22	14.740	1994	1998	2005	rVB8	7615	14259	0.19%	0.024%
23	15.316	2088	2096	2110	rBV	3598724	5293396	71.03%	8.787%
24	15.434	2110	2116	2132	rVV	942093	1401487	18.81%	2.327%
25	15.557	2134	2137	2145	rVB3	18734	29120	0.39%	0.048%
26	16.104	2225	2230	2235	rBV4	11647	18048	0.24%	0.030%
27	16.751	2335	2340	2343	rBV5	6584	9329	0.13%	0.015%
28	16.998	2378	2382	2387	rBV6	10134	11841	0.16%	0.020%
29	17.069	2387	2394	2404	rBV	2064617	2846629	38.20%	4.726%
30	17.169	2404	2411	2423	rBV2	4332377	6072365	81.48%	10.081%
31	17.463	2457	2461	2466	rBV7	4040	8055	0.11%	0.013%
32	17.739	2506	2508	2512	rVB5	6426	7546	0.10%	0.013%
33	17.969	2542	2547	2555	rBV2	118731	174947	2.35%	0.290%
34	18.845	2693	2696	2702	rVB8	5817	10432	0.14%	0.017%
35	19.033	2723	2728	2732	rBV2	58853	79853	1.07%	0.133%
36	19.104	2735	2740	2744	rBV	54493	83924	1.13%	0.139%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030805.D
Acq On : 10 Apr 2024 01:09
Operator : MA/JU
Sample : P2013-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.257	2762	2766	2771	rBV2	96860	134125	1.80%	0.223%
38	19.469	2796	2802	2814	rBV	5260236	7404547	99.36%	12.292%
39	21.304	3108	3114	3125	rBV2	2312222	3281464	44.03%	5.447%
40	24.039	3570	3579	3592	rBV2	3079386	7452264	100.00%	12.371%
41	24.239	3604	3613	3628	rVB2	1329198	3344160	44.87%	5.552%




Sum of corrected areas: 60238377

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030805.D
Acq On : 10 Apr 2024 01:09
Operator : MA/JU
Sample : P2013-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

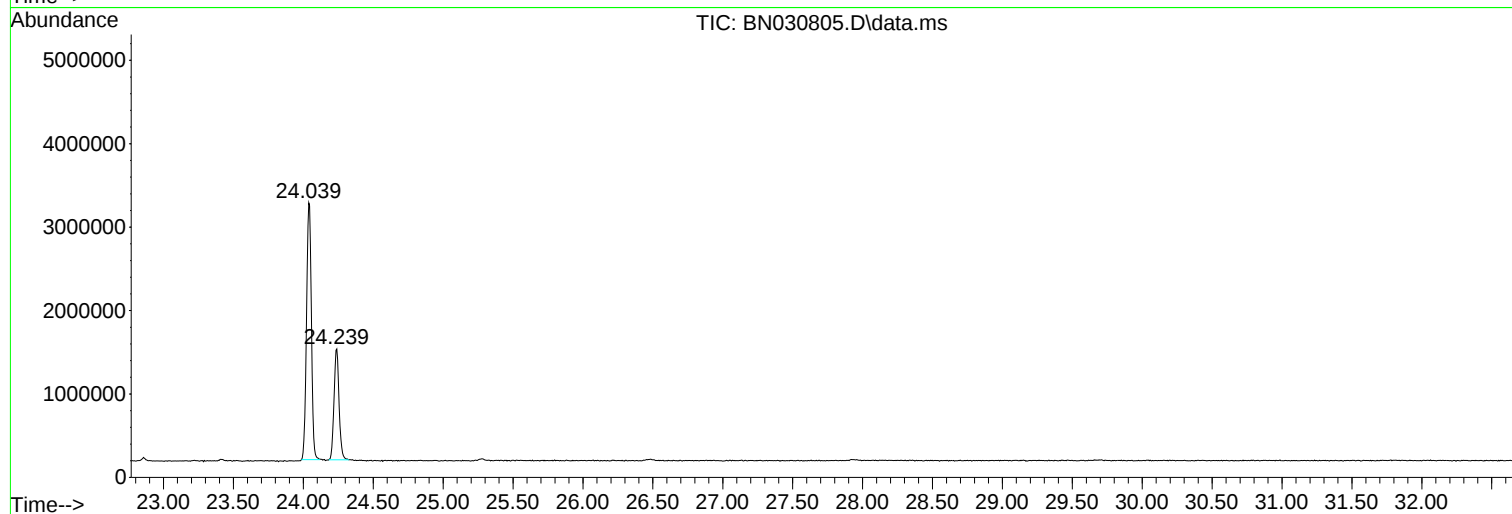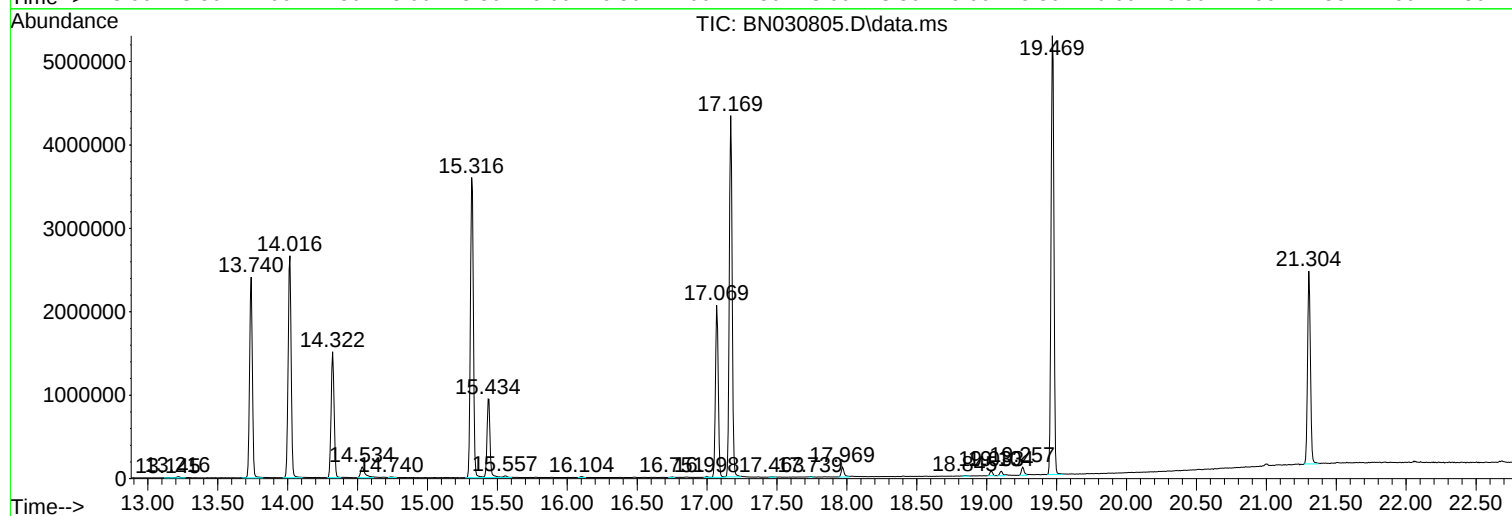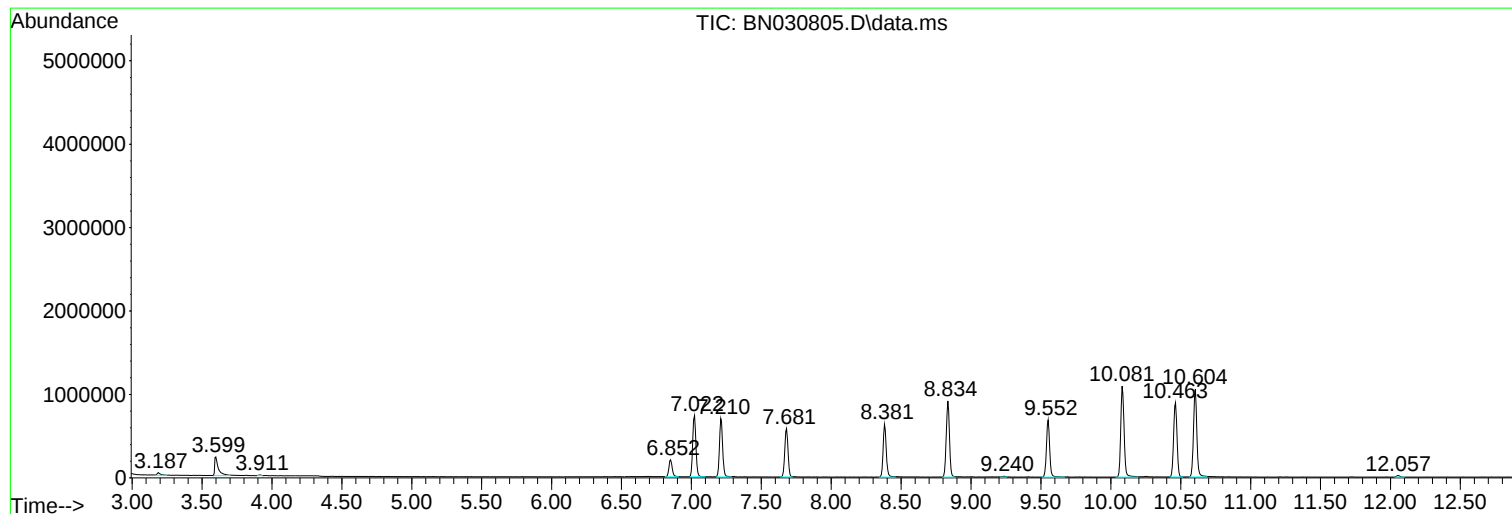

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030805.D
Acq On : 10 Apr 2024 01:09
Operator : MA/JU
Sample : P2013-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030805.D
Acq On : 10 Apr 2024 01:09
Operator : MA/JU
Sample : P2013-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc