
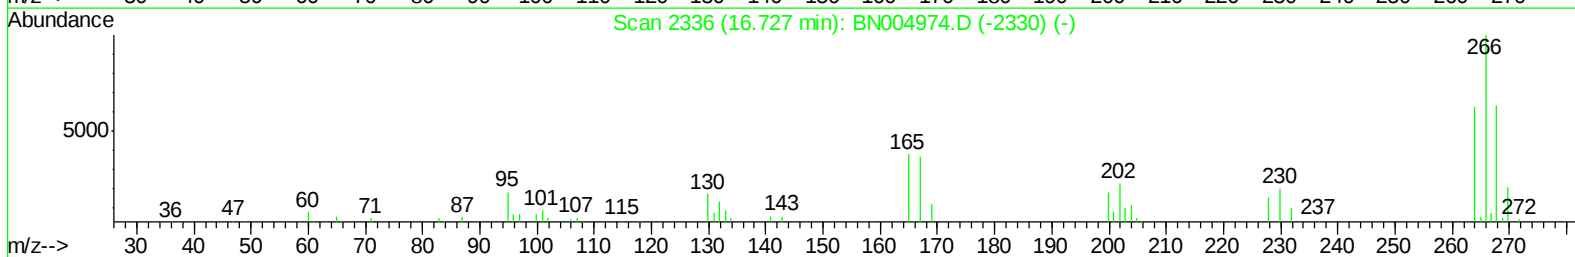
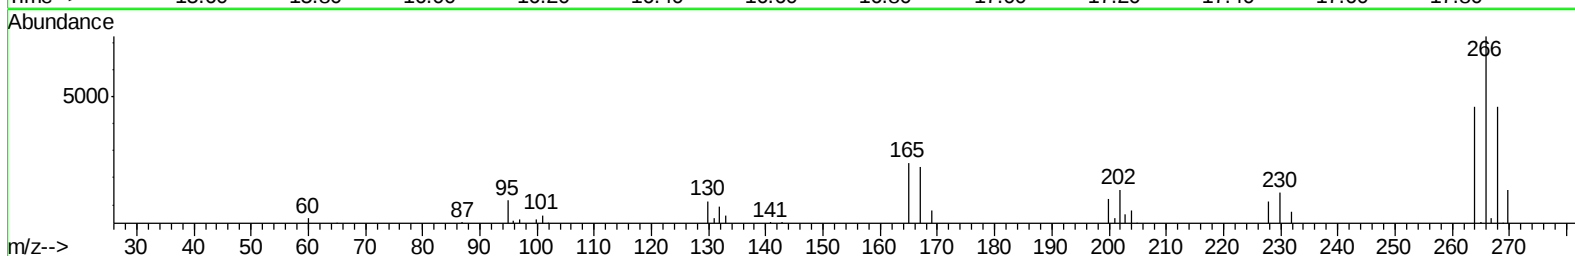


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041019\
Data File : BN005123.D
Acq On : 10 Apr 2019 12:20
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 08:30:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 05:27:09 2019
Response via : Initial Calibration

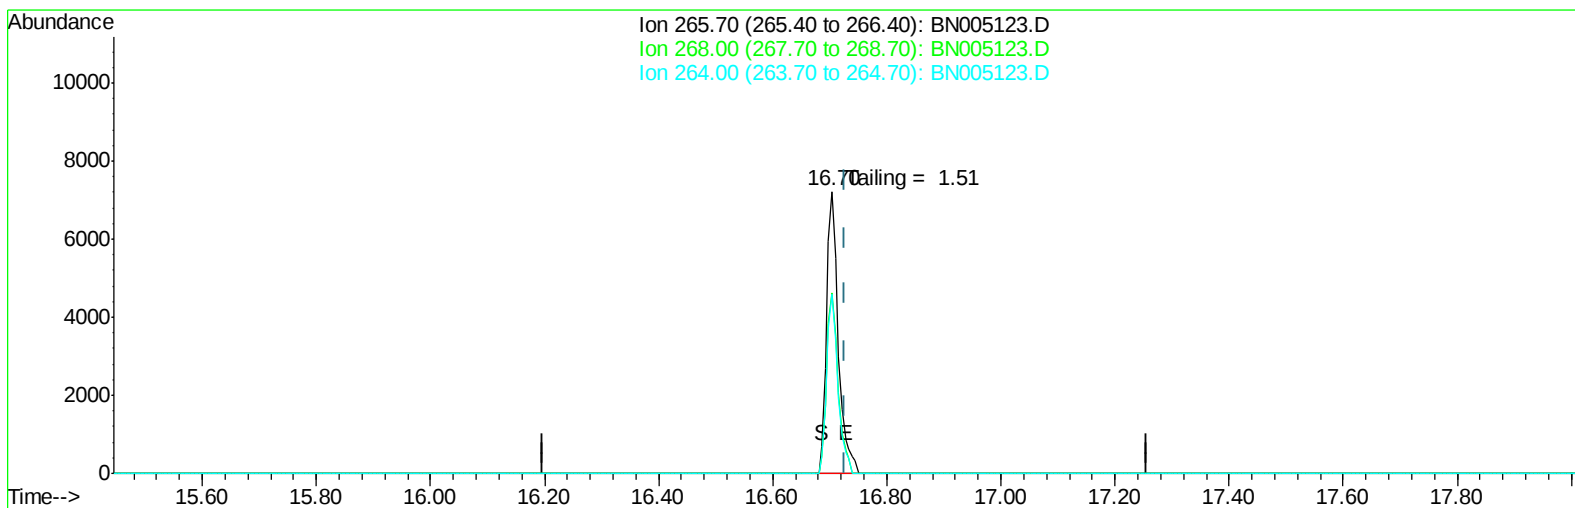

TIC: BN005123.D

(70) Pentachlorophenol (C)




16.704min (-0.024) 0.00ng

response 10188

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	64.26
264.00	62.50	63.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041019\
Data File : BN005123.D
Acq On : 10 Apr 2019 12:20
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 08:30:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 05:27:09 2019
Response via : Initial Calibration

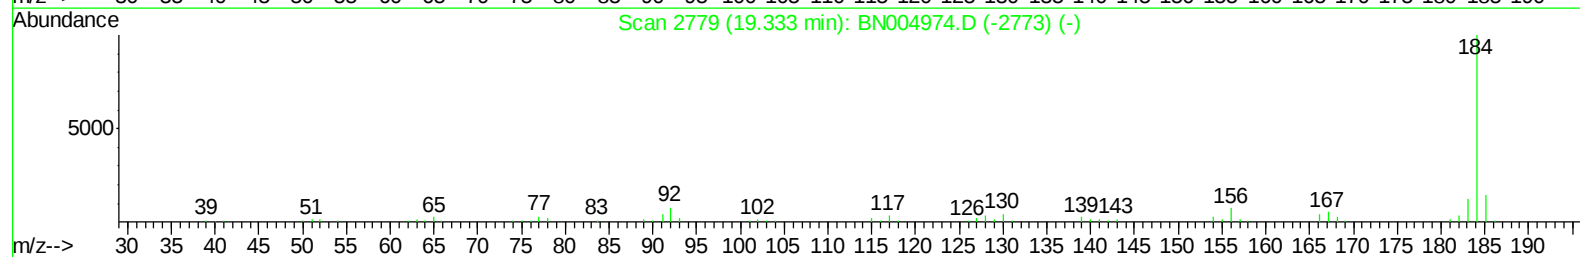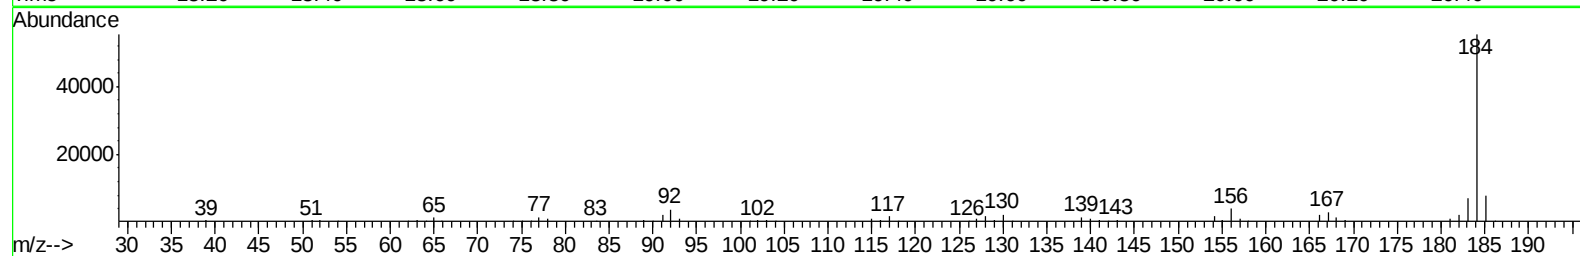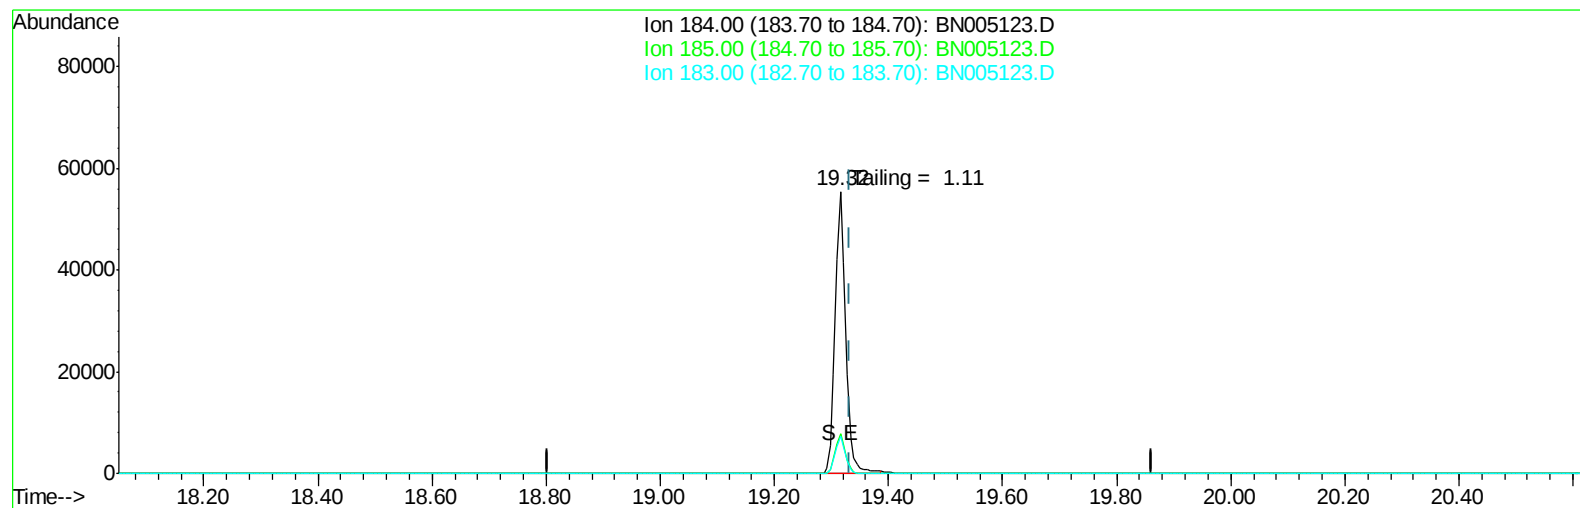

TIC: BN005123.D

(77) Benzidine

19.315min (-0.018) 0.00ng

response 71081

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.19
183.00	12.40	13.03
0.00	0.00	0.00