

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041019\
 Data File : BN005130.D
 Acq On : 10 Apr 2019 16:30
 Operator : JU/SJ
 Sample : K2343-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TP-7-D

Quant Time: Apr 11 08:21:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 05:27:09 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	7686	20.00	ng	-0.02
21) Naphthalene-d8	10.43	136	31312	20.00	ng	-0.03
39) Acenaphthene-d10	14.30	164	17954	20.00	ng	-0.03
64) Phenanthrene-d10	17.05	188	37724	20.00	ng	-0.02
76) Chrysene-d12	21.25	240	32552	20.00	ng	-0.02
87) Perylene-d12	23.48	264	33011	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	58952	132.61	ng	-0.02
7) Phenol-d6	6.83	99	76843	130.32	ng	-0.02
23) Nitrobenzene-d5	8.82	82	42644	82.38	ng	-0.03
42) 2,4,6-Tribromophenol	15.80	330	39028	134.78	ng	-0.02
45) 2-Fluorobiphenyl	12.92	172	116852	86.24	ng	-0.02
79) Terphenyl-d14	19.69	244	159710	94.46	ng	-0.02
Target Compounds						
50) Dimethylphthalate	13.76	163	10131	6.868	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041019\
Data File : BN005130.D
Acq On : 10 Apr 2019 16:30
Operator : JU/SJ
Sample : K2343-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TP-7-D

Quant Time: Apr 11 08:21:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 05:27:09 2019
Response via : Initial Calibration

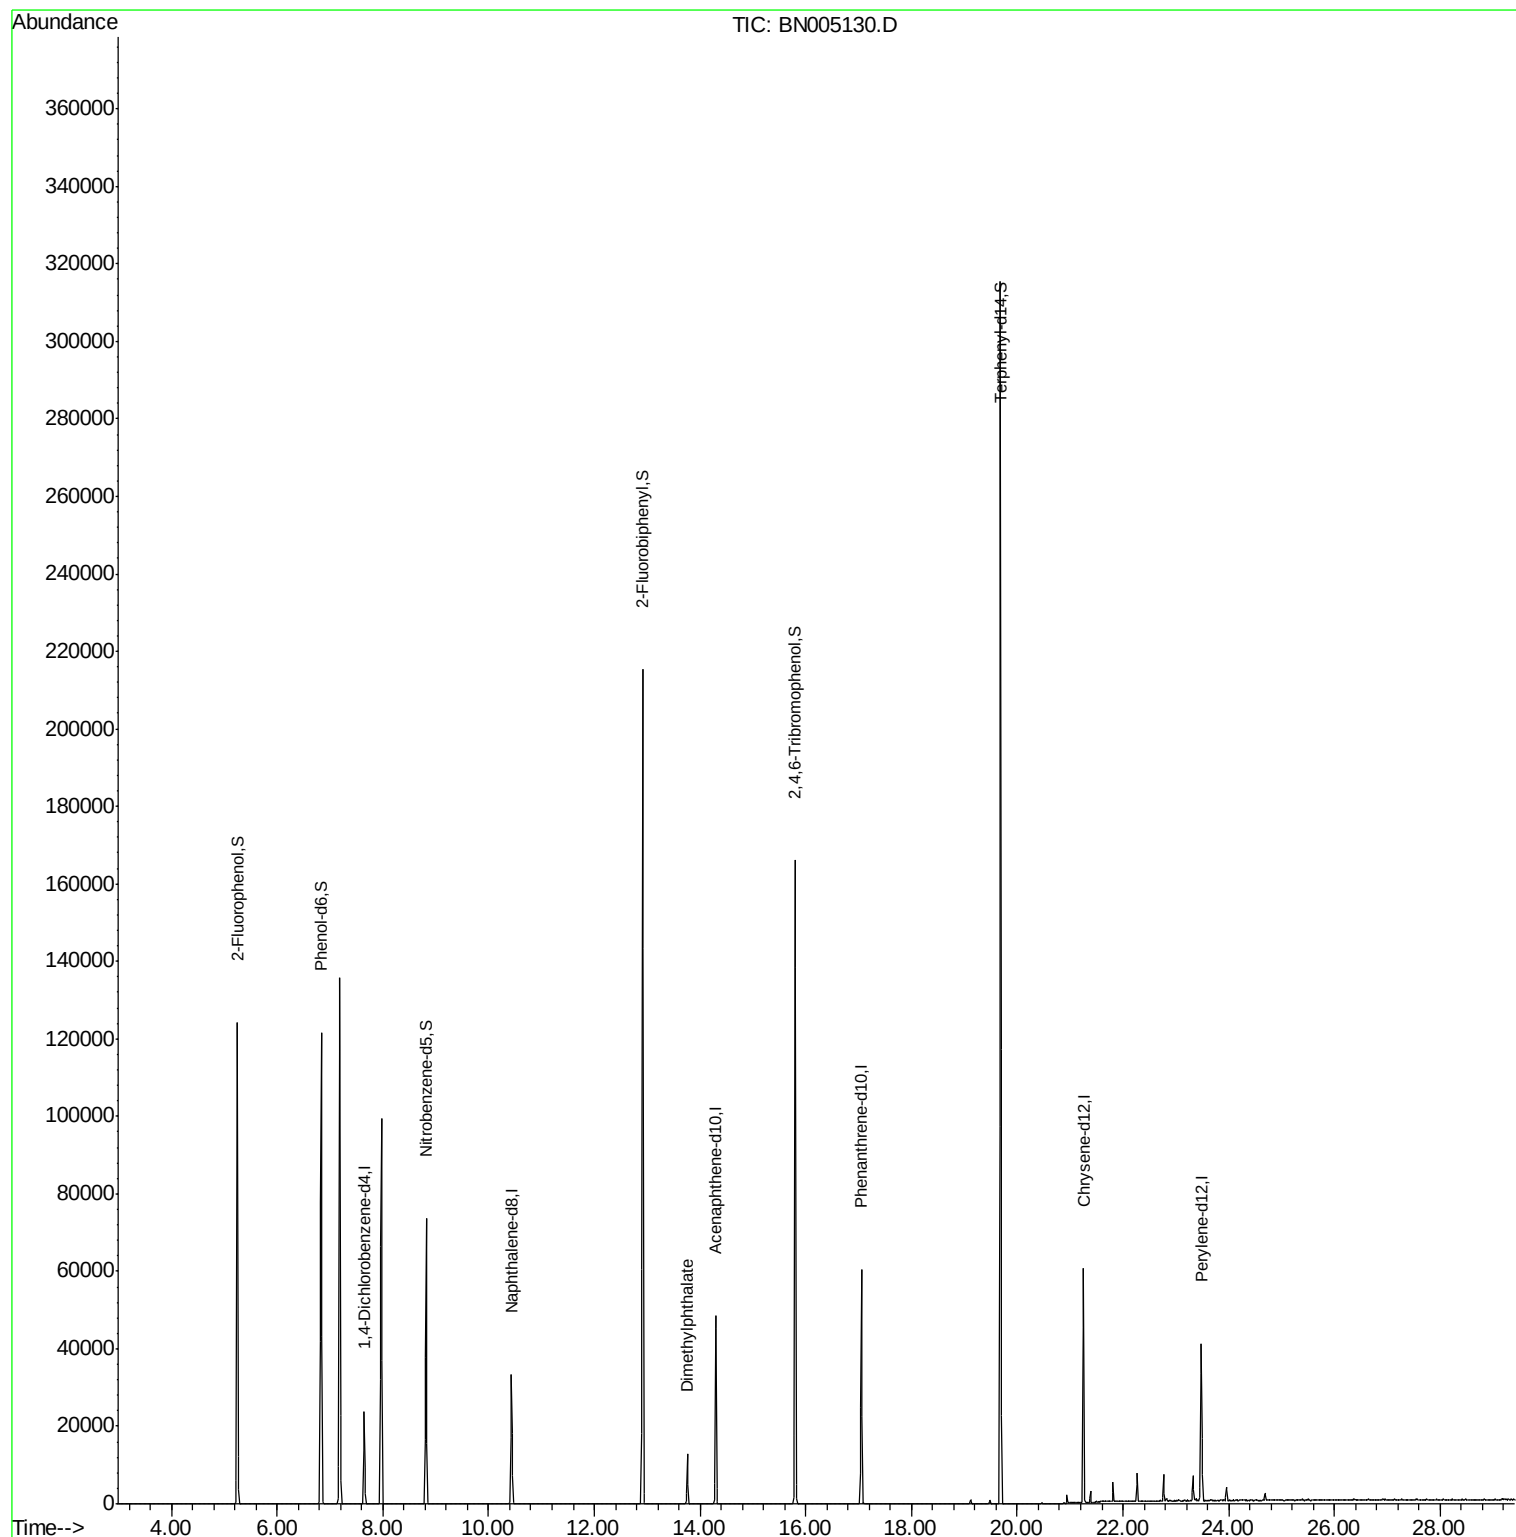

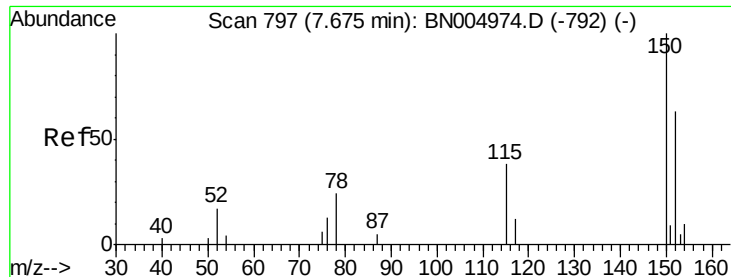


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.65 min Scan# 793
Delta R.T. -0.02 min
Lab File: BN005130.D
Acq: 10 Apr 2019 16:30

Instrument :
BNA_N
ClientSampleId :
TP-7-D

Tot Ion:152 Resp: 7686
Ion Ratio Lower Upper
152 100
150 155.7 126.9 190.3
115 57.1 47.8 71.6

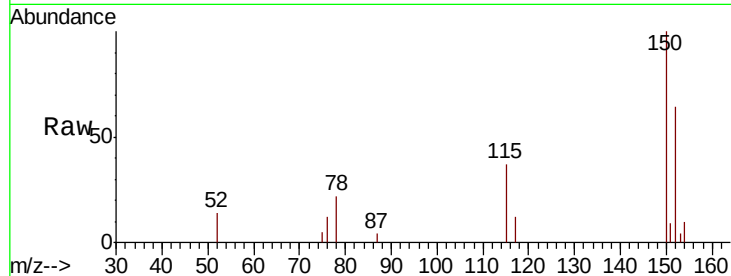


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

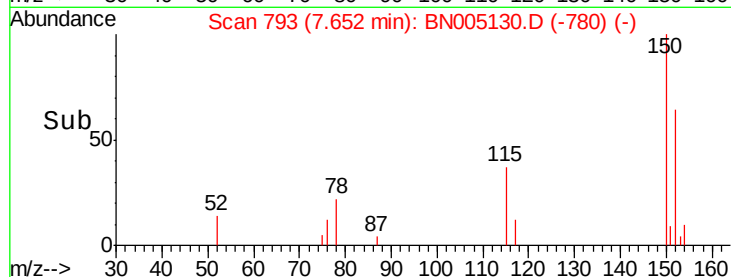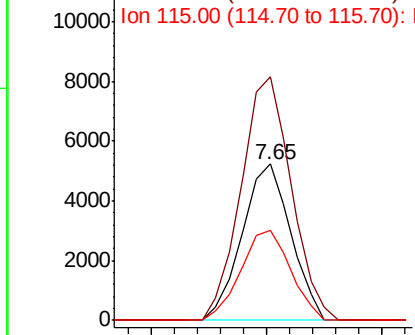



#5


2-Fluorophenol
Concen: 132.607 ng
RT: 5.25 min Scan# 384
Delta R.T. -0.02 min
Lab File: BN005130.D
Acq: 10 Apr 2019 16:30

Tgt Ion:112 Resp: 58952
Ion Ratio Lower Upper
112 100
64 50.0 41.9 62.9
63 25.2 21.4 32.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

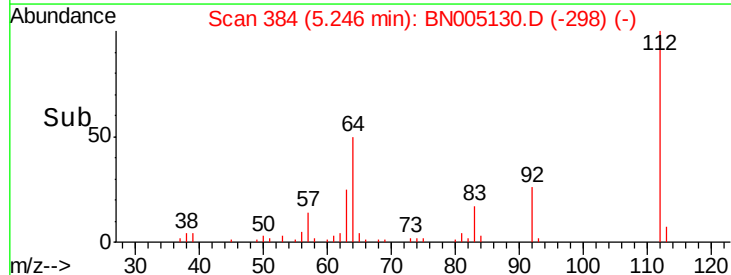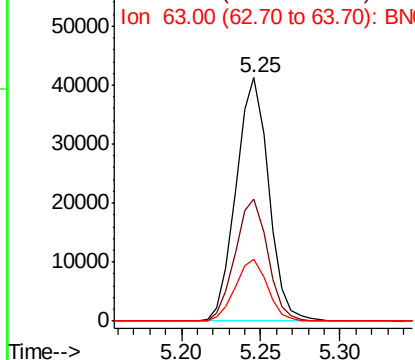

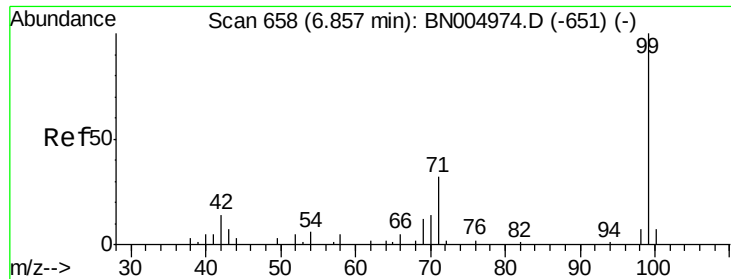

#7

Phenol-d6

Concen: 130.322 ng

RT: 6.83 min Scan# 654

Delta R.T. -0.02 min

Lab File: BN005130.D

Acq: 10 Apr 2019 16:30

Instrument :

BNA_N

ClientSampleId :

TP-7-D


Tot Ion: 99 Resp: 76843

Ion Ratio Lower Upper

99 100

42 13.1 11.4 17.0




71 31.4 25.8 38.8

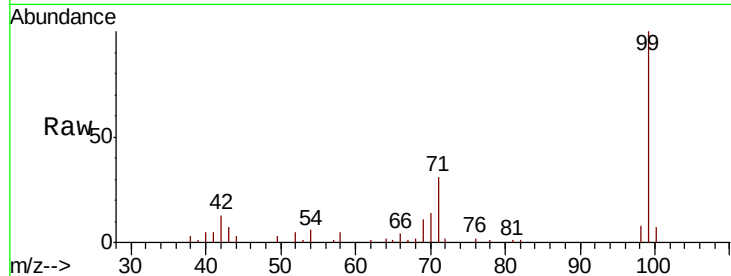

Abundance Ion 99.00 (98.70 to 99.70): BN004974.D (-651) (-)

Ion 42.00 (41.70 to 42.70): BN004974.D (-651) (-)

Ion 71.00 (70.70 to 71.70): BN004974.D (-651) (-)

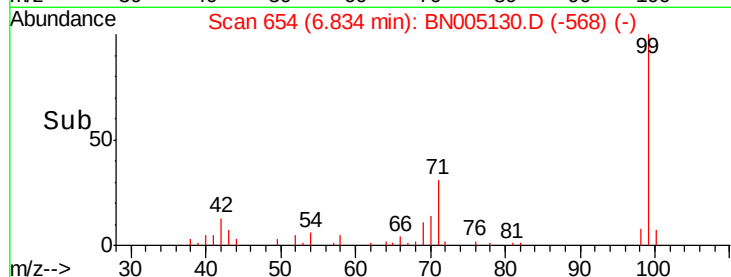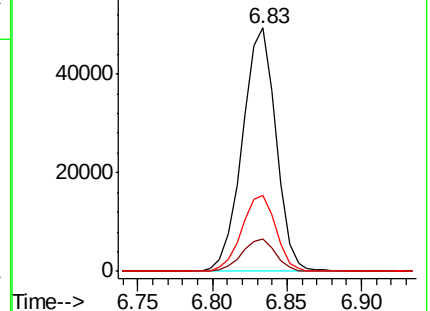

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.43 min Scan# 1266

Delta R.T. -0.03 min

Lab File: BN005130.D

Acq: 10 Apr 2019 16:30

Tgt Ion:136 Resp: 31312


Ion Ratio Lower Upper

136 100

137 11.0 8.9 13.3

54 6.4 5.3 7.9

68 5.3 4.6 6.8






Abundance Ion 136.00 (135.70 to 136.70): BN004974.D (-1264) (-)

Ion 137.00 (136.70 to 137.70): BN004974.D (-1264) (-)

Ion 54.00 (53.70 to 54.70): BN004974.D (-1264) (-)

Ion 68.00 (67.70 to 68.70): BN004974.D (-1264) (-)

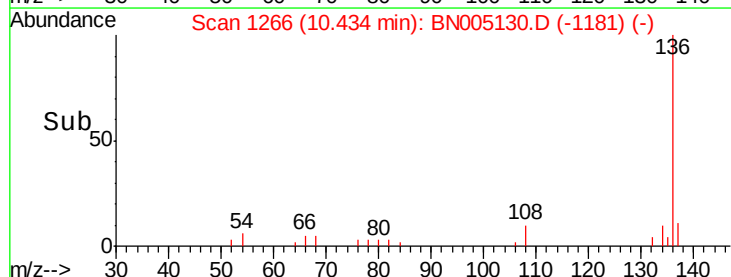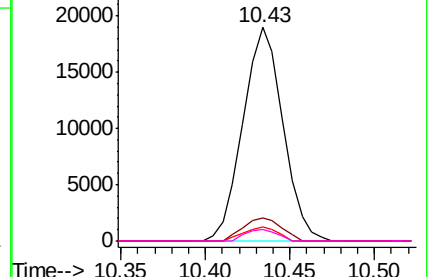


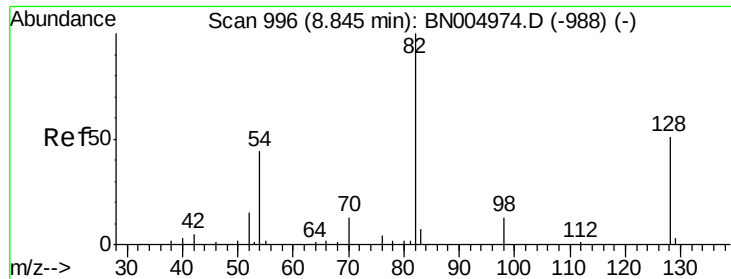




#23
Nitrobenzene-d5
Concen: 82.384 ng
RT: 8.82 min Scan# 991
Delta R.T. -0.03 min
Lab File: BN005130.D
Acq: 10 Apr 2019 16:30

Instrument :
BNA_N
ClientSampleId :
TP-7-D

Tot Ion: 82 Resp: 42644
Ion Ratio Lower Upper
82 100
128 51.0 40.6 60.8
54 42.9 35.2 52.8

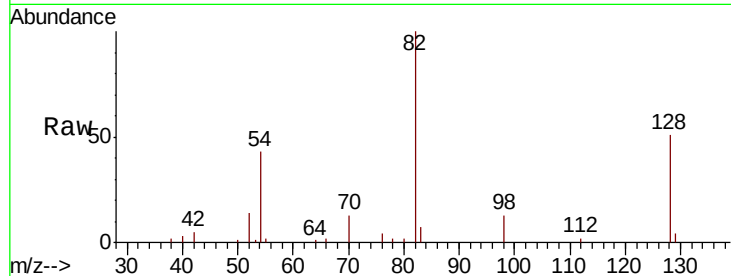


Abundance Ion 82.00 (81.70 to 82.70): BN0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BN0

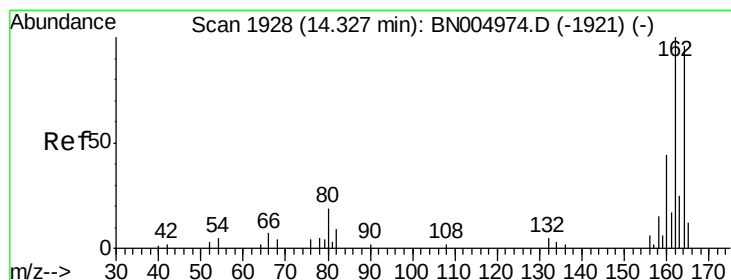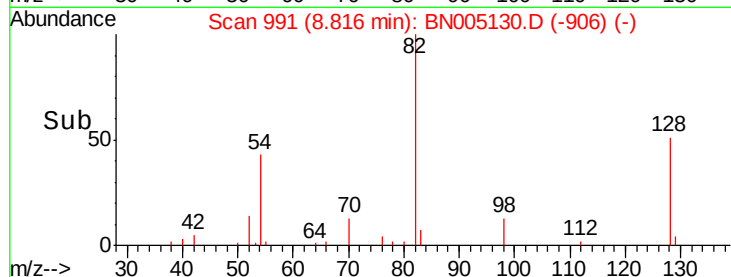
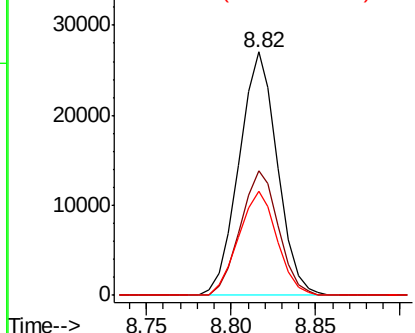



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.30 min Scan# 1923
Delta R.T. -0.03 min
Lab File: BN005130.D
Acq: 10 Apr 2019 16:30

Tgt Ion:164 Resp: 17954
Ion Ratio Lower Upper
164 100
162 103.5 83.4 125.0
160 45.7 36.6 55.0



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

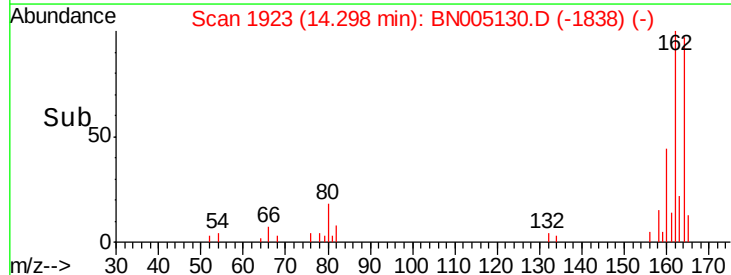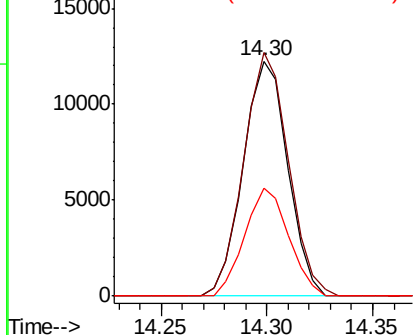


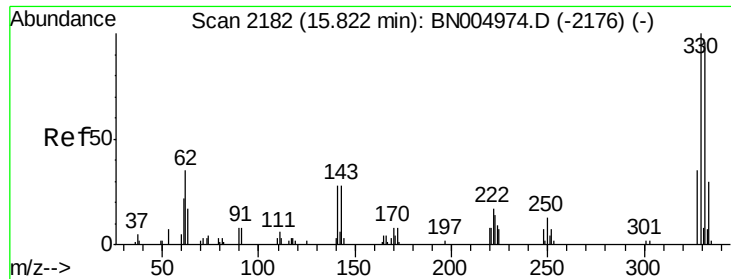




#42
 2,4,6-Tribromophenol
 Concen: 134.782 ng
 RT: 15.80 min Scan# 2178
 Delta R.T. -0.02 min
 Lab File: BN005130.D
 Acq: 10 Apr 2019 16:30

Instrument :
 BNA_N
 ClientSampleId :
 TP-7-D

Tot Ion:330 Resp: 39028
 Ion Ratio Lower Upper
 330 100
 332 96.5 77.4 116.0
 141 23.6 22.1 33.1

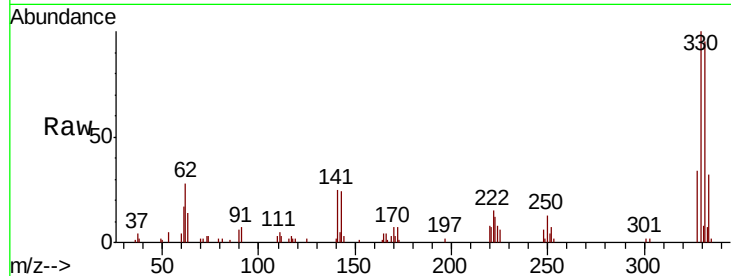


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

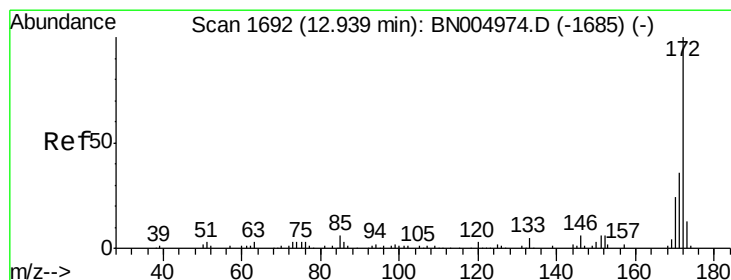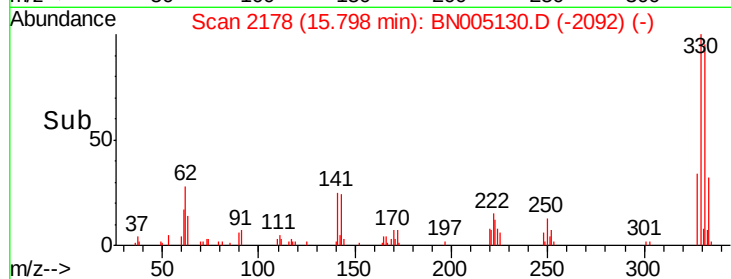
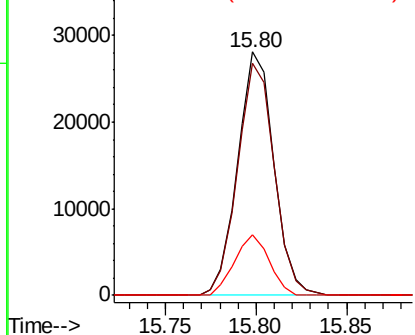



#45
 2-Fluorobiphenyl
 Concen: 86.245 ng
 RT: 12.92 min Scan# 1688
 Delta R.T. -0.02 min
 Lab File: BN005130.D
 Acq: 10 Apr 2019 16:30

Tgt Ion:172 Resp: 116852
 Ion Ratio Lower Upper
 172 100
 171 36.3 28.6 42.8
 170 23.3 18.9 28.3



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

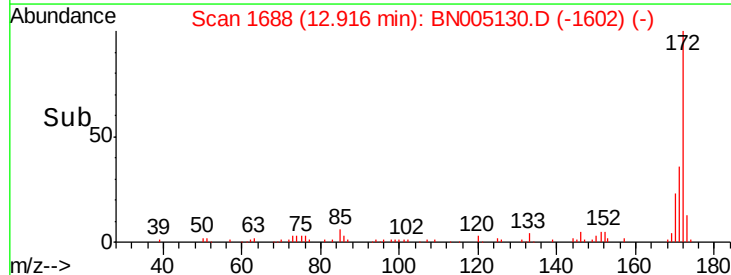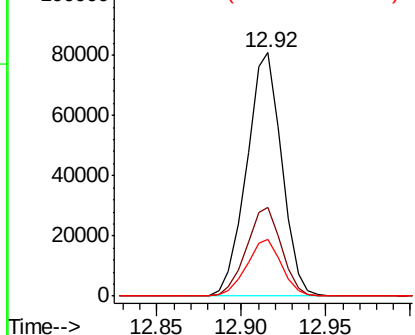

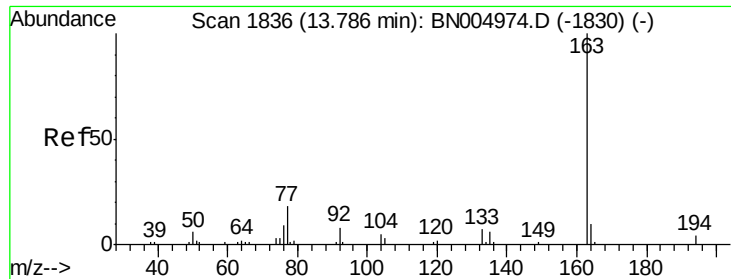

#50

Dimethylphthalate

Concen: 6.868 ng

RT: 13.76 min Scan# 1831

Delta R.T. -0.03 min

Lab File: BN005130.D

Acq: 10 Apr 2019 16:30

Instrument :

BNA_N

ClientSampleId :

TP-7-D


Tot Ion:163 Resp: 10131

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0




164 10.2 8.3 12.5

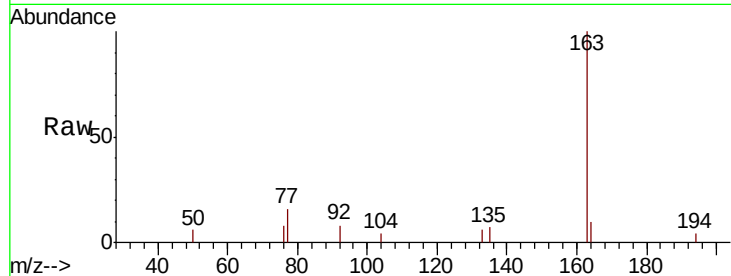

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

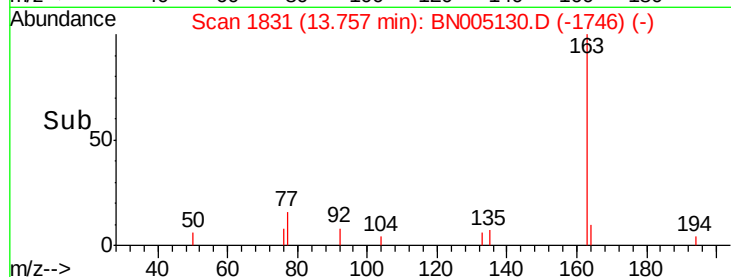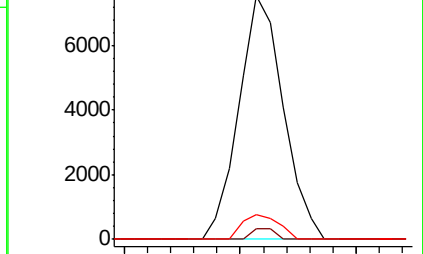

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.05 min Scan# 2391

Delta R.T. -0.02 min

Lab File: BN005130.D

Acq: 10 Apr 2019 16:30


Tgt Ion:188 Resp: 37724

Ion Ratio Lower Upper

188 100

94 8.2 7.2 10.8



80 9.0 7.8 11.6




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

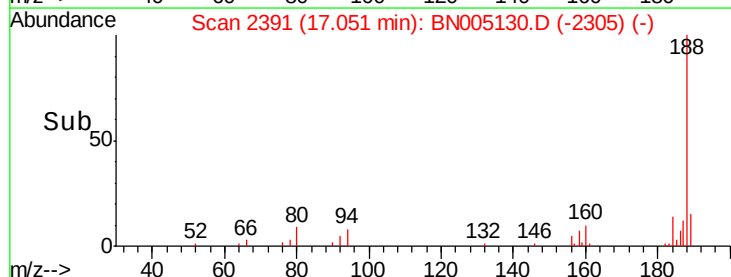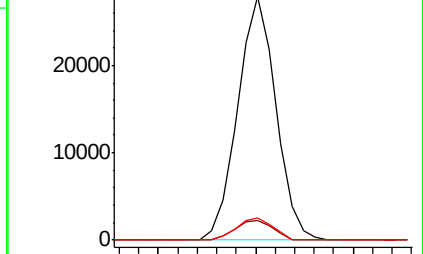

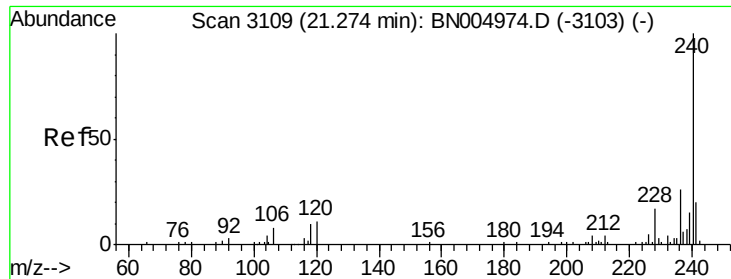

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.25 min Scan# 3105

Delta R.T. -0.02 min

Lab File: BN005130.D

Acq: 10 Apr 2019 16:30

Instrument :

BNA_N

ClientSampleId :

TP-7-D


Tot Ion:240 Resp: 32552

Ion Ratio Lower Upper

240 100

120 10.1 8.5 12.7




236 25.2 21.2 31.8

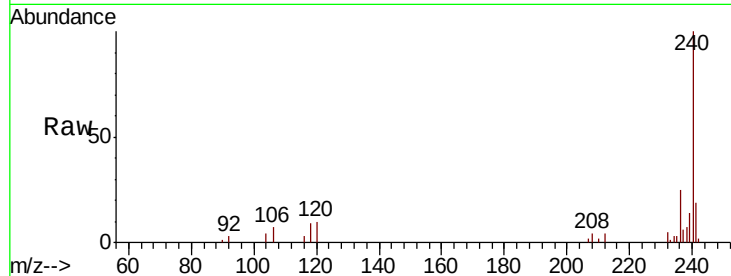

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

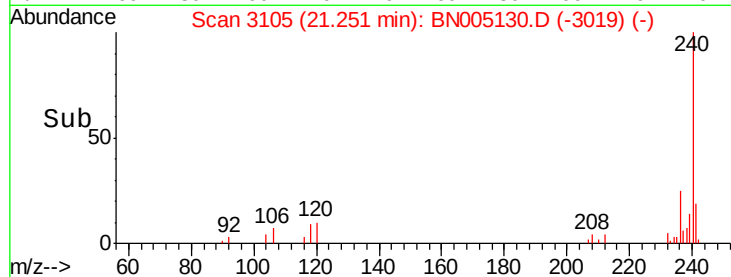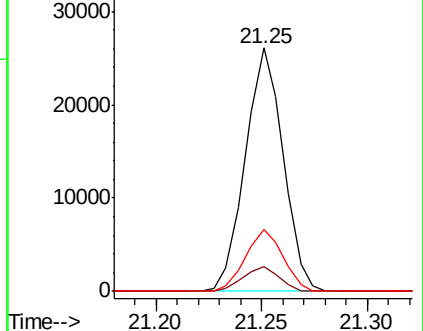

#79

Terphenyl-d14

Concen: 94.458 ng

RT: 19.69 min Scan# 2839

Delta R.T. -0.02 min

Lab File: BN005130.D

Acq: 10 Apr 2019 16:30


Tgt Ion:244 Resp: 159710

Ion Ratio Lower Upper

244 100

212 6.4 5.4 8.0



122 9.7 7.4 11.2




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

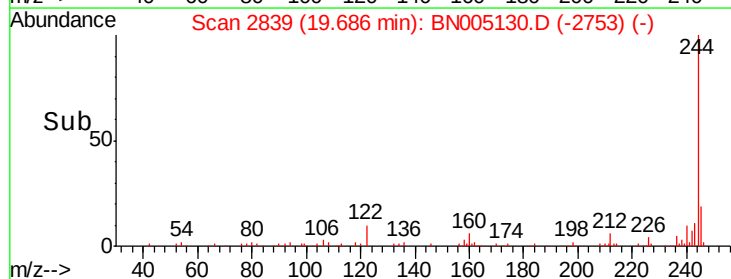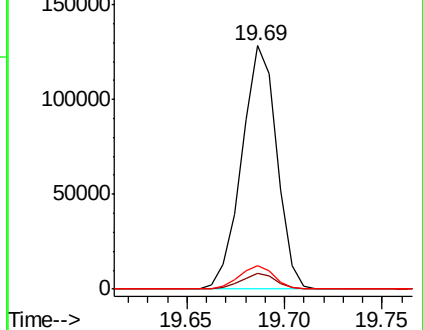


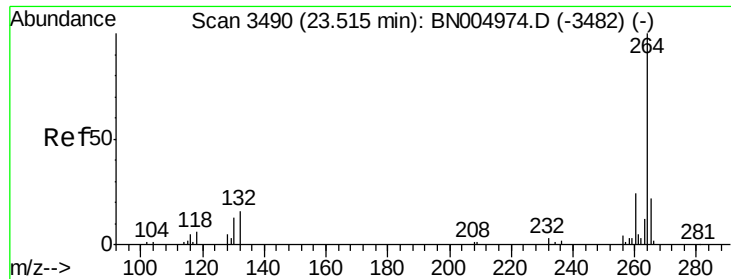

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 23.48 min Scan# 3484
 Delta R.T. -0.04 min
 Lab File: BN005130.D
 Acq: 10 Apr 2019 16:30

Instrument :
 BNA_N
 ClientSampleId :
 TP-7-D

Tot Ion:	264	Resp:	33011
Ion	Ratio	Lower	Upper
264	100		
260	23.2	19.0	28.4
265	21.7	17.2	25.8



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

