

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041019\
 Data File : BN005135.D
 Acq On : 10 Apr 2019 19:29
 Operator : JU/SJ
 Sample : K2311-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 0168-SITE-WATER

Quant Time: Apr 11 08:40:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 05:27:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	7365	20.00	ng	-0.02
21) Naphthalene-d8	10.43	136	29812	20.00	ng	-0.03
39) Acenaphthene-d10	14.30	164	16986	20.00	ng	-0.03
64) Phenanthrene-d10	17.05	188	35865	20.00	ng	-0.02
76) Chrysene-d12	21.25	240	30806	20.00	ng	-0.02
87) Perylene-d12	23.48	264	31069	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.24	112	34304	80.53	ng	-0.03
7) Phenol-d6	6.83	99	33982	60.14	ng	-0.03
23) Nitrobenzene-d5	8.82	82	42438	86.11	ng	-0.03
42) 2,4,6-Tribromophenol	15.80	330	39490	144.15	ng	-0.02
45) 2-Fluorobiphenyl	12.92	172	110680	86.34	ng	-0.02
79) Terphenyl-d14	19.69	244	172222	107.63	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041019\
Data File : BN005135.D
Acq On : 10 Apr 2019 19:29
Operator : JU/SJ
Sample : K2311-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
0168-SITE-WATER

Quant Time: Apr 11 08:40:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 05:27:09 2019
Response via : Initial Calibration

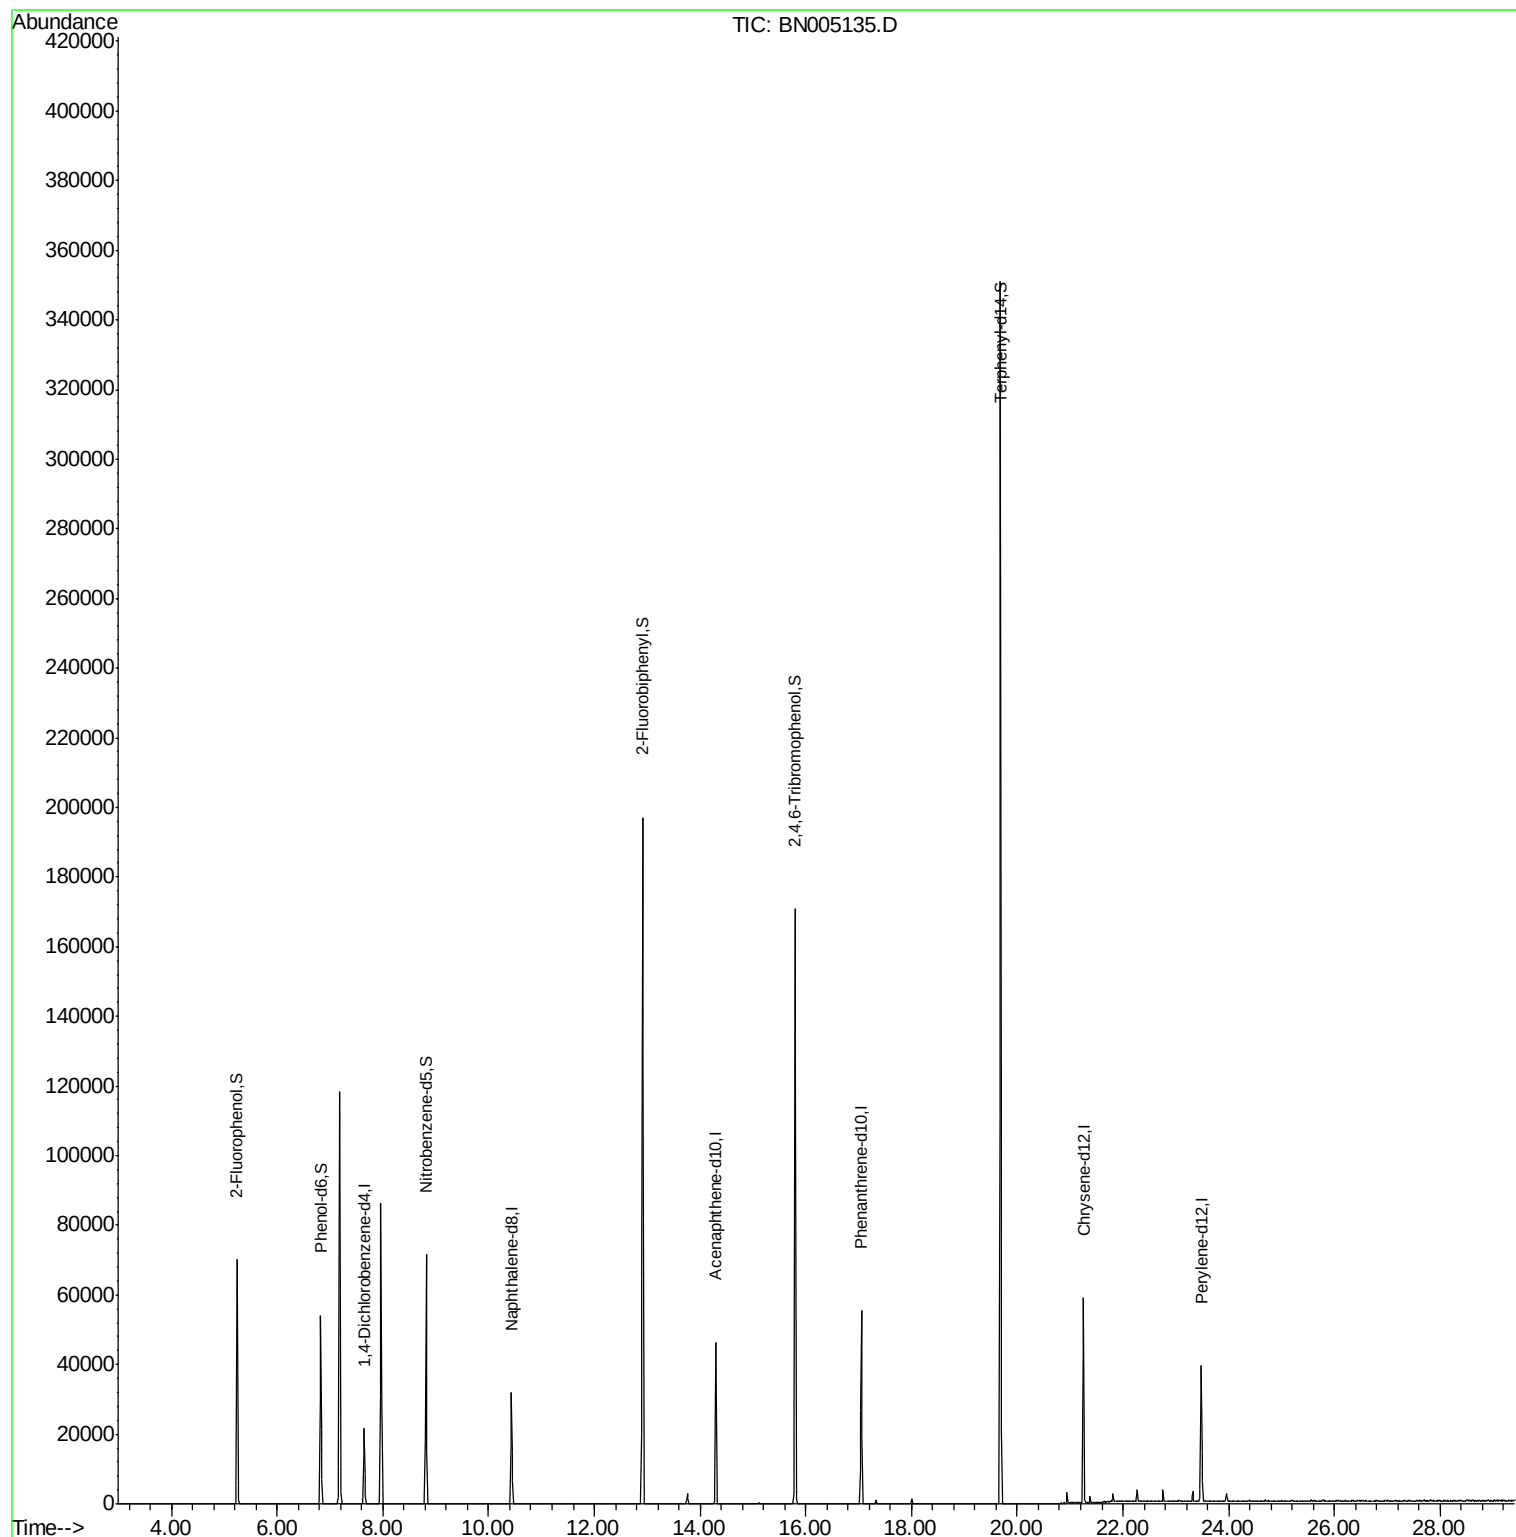




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.65 min Scan# 793
Delta R.T. -0.02 min
Lab File: BN005135.D
Acq: 10 Apr 2019 19:29

Instrument :
BNA_N
ClientSampleId :
0168-SITE-WATER

Tot Ion:152 Resp: 7365
Ion Ratio Lower Upper
152 100
150 157.8 126.9 190.3
115 58.5 47.8 71.6

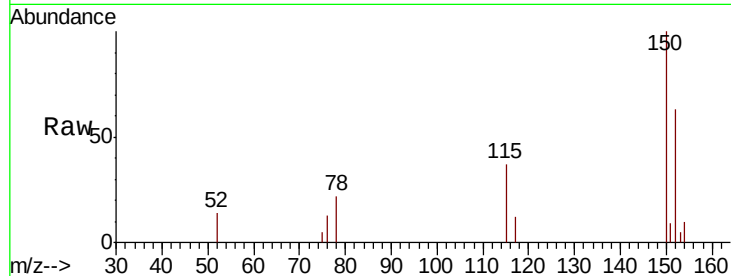


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

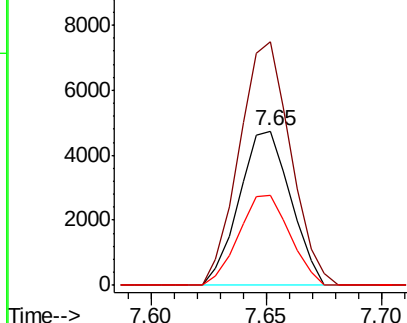



#5


2-Fluorophenol
Concen: 80.527 ng
RT: 5.24 min Scan# 383
Delta R.T. -0.03 min
Lab File: BN005135.D
Acq: 10 Apr 2019 19:29

Tgt Ion:112 Resp: 34304
Ion Ratio Lower Upper
112 100
64 51.1 41.9 62.9
63 25.6 21.4 32.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

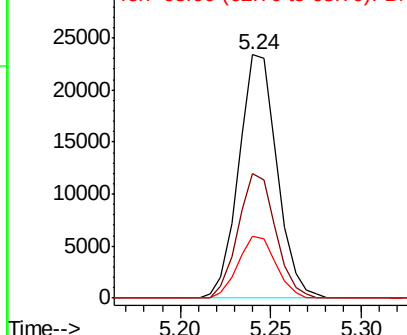

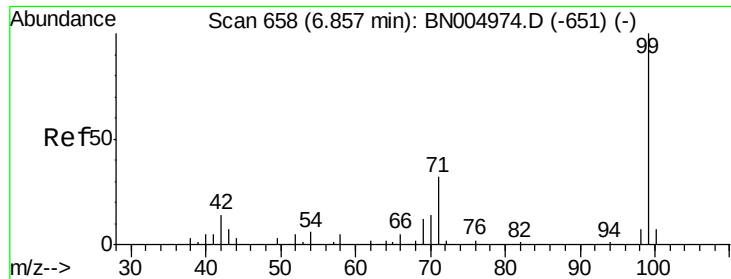

#7

Phenol-d6

Concen: 60.144 ng

RT: 6.83 min Scan# 653

Delta R.T. -0.03 min

Lab File: BN005135.D

Acq: 10 Apr 2019 19:29

Instrument :

BNA_N

ClientSampleId :

0168-SITE-WATER


Tot Ion: 99 Resp: 33982

Ion Ratio Lower Upper

99 100

42 13.2 11.4 17.0




71 32.1 25.8 38.8

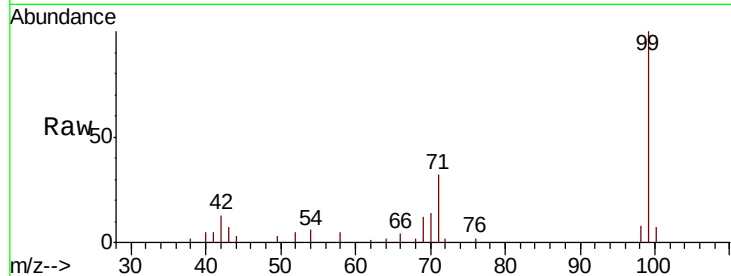

Abundance Ion 99.00 (98.70 to 99.70): BN004974.D (-651) (-)

Ion 42.00 (41.70 to 42.70): BN004974.D (-651) (-)

Ion 71.00 (70.70 to 71.70): BN004974.D (-651) (-)

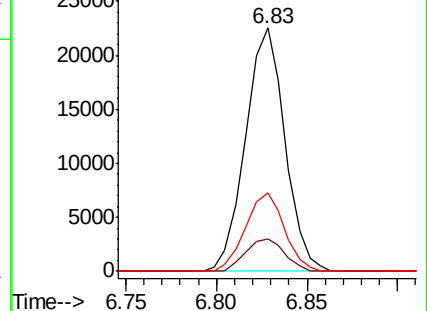

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.43 min Scan# 1266

Delta R.T. -0.03 min

Lab File: BN005135.D

Acq: 10 Apr 2019 19:29

Tgt Ion: 136 Resp: 29812


Ion Ratio Lower Upper

136 100

137 11.0 8.9 13.3

54 5.9 5.3 7.9

68 5.4 4.6 6.8






Abundance Ion 136.00 (135.70 to 136.70): BN004974.D (-1264) (-)

Ion 137.00 (136.70 to 137.70): BN004974.D (-1264) (-)

Ion 54.00 (53.70 to 54.70): BN004974.D (-1264) (-)

Ion 68.00 (67.70 to 68.70): BN004974.D (-1264) (-)

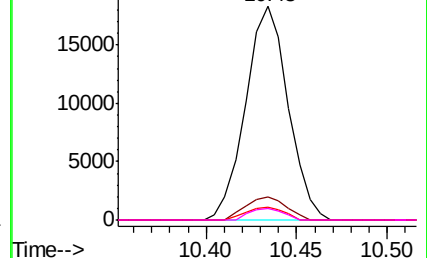

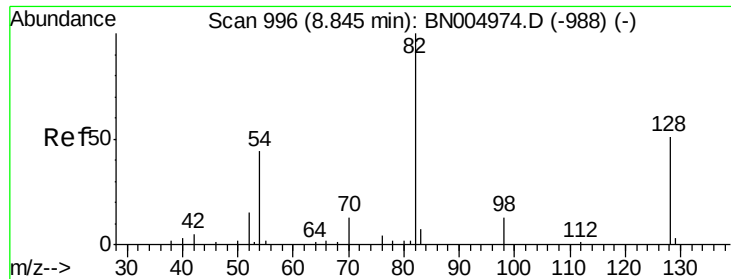

#23

Nitrobenzene-d5

Concen: 86.111 ng

RT: 8.82 min Scan# 991

Delta R.T. -0.03 min

Lab File: BN005135.D

Acq: 10 Apr 2019 19:29

Instrument :

BNA_N

ClientSampleId :

0168-SITE-WATER


Tot Ion: 82 Resp: 42438

Ion Ratio Lower Upper

82 100

128 52.6 40.6 60.8




54 43.1 35.2 52.8

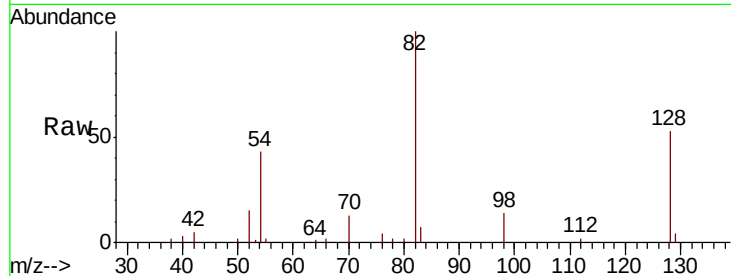

Abundance Ion 82.00 (81.70 to 82.70): BN004974.D (-988) (-)

Ion 128.00 (127.70 to 128.70): BN004974.D (-988) (-)

Ion 54.00 (53.70 to 54.70): BN004974.D (-988) (-)

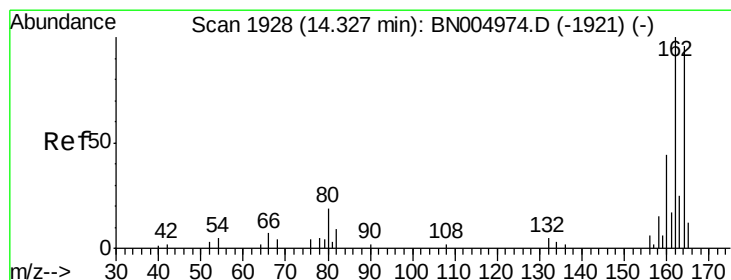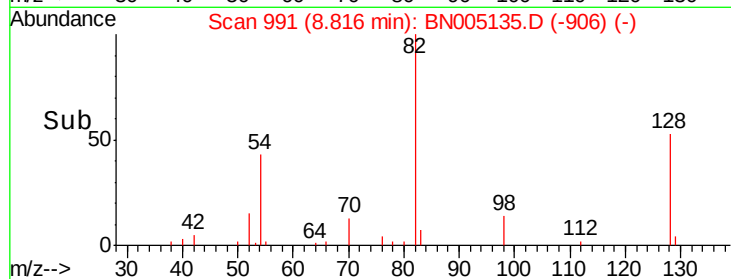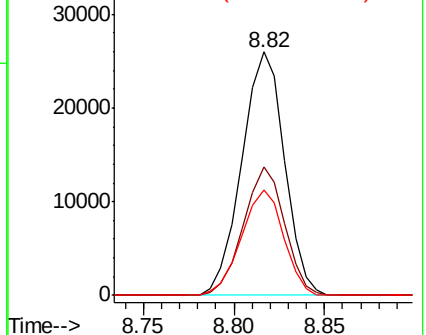

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.30 min Scan# 1923

Delta R.T. -0.03 min

Lab File: BN005135.D

Acq: 10 Apr 2019 19:29


Tgt Ion: 164 Resp: 16986

Ion Ratio Lower Upper

164 100

162 103.3 83.4 125.0



160 44.5 36.6 55.0

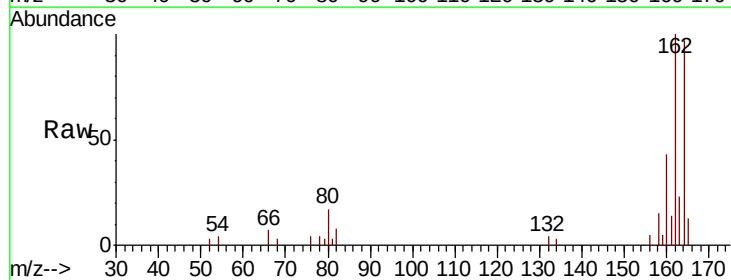


Abundance Ion 164.00 (163.70 to 164.70): BN004974.D (-1921) (-)

Ion 162.00 (161.70 to 162.70): BN004974.D (-1921) (-)

Ion 160.00 (159.70 to 160.70): BN004974.D (-1921) (-)

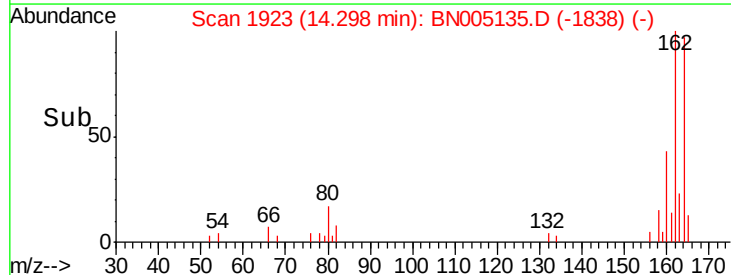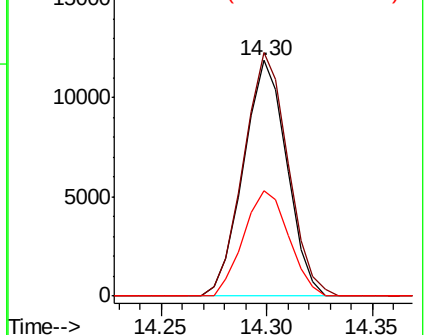



#42

2,4,6-Tribromophenol

Concen: 144.149 ng

RT: 15.80 min Scan# 2178

Delta R.T. -0.02 min

Lab File: BN005135.D

Acq: 10 Apr 2019 19:29

Instrument :

BNA_N

ClientSampleId :

0168-SITE-WATER


Tot Ion:330 Resp: 39490

Ion Ratio Lower Upper

330 100

332 97.3 77.4 116.0

141 23.5 22.1 33.1



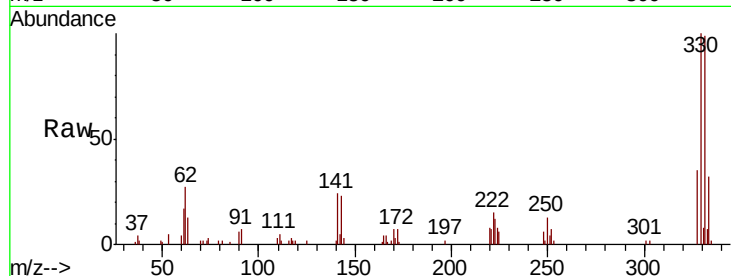


Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

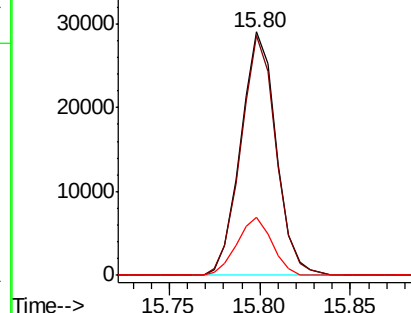

#45

2-Fluorobiphenyl

Concen: 86.345 ng

RT: 12.92 min Scan# 1688

Delta R.T. -0.02 min

Lab File: BN005135.D

Acq: 10 Apr 2019 19:29


Tgt Ion:172 Resp: 110680

Ion Ratio Lower Upper

172 100

171 35.9 28.6 42.8

170 23.0 18.9 28.3






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

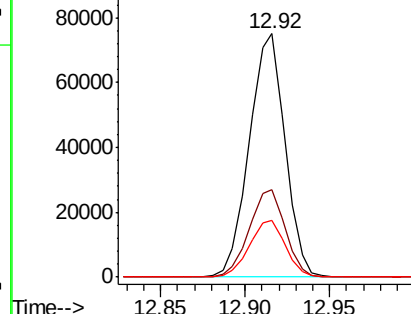



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.05 min Scan# 2391

Delta R.T. -0.02 min

Lab File: BN005135.D

Acq: 10 Apr 2019 19:29

Instrument :

BNA_N

ClientSampleId :

0168-SITE-WATER


Tot Ion:188 Resp: 35865

Ion Ratio Lower Upper

188 100

94 8.2 7.2 10.8




80 9.1 7.8 11.6

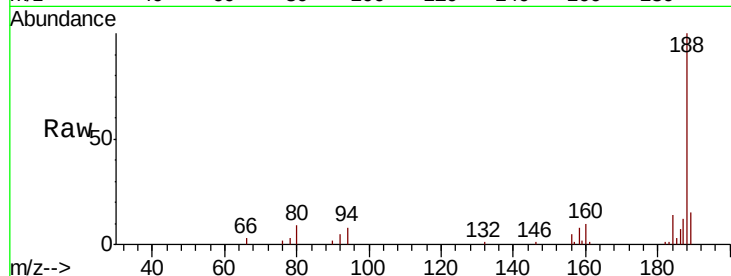

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

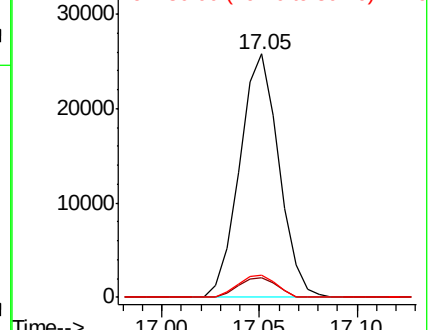

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.25 min Scan# 3105

Delta R.T. -0.02 min

Lab File: BN005135.D

Acq: 10 Apr 2019 19:29


Tgt Ion:240 Resp: 30806

Ion Ratio Lower Upper

240 100

120 9.7 8.5 12.7



236 25.3 21.2 31.8




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

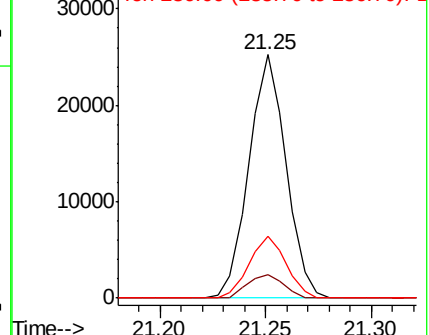

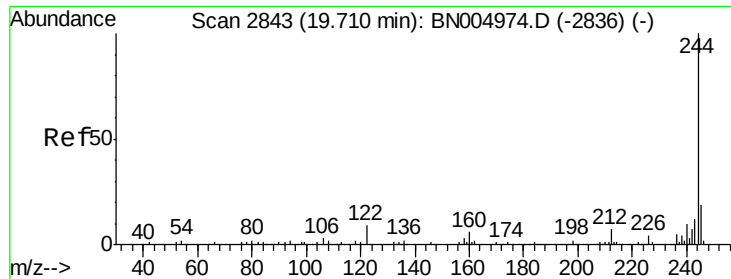

#79

Terphenyl-d14

Concen: 107.631 ng

RT: 19.69 min Scan# 2839

Delta R.T. -0.02 min

Lab File: BN005135.D

Acq: 10 Apr 2019 19:29

Instrument :

BNA_N

ClientSampleId :

0168-SITE-WATER


Tot Ion:244 Resp: 172222

Ion Ratio Lower Upper

244 100

212 6.3 5.4 8.0




122 9.8 7.4 11.2

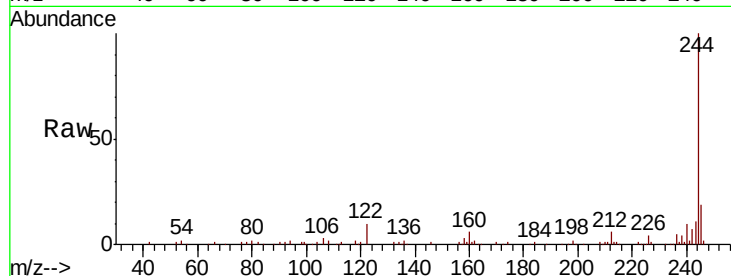

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

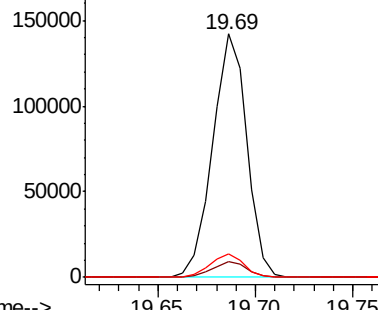

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.48 min Scan# 3484

Delta R.T. -0.04 min

Lab File: BN005135.D

Acq: 10 Apr 2019 19:29


Tgt Ion:264 Resp: 31069

Ion Ratio Lower Upper

264 100

260 23.1 19.0 28.4

265 21.7 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

