

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041019\
 Data File : BN005139.D
 Acq On : 10 Apr 2019 21:52
 Operator : JU/SJ
 Sample : K2200-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EO-01-040919-C

Quant Time: Apr 11 08:49:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 05:27:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	8246	20.00	ng	-0.02
21) Naphthalene-d8	10.43	136	31619	20.00	ng	-0.03
39) Acenaphthene-d10	14.30	164	17422	20.00	ng	-0.03
64) Phenanthrene-d10	17.05	188	35864	20.00	ng	-0.02
76) Chrysene-d12	21.25	240	30227	20.00	ng	-0.02
87) Perylene-d12	23.48	264	32798	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	64613	135.47	ng	-0.02
7) Phenol-d6	6.83	99	69643	110.09	ng	-0.02
23) Nitrobenzene-d5	8.82	82	55229	105.66	ng	-0.03
42) 2,4,6-Tribromophenol	15.80	330	49196	175.08	ng	-0.02
45) 2-Fluorobiphenyl	12.92	172	150388	114.39	ng	-0.02
79) Terphenyl-d14	19.69	244	205187	130.69	ng	-0.02


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041019\
Data File : BN005139.D
Acq On : 10 Apr 2019 21:52
Operator : JU/SJ
Sample : K2200-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EO-01-040919-C

Quant Time: Apr 11 08:49:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 05:27:09 2019
Response via : Initial Calibration

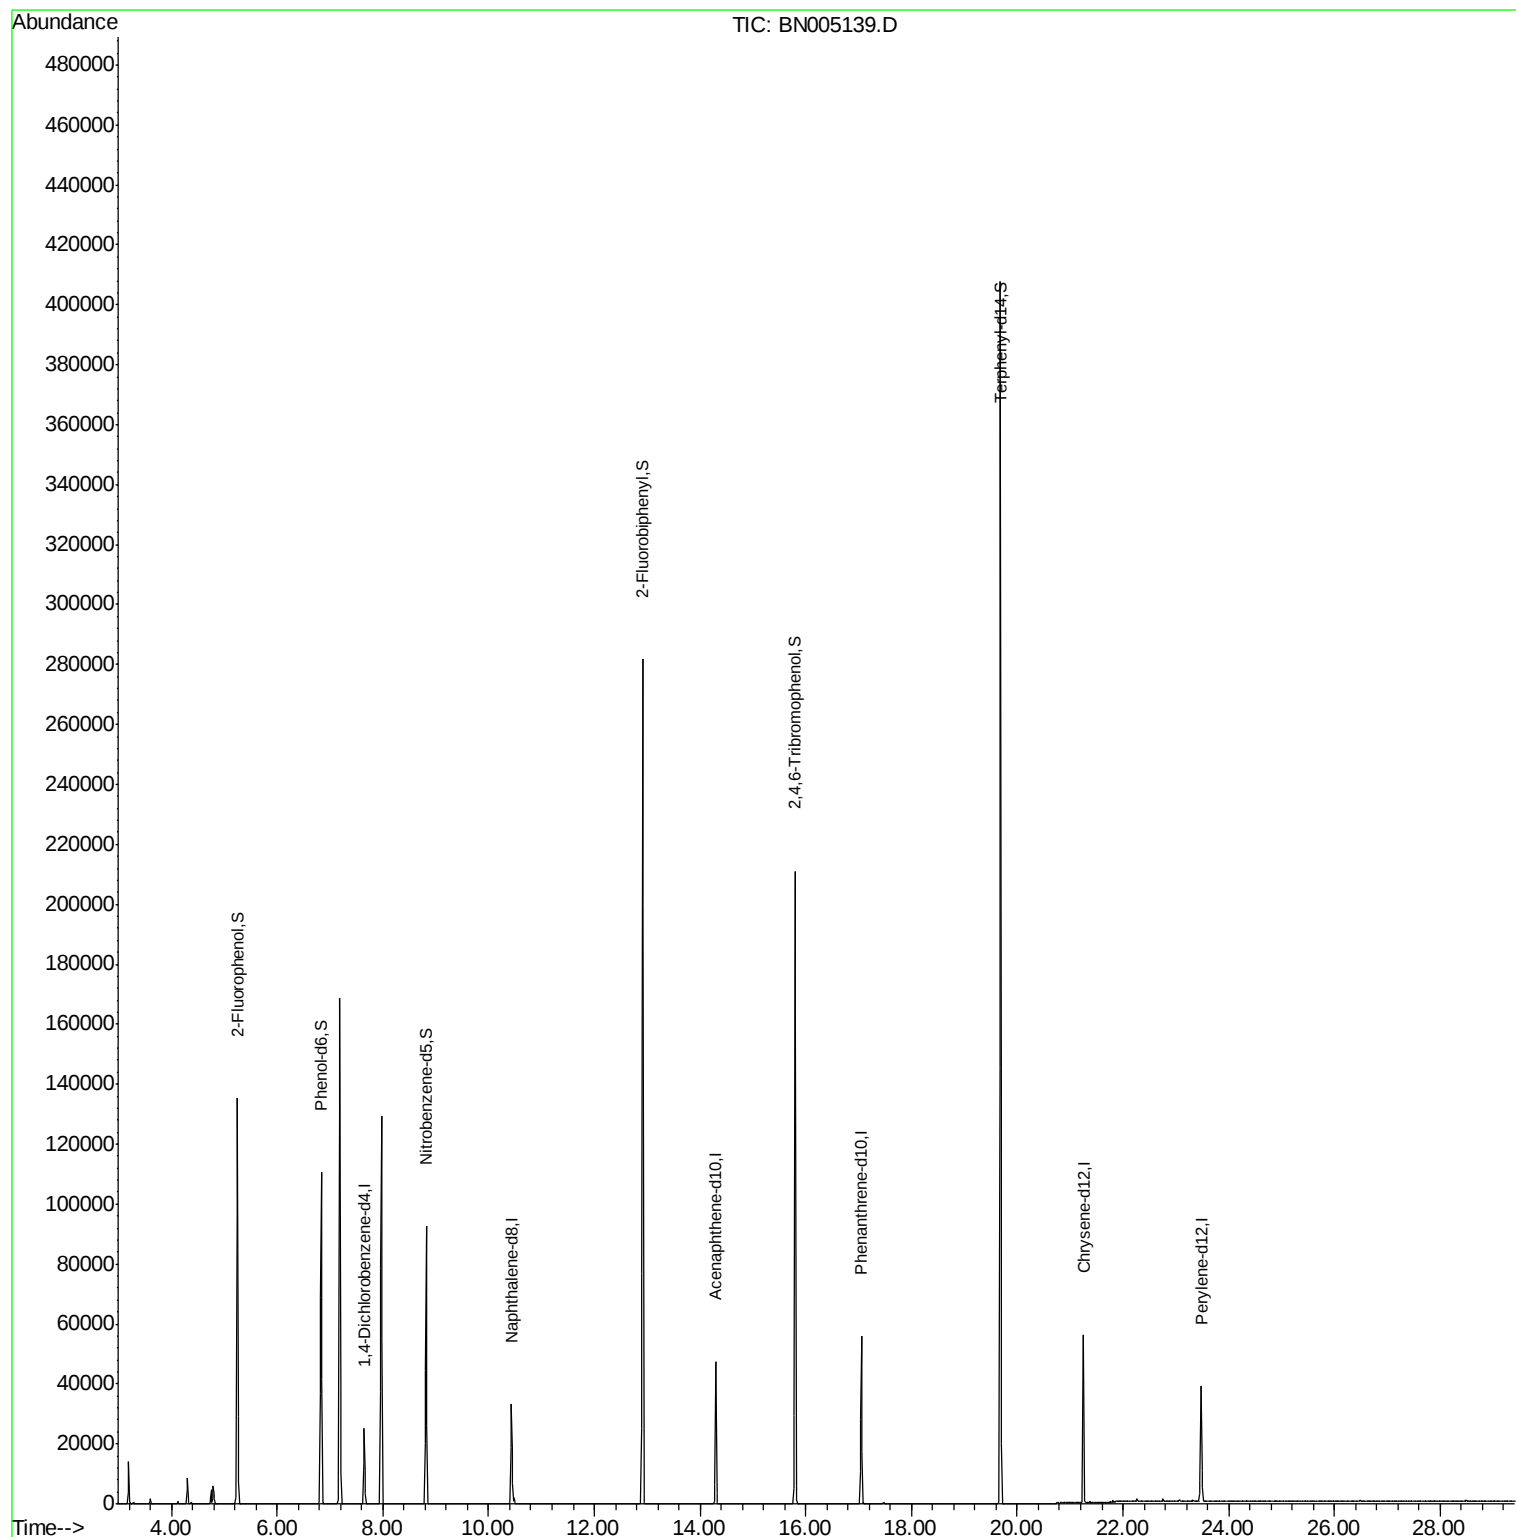




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.65 min Scan# 793
Delta R.T. -0.02 min
Lab File: BN005139.D
Acq: 10 Apr 2019 21:52

Instrument :
BNA_N
ClientSampleId :
EO-01-040919-C

Tot Ion:152 Resp: 8246
Ion Ratio Lower Upper
152 100
150 155.2 126.9 190.3
115 59.0 47.8 71.6

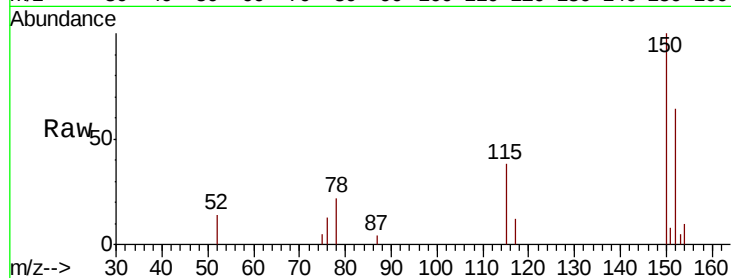


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

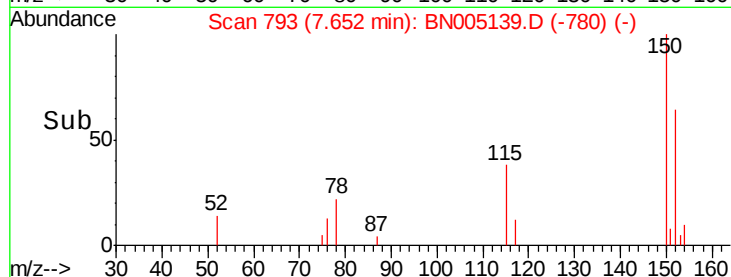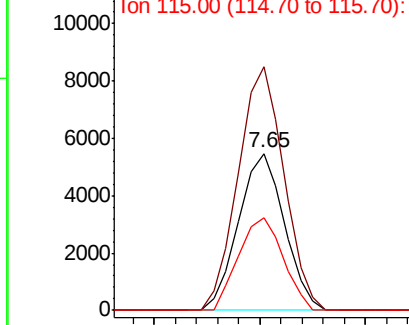



#5


2-Fluorophenol
Concen: 135.471 ng
RT: 5.25 min Scan# 384
Delta R.T. -0.02 min
Lab File: BN005139.D
Acq: 10 Apr 2019 21:52

Tgt Ion:112 Resp: 64613
Ion Ratio Lower Upper
112 100
64 50.8 41.9 62.9
63 25.5 21.4 32.0

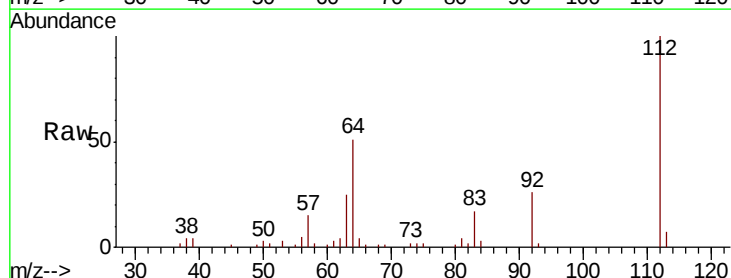

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

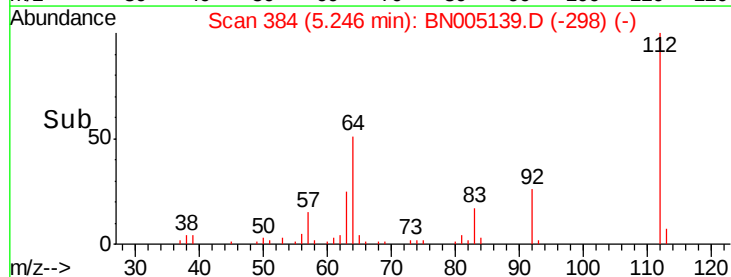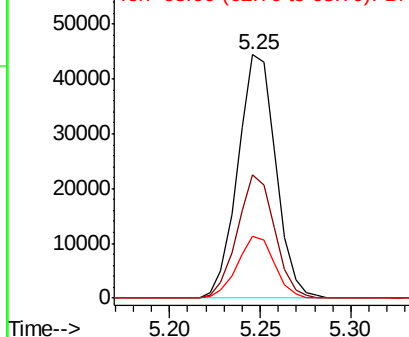

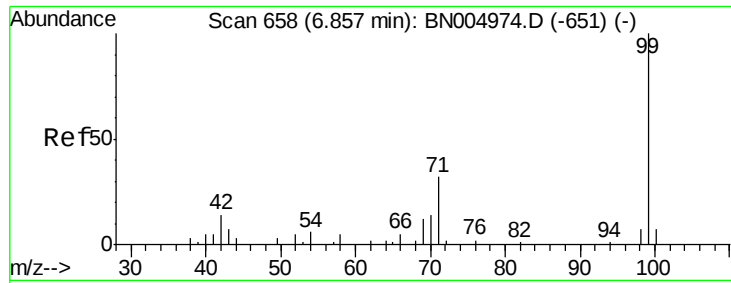

#7

Phenol-d6

Concen: 110.090 ng

RT: 6.83 min Scan# 654

Delta R.T. -0.02 min

Lab File: BN005139.D

Acq: 10 Apr 2019 21:52

Instrument :

BNA_N

ClientSampleId :

EO-01-040919-C


Tot Ion: 99 Resp: 69643

Ion Ratio Lower Upper




99 100

42 13.1 11.4 17.0

71 32.3 25.8 38.8

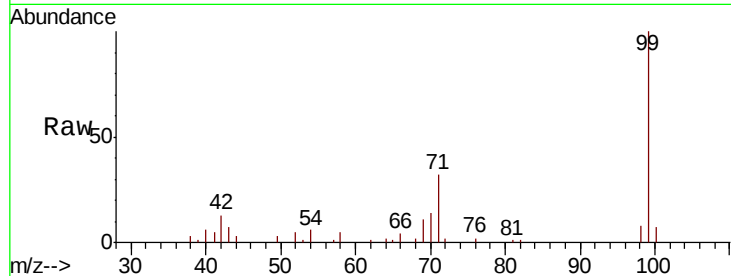

Abundance Ion 99.00 (98.70 to 99.70): BNC
Ion 42.00 (41.70 to 42.70): BNC
Ion 71.00 (70.70 to 71.70): BNC

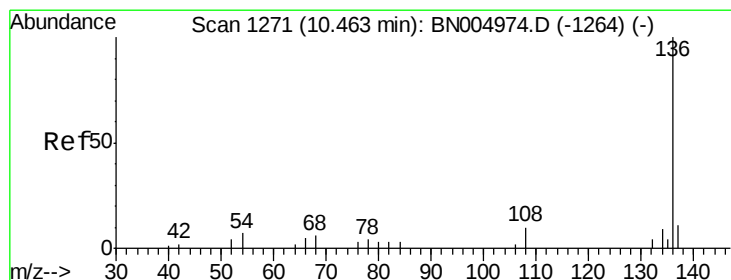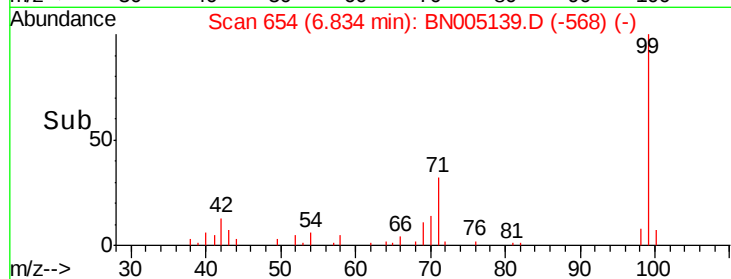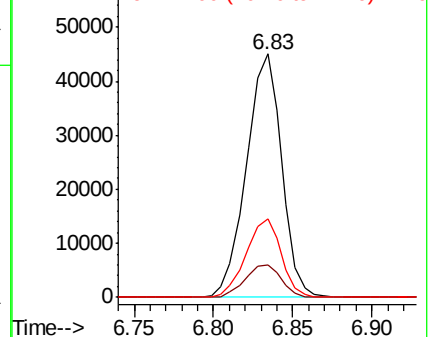

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.43 min Scan# 1266

Delta R.T. -0.03 min

Lab File: BN005139.D

Acq: 10 Apr 2019 21:52

Tgt Ion: 136 Resp: 31619


Ion Ratio Lower Upper

136 100



137 11.1 8.9 13.3

54 6.1 5.3 7.9

68 5.3 4.6 6.8

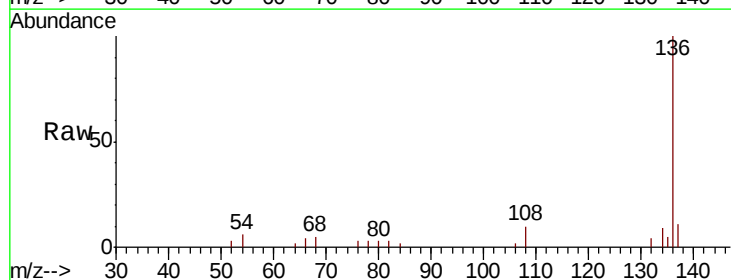

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BNC
Ion 68.00 (67.70 to 68.70): BNC

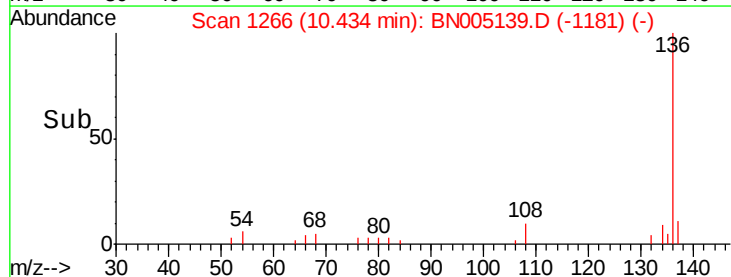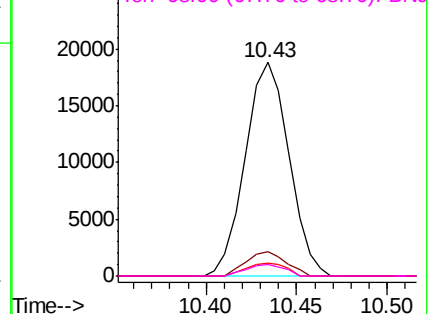







#23
 Nitrobenzene-d5
 Concen: 105.661 ng
 RT: 8.82 min Scan# 991
 Delta R.T. -0.03 min
 Lab File: BN005139.D
 Acq: 10 Apr 2019 21:52

Instrument :
 BNA_N
 ClientSampleId :
 EO-01-040919-C

Tot Ion: 82 Resp: 55229
 Ion Ratio Lower Upper
 82 100
 128 51.7 40.6 60.8
 54 43.1 35.2 52.8

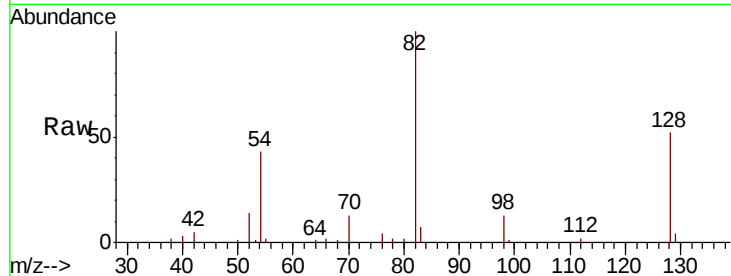


Abundance Ion 82.00 (81.70 to 82.70): BN0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BN0

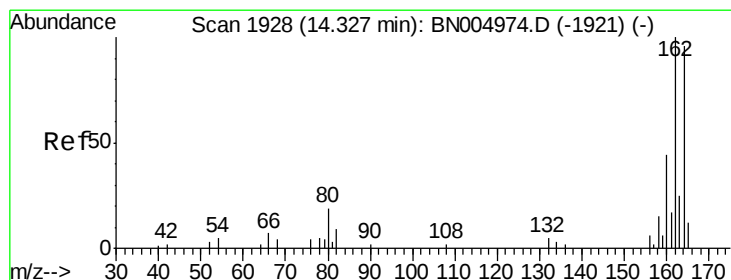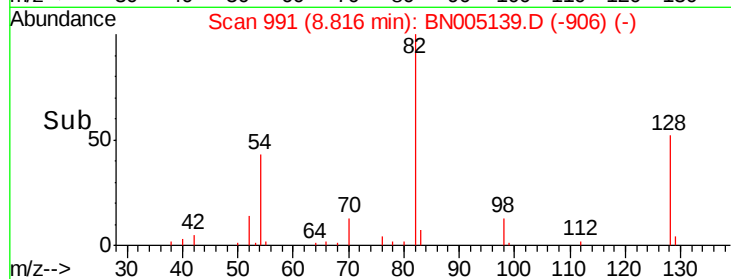
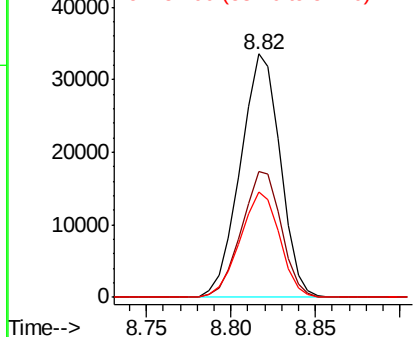



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.30 min Scan# 1923
 Delta R.T. -0.03 min
 Lab File: BN005139.D
 Acq: 10 Apr 2019 21:52

Tgt Ion:164 Resp: 17422
 Ion Ratio Lower Upper
 164 100
 162 105.5 83.4 125.0
 160 45.8 36.6 55.0

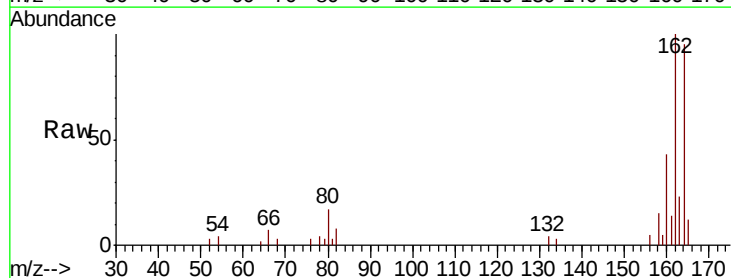

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

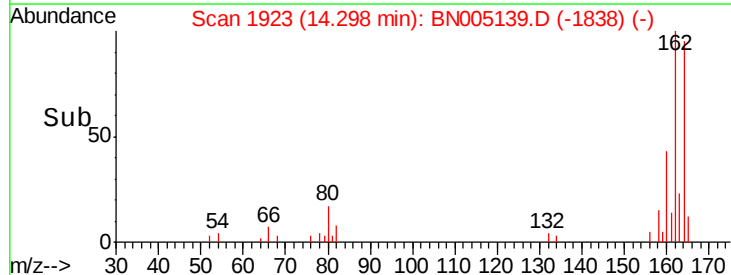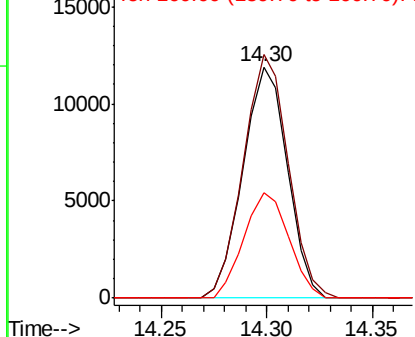


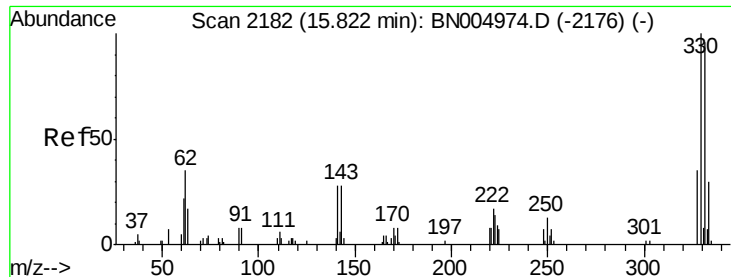

#42
 2,4,6-Tribromophenol
 Concen: 175.084 ng
 RT: 15.80 min Scan# 2178
 Delta R.T. -0.02 min
 Lab File: BN005139.D
 Acq: 10 Apr 2019 21:52

Instrument :
 BNA_N
 ClientSampleId :
 EO-01-040919-C

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.5	77.4	116.0
141	23.8	22.1	33.1



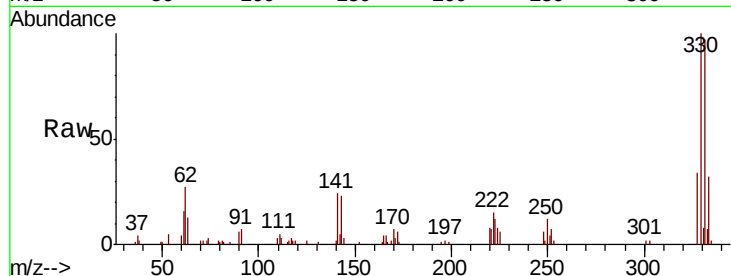


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

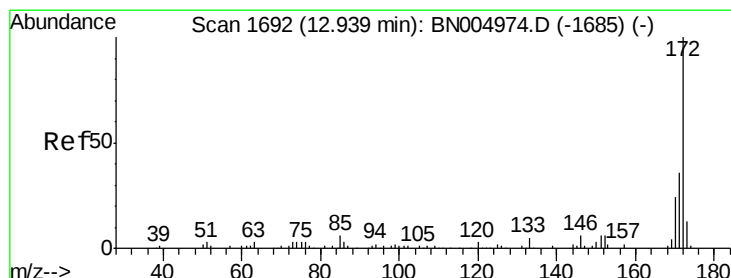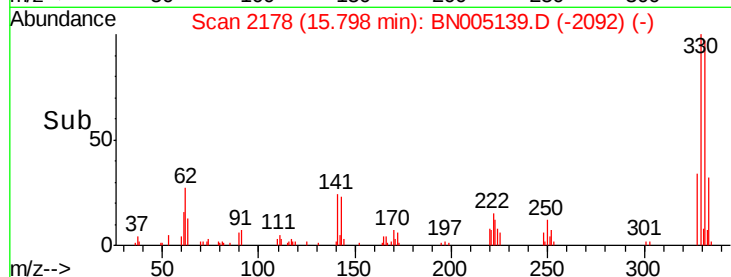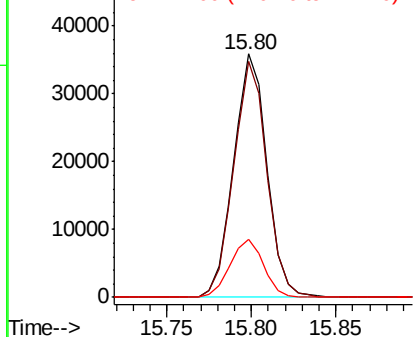

#45
 2-Fluorobiphenyl
 Concen: 114.386 ng
 RT: 12.92 min Scan# 1688
 Delta R.T. -0.02 min
 Lab File: BN005139.D
 Acq: 10 Apr 2019 21:52

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	28.6	42.8
170	23.8	18.9	28.3


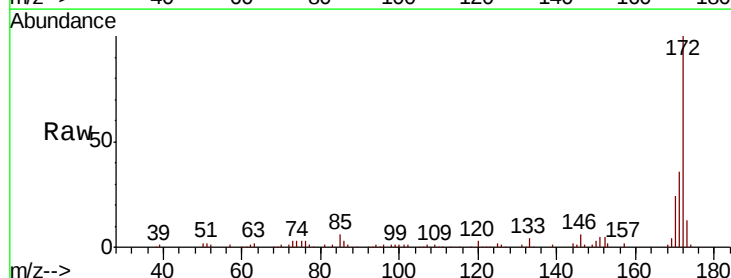



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

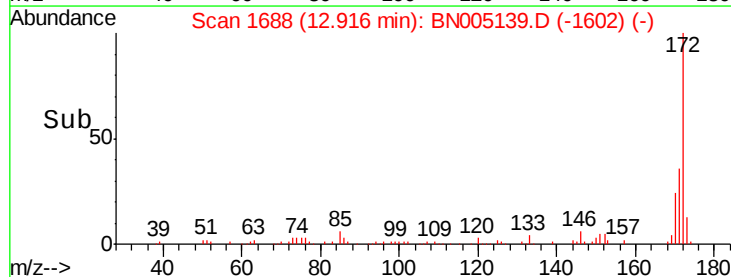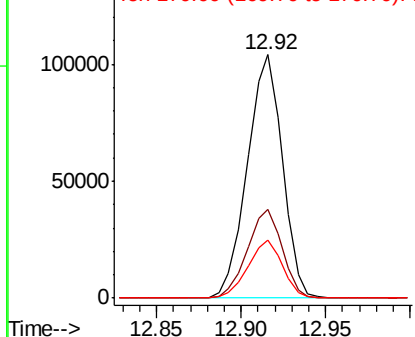

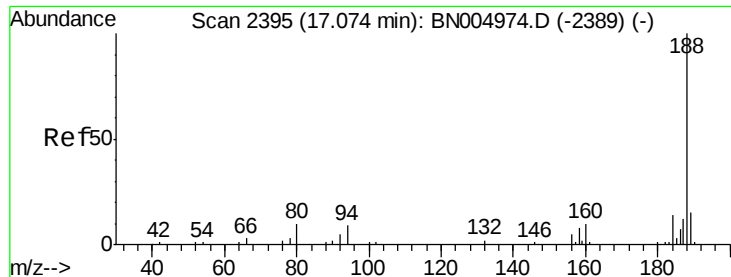

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.05 min Scan# 2391

Delta R.T. -0.02 min

Lab File: BN005139.D

Acq: 10 Apr 2019 21:52

Instrument :

BNA_N

ClientSampleId :

EO-01-040919-C


Tot Ion:188 Resp: 35864

Ion Ratio Lower Upper

188 100

94 8.2 7.2 10.8




80 8.3 7.8 11.6

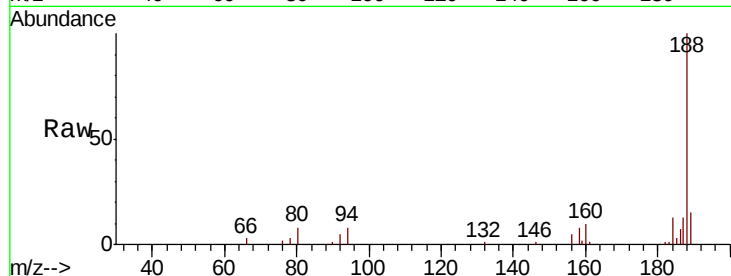

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

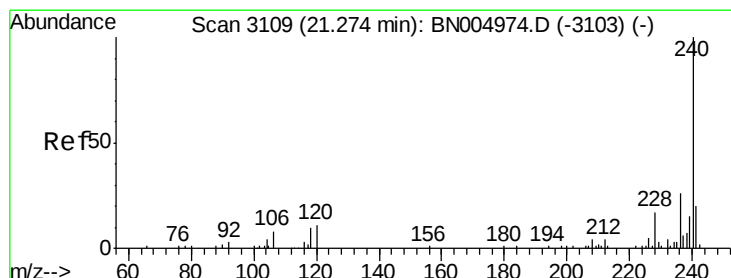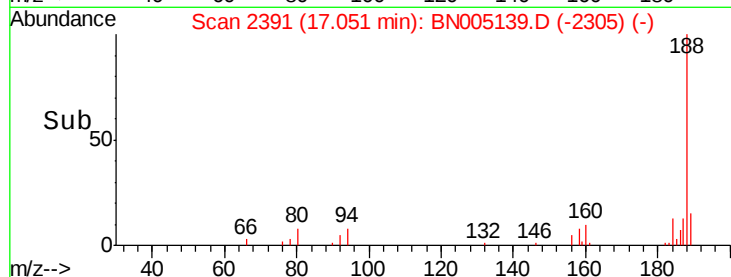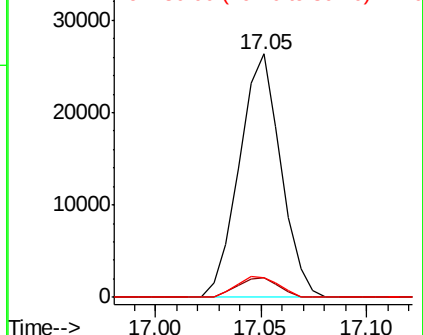

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.25 min Scan# 3105

Delta R.T. -0.02 min

Lab File: BN005139.D

Acq: 10 Apr 2019 21:52


Tgt Ion:240 Resp: 30227

Ion Ratio Lower Upper

240 100

120 9.6 8.5 12.7



236 25.9 21.2 31.8

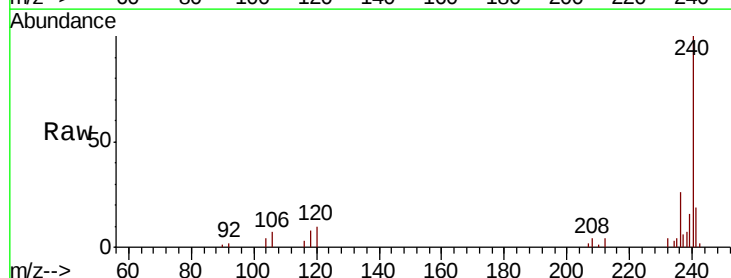


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

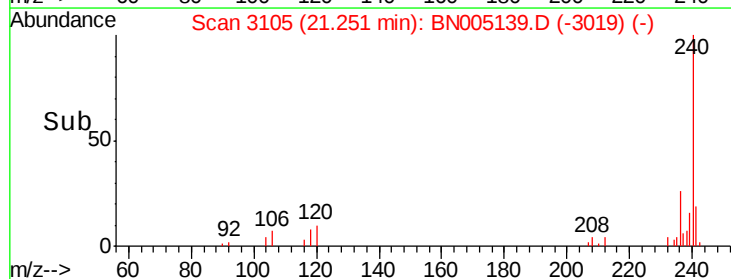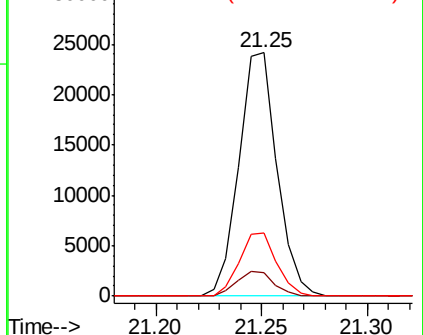

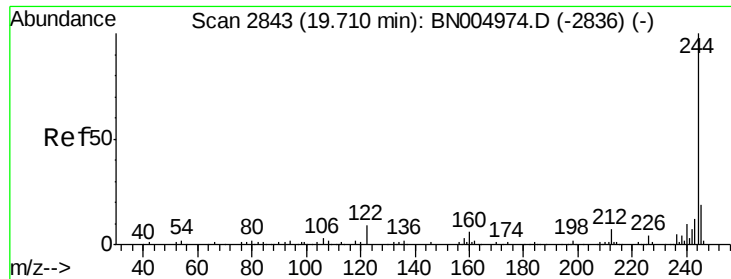

#79

Terphenyl-d14

Concen: 130.689 ng

RT: 19.69 min Scan# 2839

Delta R.T. -0.02 min

Lab File: BN005139.D

Acq: 10 Apr 2019 21:52

Instrument :

BNA_N

ClientSampleId :

EO-01-040919-C


Tot Ion:244 Resp: 205187

Ion Ratio Lower Upper

244 100

212 6.5 5.4 8.0




122 9.5 7.4 11.2

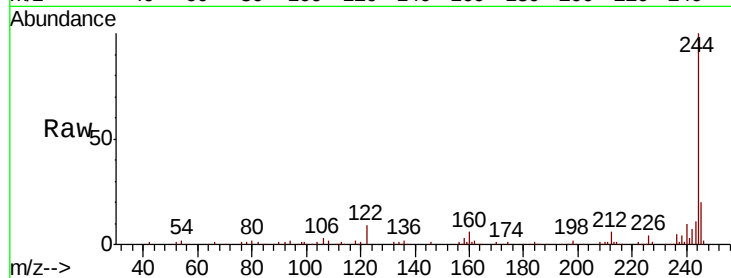

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

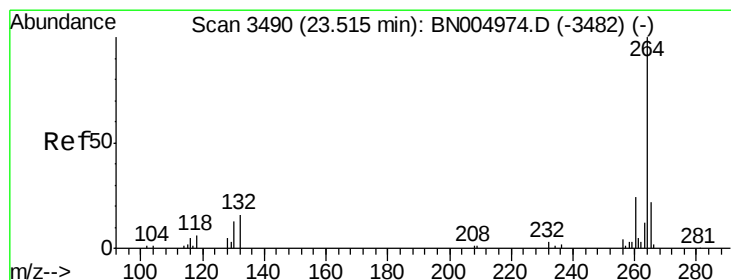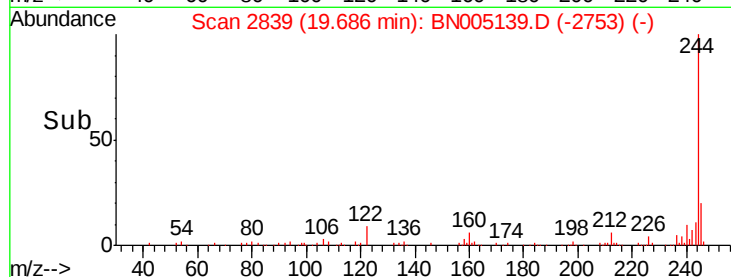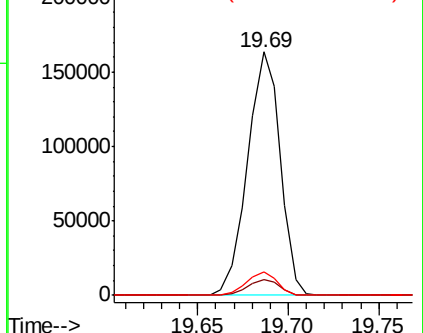

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.48 min Scan# 3484

Delta R.T. -0.04 min

Lab File: BN005139.D

Acq: 10 Apr 2019 21:52


Tgt Ion:264 Resp: 32798

Ion Ratio Lower Upper

264 100

260 23.2 19.0 28.4

265 21.1 17.2 25.8

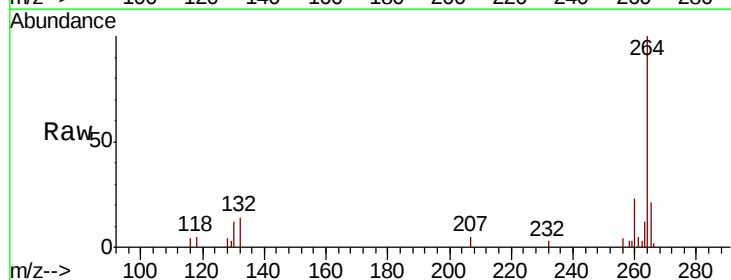

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

