

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041019\
 Data File : BN005126.D
 Acq On : 10 Apr 2019 14:07
 Operator : JU/SJ
 Sample : PB118762BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB118762BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	379	384	391	rBB	123031	167263	54.27%	9.010%
2	6.834	647	654	661	rBB	112760	172672	56.03%	9.301%
3	7.187	708	714	720	rBB	130578	194307	63.05%	10.466%
4	7.652	788	793	798	rBB	20977	29969	9.72%	1.614%
5	7.969	841	847	853	rBB	96359	148868	48.31%	8.019%
6	8.816	985	991	998	rBB	69321	104144	33.79%	5.610%
7	10.434	1260	1266	1273	rBB	28250	43972	14.27%	2.369%
8	12.916	1681	1688	1694	rBB	203241	286262	92.89%	15.419%
9	14.298	1918	1923	1929	rBB2	42187	58797	19.08%	3.167%
10	15.798	2173	2178	2185	rBB	131135	169801	55.10%	9.146%
11	17.051	2386	2391	2397	rBB	43983	58975	19.14%	3.177%
12	19.686	2834	2839	2844	rBV	267903	308179	100.00%	16.600%
13	21.251	3100	3105	3112	rBV	44914	54483	17.68%	2.935%
14	23.480	3478	3484	3492	rBV2	32166	58814	19.08%	3.168%


Sum of corrected areas: 1856506

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041019\
Data File : BN005126.D
Acq On : 10 Apr 2019 14:07
Operator : JU/SJ
Sample : PB118762BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118762BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

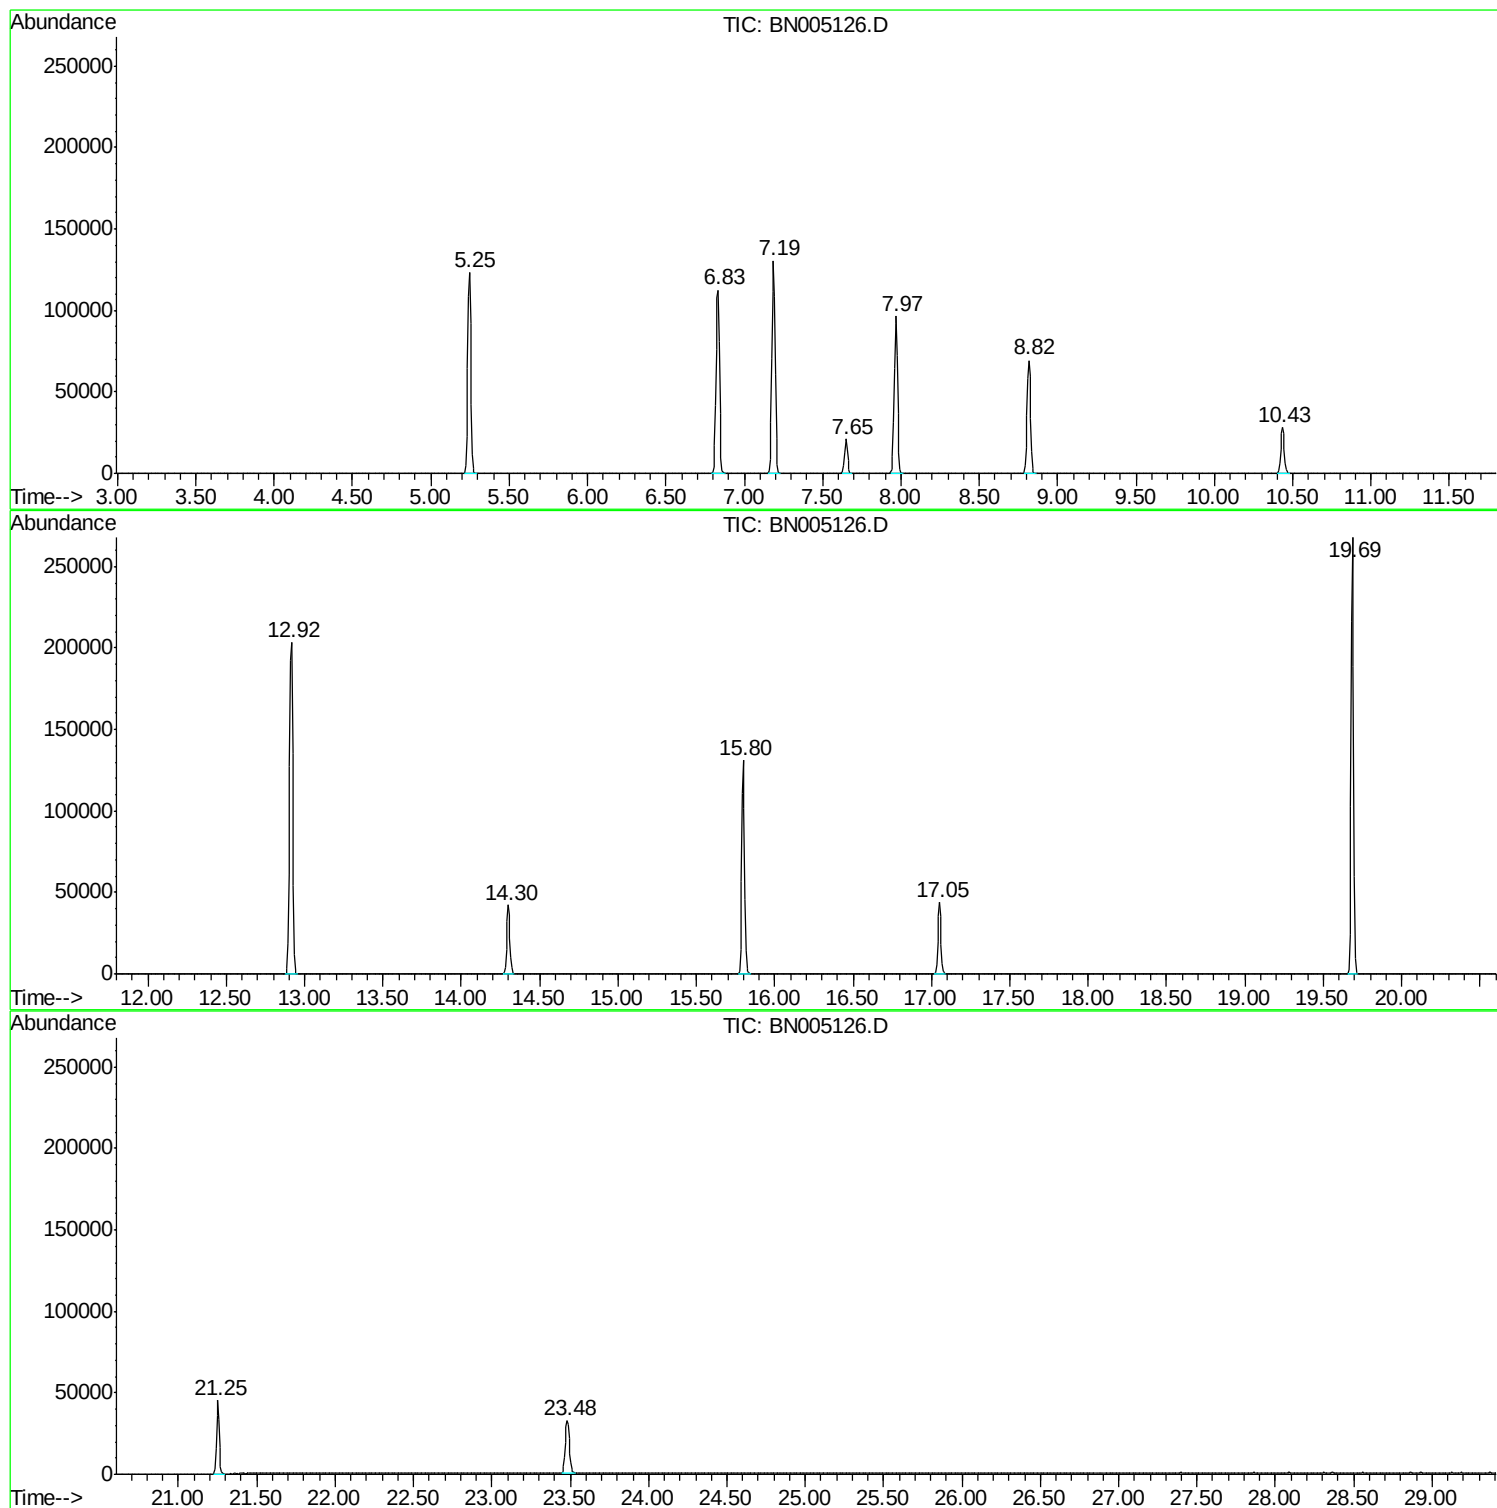

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041019\
Data File : BN005126.D
Acq On : 10 Apr 2019 14:07
Operator : JU/SJ
Sample : PB118762BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118762BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.19 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	129.67 ng	194307	1,4-Dichlorobenzene-d4	7.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

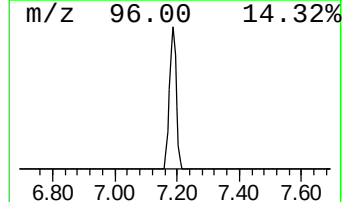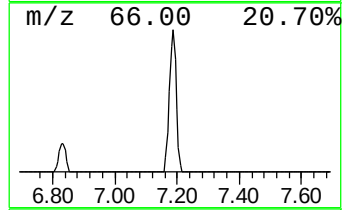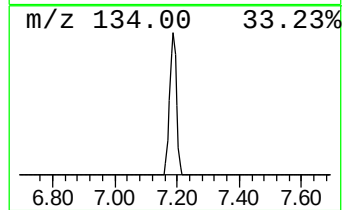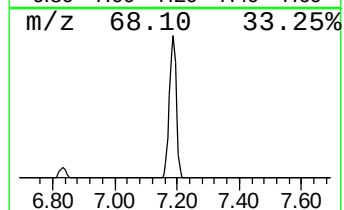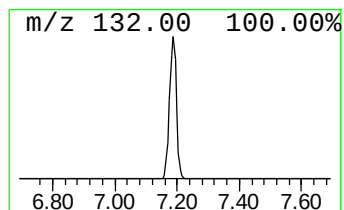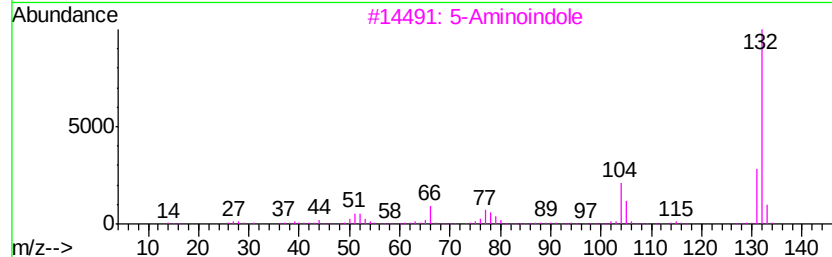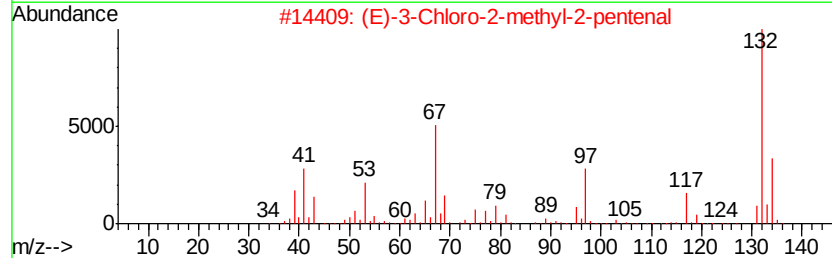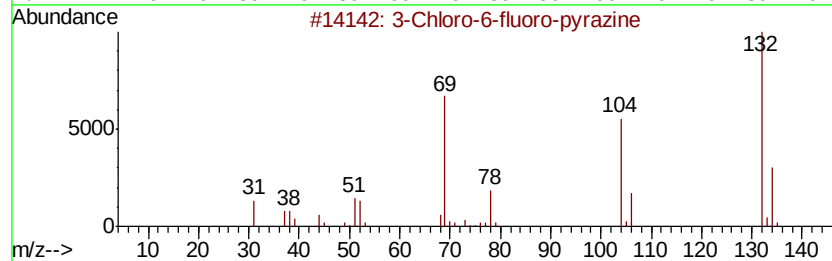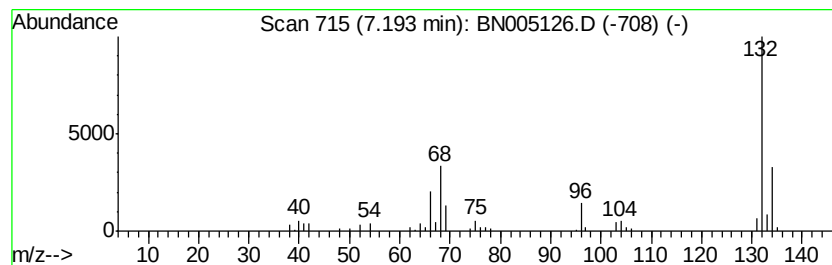

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041019\
Data File : BN005126.D
Acq On : 10 Apr 2019 14:07
Operator : JU/SJ
Sample : PB118762BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118762BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.19	7.19	129.7	ng	194307	1	7.65	29969	20.0