

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041019\
 Data File : BN005127.D
 Acq On : 10 Apr 2019 14:43
 Operator : JU/SJ
 Sample : K2343-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TP-7-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	378	384	391	rBB	120656	167704	42.60%	7.287%
2	6.834	647	654	661	rBB	116046	179870	45.69%	7.815%
3	7.187	708	714	720	rBB	134581	199518	50.68%	8.669%
4	7.652	788	793	798	rBB	26859	38440	9.76%	1.670%
5	7.969	841	847	852	rBB	96140	149234	37.90%	6.484%
6	8.816	985	991	997	rBB	70234	109805	27.89%	4.771%
7	10.434	1260	1266	1272	rBB	37464	57846	14.69%	2.513%
8	12.916	1681	1688	1694	rBB	217219	299982	76.19%	13.034%
9	13.757	1827	1831	1836	rBB	10915	13353	3.39%	0.580%
10	14.298	1918	1923	1929	rBB2	55511	78713	19.99%	3.420%
11	15.798	2173	2178	2185	rBB	157285	203121	51.59%	8.826%
12	17.051	2386	2391	2395	rBV2	65459	88782	22.55%	3.858%
13	17.092	2395	2398	2403	rVB	13869	16349	4.15%	0.710%
14	19.116	2738	2742	2747	rBB	18621	22480	5.71%	0.977%
15	19.480	2801	2804	2809	rVB	15416	19547	4.96%	0.849%
16	19.686	2834	2839	2844	rBV	342723	393716	100.00%	17.107%
17	20.945	3049	3053	3056	rBV	9541	9002	2.29%	0.391%
18	21.251	3097	3105	3109	rBV2	74533	100116	25.43%	4.350%
19	21.286	3109	3111	3115	rVB	7040	6983	1.77%	0.303%
20	21.810	3196	3200	3203	rBV2	5243	5764	1.46%	0.250%
21	22.269	3274	3278	3282	rVB	6824	6759	1.72%	0.294%
22	22.763	3358	3362	3366	rBV	6131	7409	1.88%	0.322%
23	22.810	3366	3370	3375	rBV	5741	11356	2.88%	0.493%
24	23.286	3446	3451	3454	rBV	2871	4697	1.19%	0.204%
25	23.321	3454	3457	3463	rVB	4925	6373	1.62%	0.277%
26	23.380	3463	3467	3473	rVB	4961	7938	2.02%	0.345%
27	23.480	3477	3484	3490	rBV2	46511	81442	20.69%	3.539%
28	23.957	3561	3565	3568	rVB	2970	4582	1.16%	0.199%
29	25.721	3860	3865	3873	rBV	2952	5632	1.43%	0.245%
30	26.421	3976	3984	3990	rBV	2111	4961	1.26%	0.216%


Sum of corrected areas: 2301474

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041019\
Data File : BN005127.D
Acq On : 10 Apr 2019 14:43
Operator : JU/SJ
Sample : K2343-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
TP-7-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

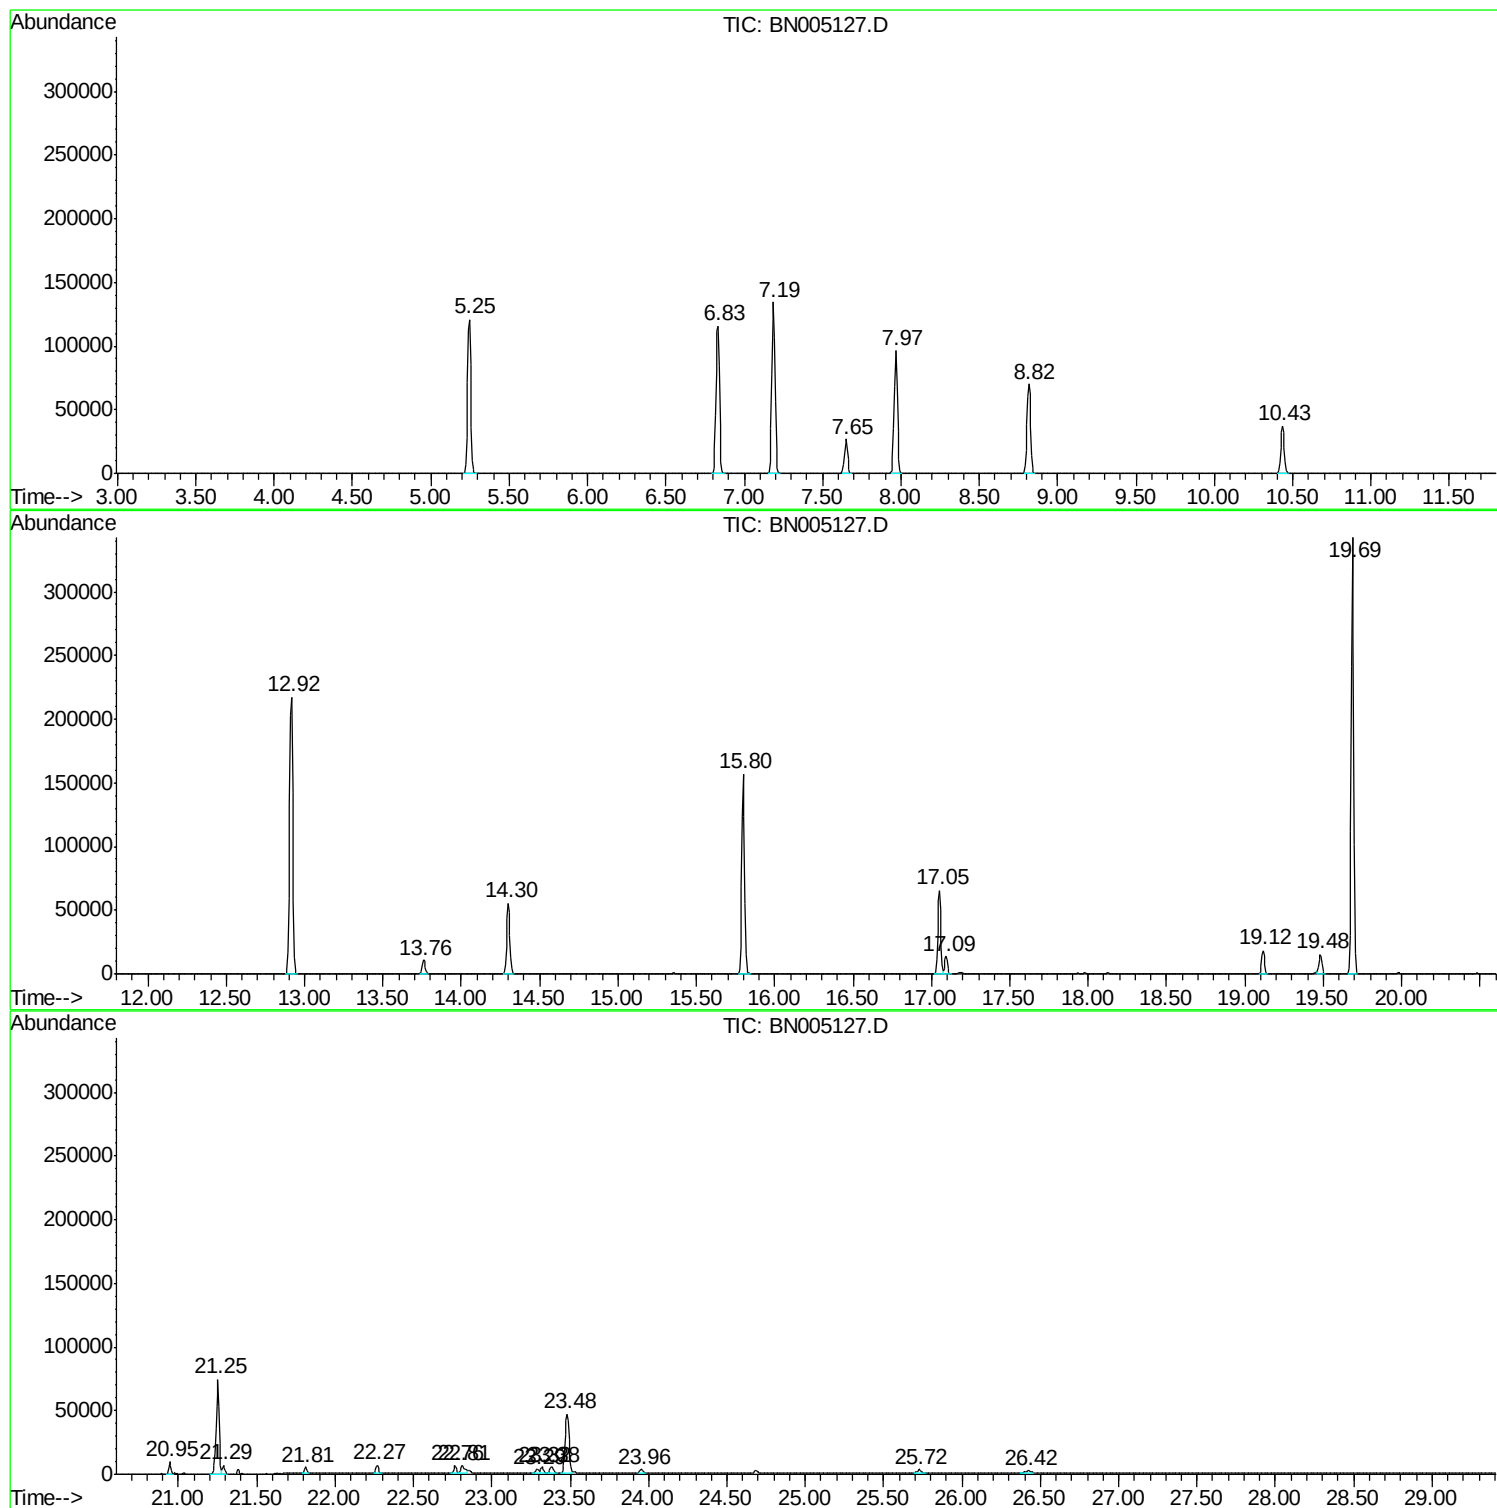

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041019\
Data File : BN005127.D
Acq On : 10 Apr 2019 14:43
Operator : JU/SJ
Sample : K2343-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TP-7-S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.19 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	103.81 ng	199518	1,4-Dichlorobenzene-d4	7.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

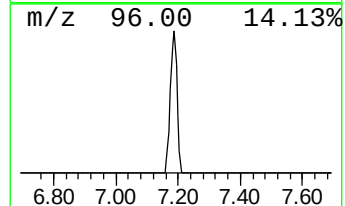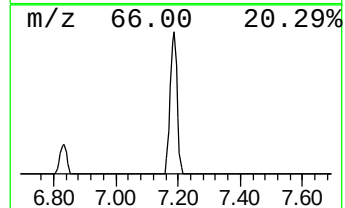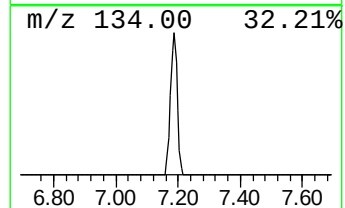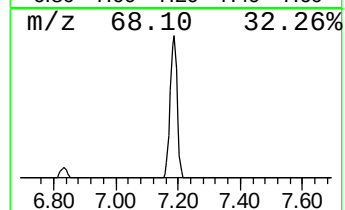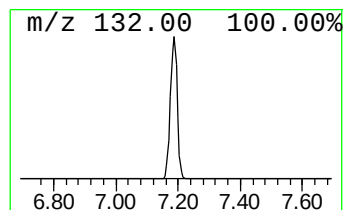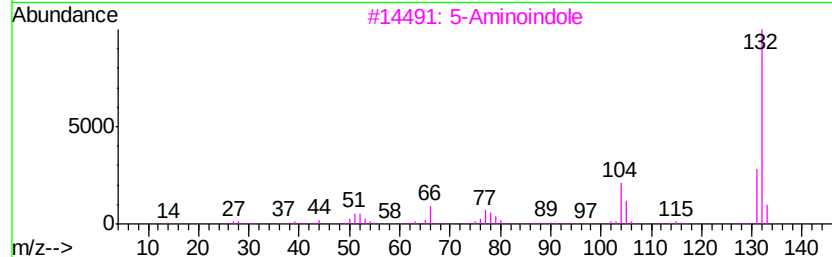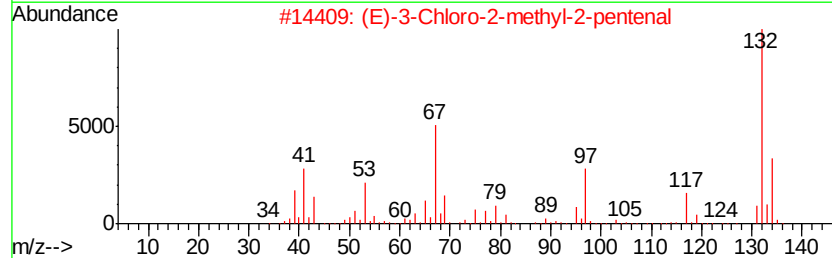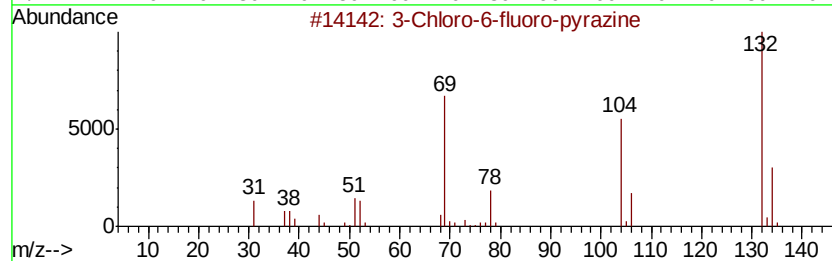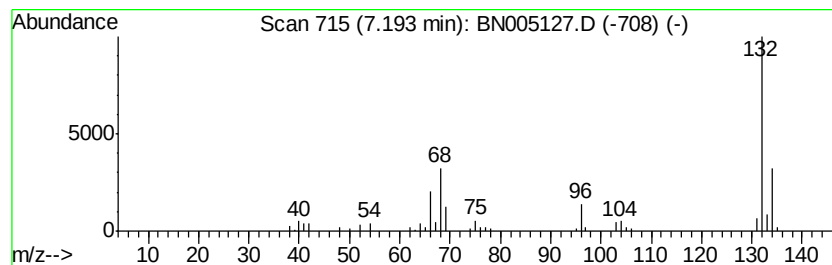

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041019\
Data File : BN005127.D
Acq On : 10 Apr 2019 14:43
Operator : JU/SJ
Sample : K2343-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TP-7-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.19	7.19	103.8	ng	199518	1	7.65	38440	20.0