

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041019\
 Data File : BN005138.D
 Acq On : 10 Apr 2019 21:16
 Operator : JU/SJ
 Sample : PB118783BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB118783BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	378	384	391	rBB	127851	173630	51.59%	8.727%
2	6.834	647	654	661	rBB	118415	180357	53.59%	9.065%
3	7.187	708	714	720	rBB	136646	201700	59.93%	10.138%
4	7.651	788	793	798	rBB	23709	34190	10.16%	1.718%
5	7.969	841	847	852	rBB	98088	153334	45.56%	7.707%
6	8.816	985	991	997	rBB	70265	108997	32.39%	5.478%
7	10.434	1260	1266	1273	rBB	31862	49785	14.79%	2.502%
8	12.916	1681	1688	1694	rBB	209277	302244	89.80%	15.191%
9	14.298	1918	1923	1929	rBB2	46429	65921	19.59%	3.313%
10	15.798	2173	2178	2185	rBB	142456	187486	55.71%	9.423%
11	17.051	2386	2391	2397	rBB	51349	67919	20.18%	3.414%
12	19.686	2833	2839	2844	rBV	280164	336564	100.00%	16.916%
13	21.251	3100	3105	3111	rBV	50858	62350	18.53%	3.134%
14	23.480	3477	3484	3492	rVB	36256	65145	19.36%	3.274%


Sum of corrected areas: 1989622

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041019\
Data File : BN005138.D
Acq On : 10 Apr 2019 21:16
Operator : JU/SJ
Sample : PB118783BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118783BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

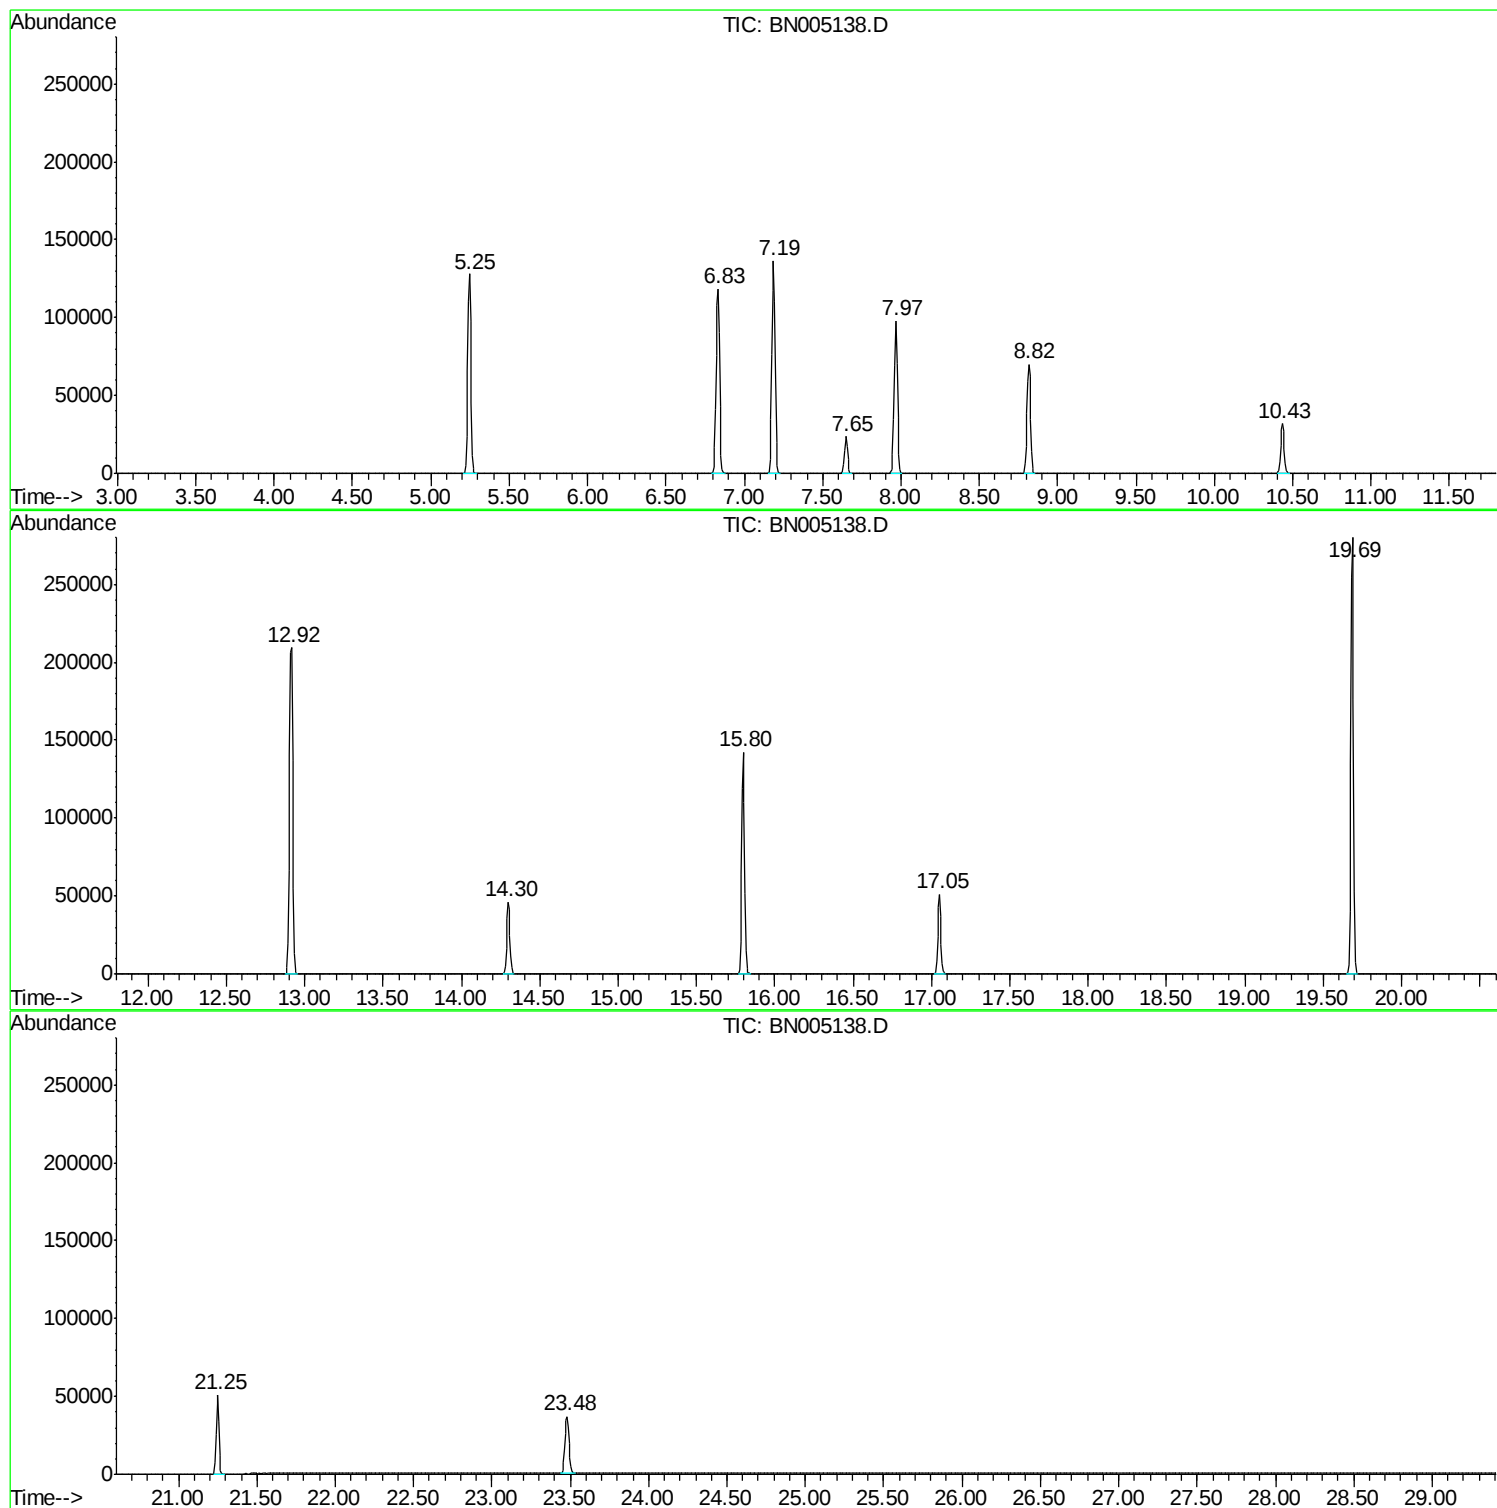

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041019\
Data File : BN005138.D
Acq On : 10 Apr 2019 21:16
Operator : JU/SJ
Sample : PB118783BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118783BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.19 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	117.99 ng	201700	1,4-Dichlorobenzene-d4	7.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

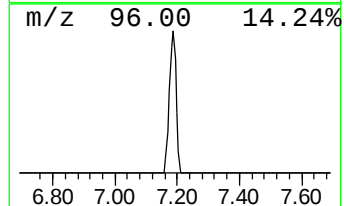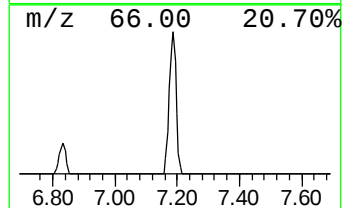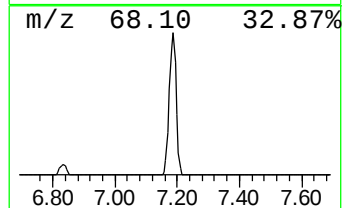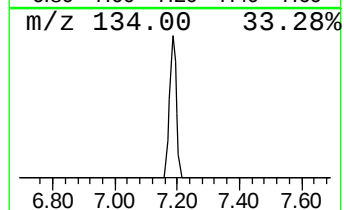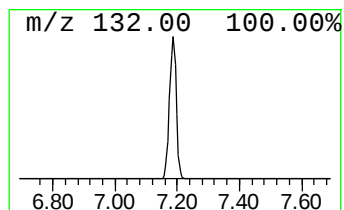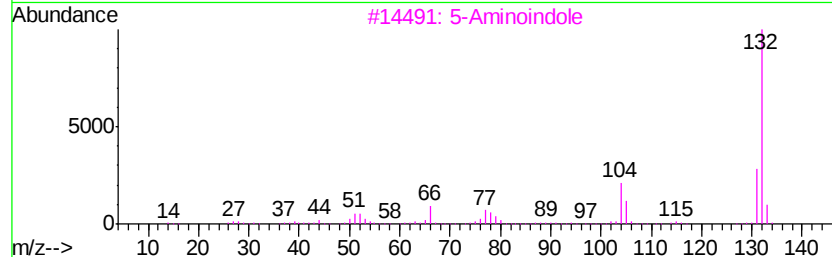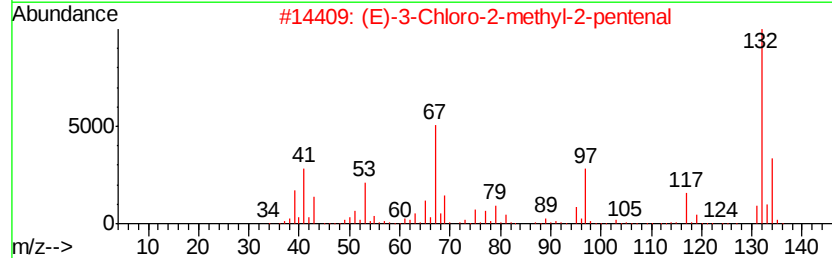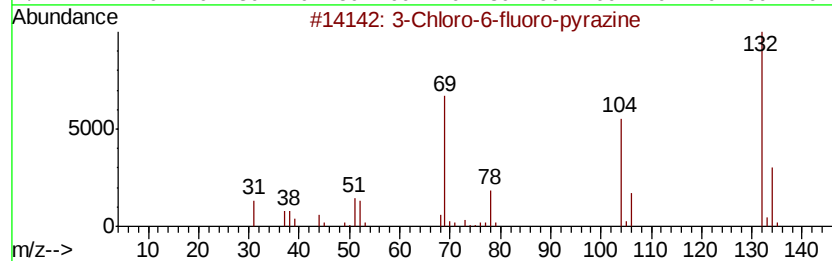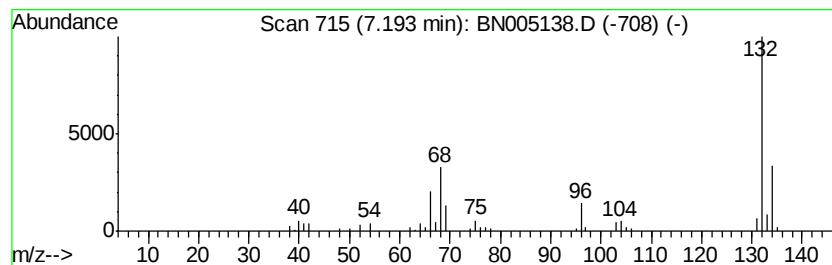

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041019\
Data File : BN005138.D
Acq On : 10 Apr 2019 21:16
Operator : JU/SJ
Sample : PB118783BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118783BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.19	7.19	118.0	ng	201700	1	7.65	34190	20.0