
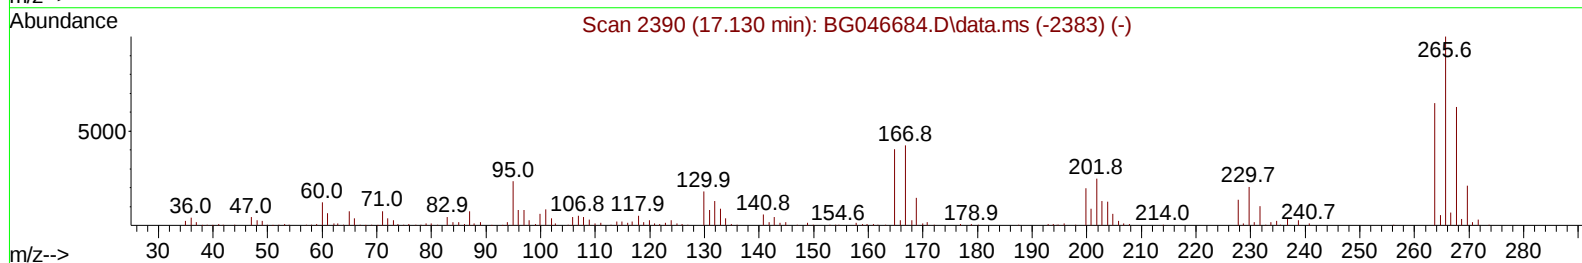
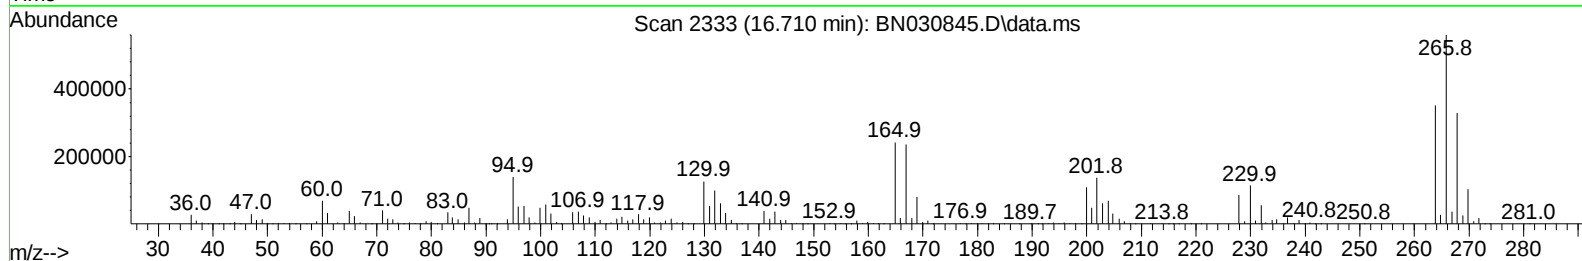


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041124\
Data File : BN030845.D
Acq On : 11 Apr 2024 17:00
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 01:44:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 12 01:44:27 2024
Response via : Initial Calibration

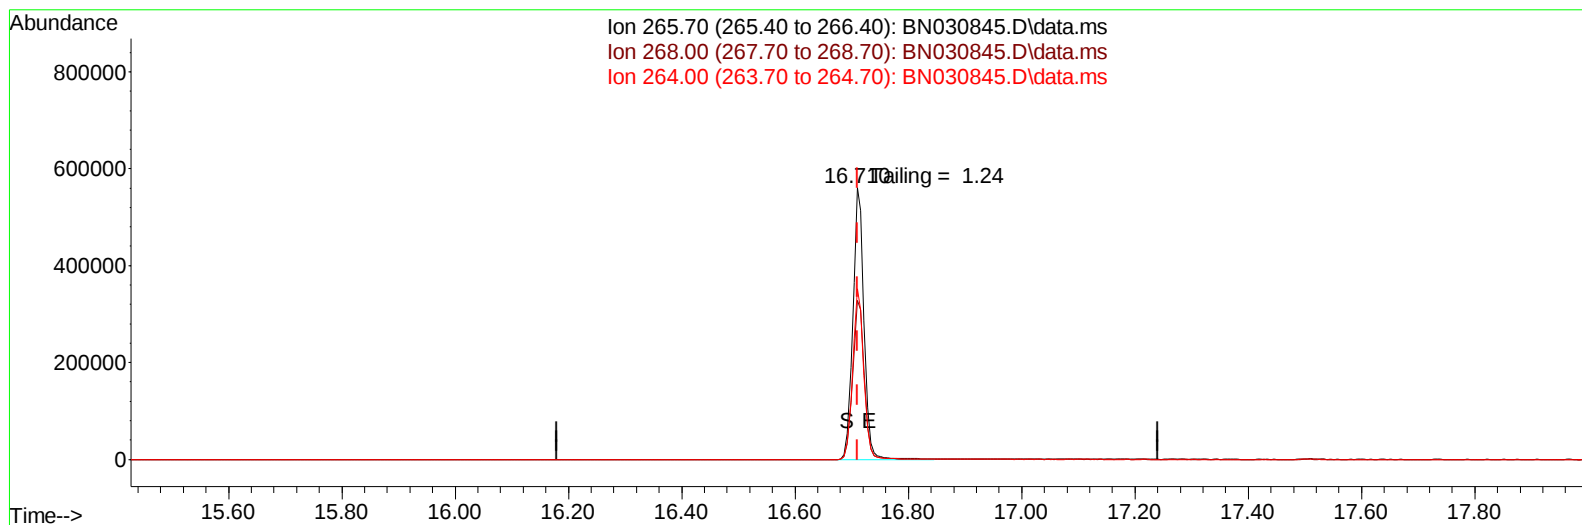




TIC: BN030845.D\data.ms

(70) Pentachlorophenol (C)**16.710min (0.000) 27669.81 ng****response 769130**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.55
264.00	61.60	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041124\
Data File : BN030845.D
Acq On : 11 Apr 2024 17:00
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 01:44:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 12 01:44:27 2024
Response via : Initial Calibration

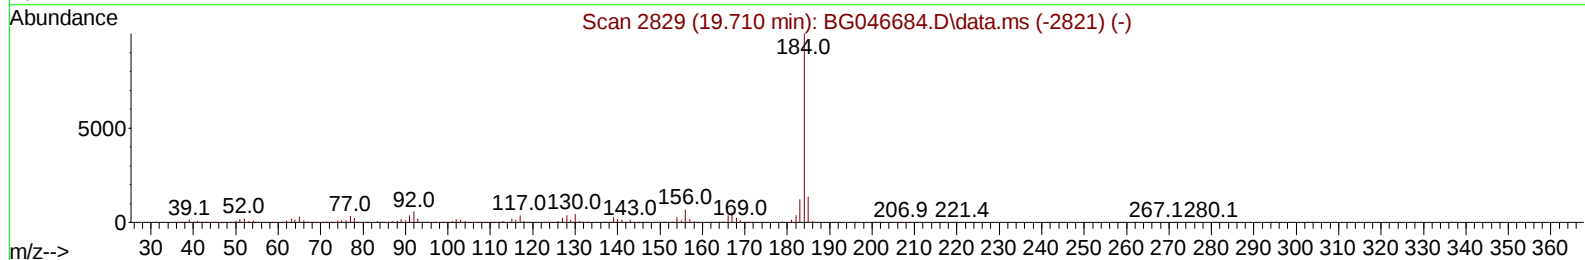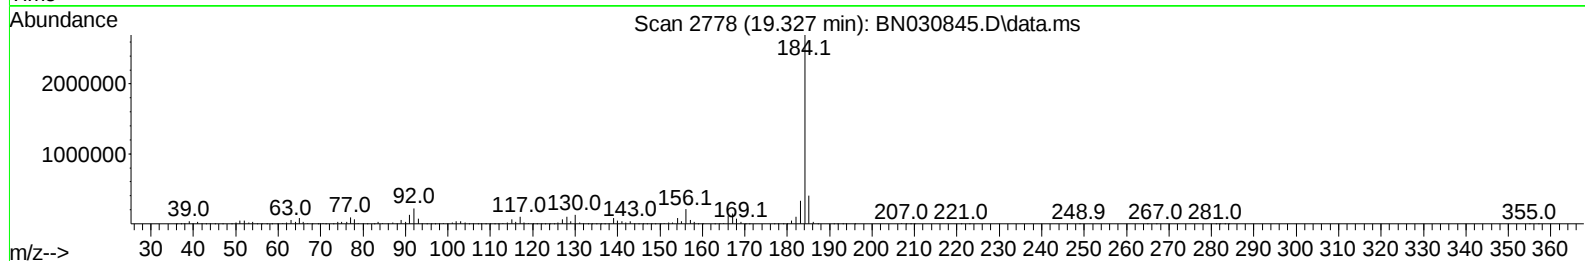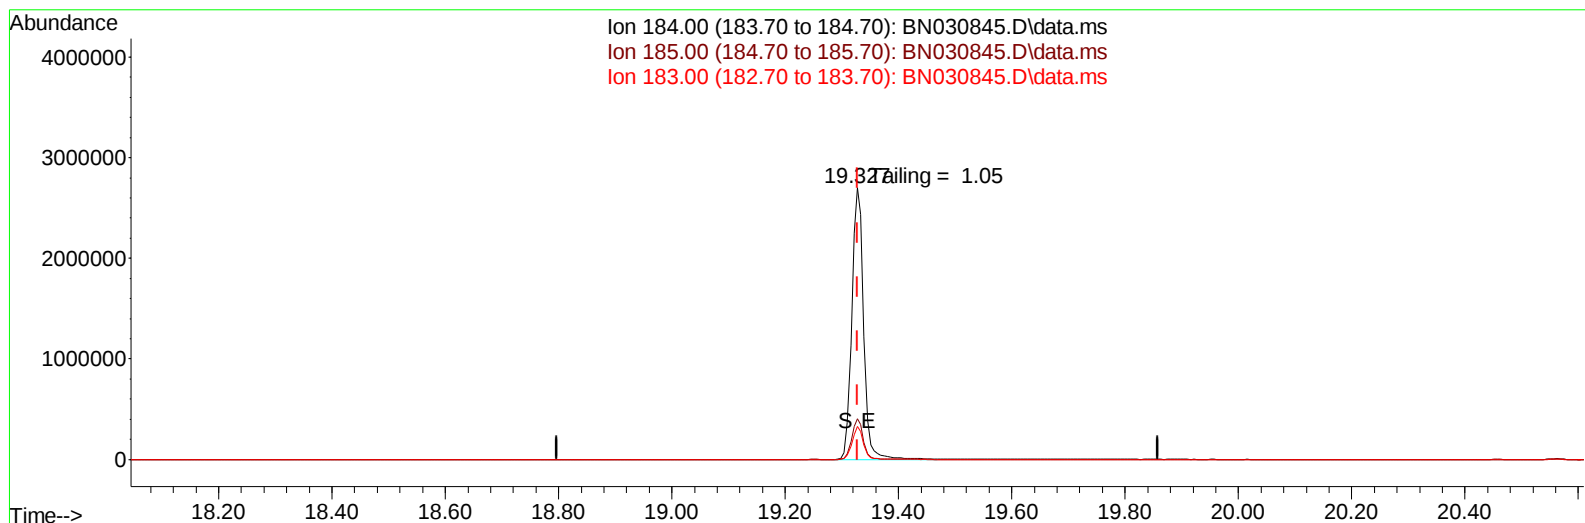

TIC: BN030845.D\data.ms

(77) Benzidine

19.327min (0.000) 0.00 ng

response 3947947

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.99
183.00	13.20	12.10
0.00	0.00	0.00