
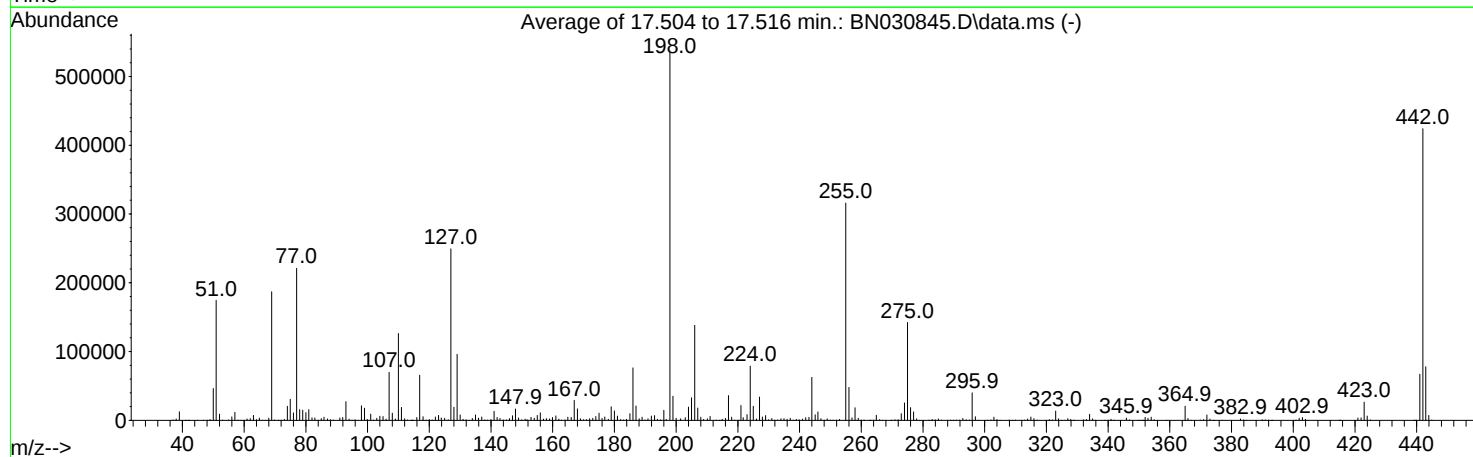


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041124\
Data File : BN030845.D
Acq On : 11 Apr 2024 17:00
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 12 01:10:04 2024

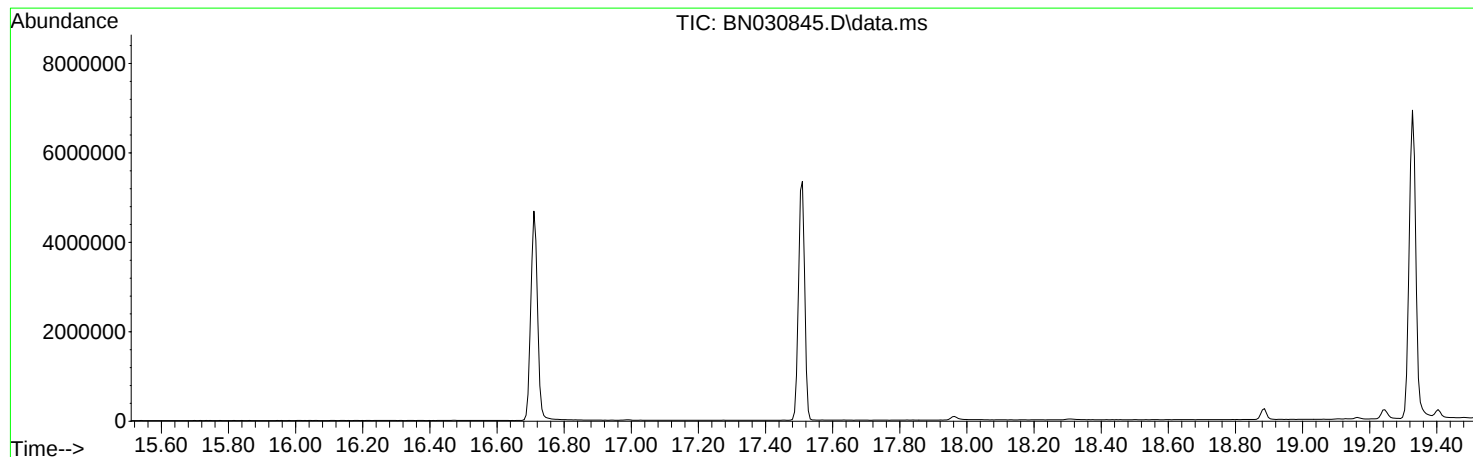




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	174373	PASS
68	69	0.00	2	1.8	3313	PASS
69	198	0.00	100	35.0	187067	PASS
70	69	0.00	2	0.4	827	PASS
127	198	10	80	46.6	249301	PASS
197	198	0.00	2	0.3	1464	PASS
198	198	100	100	100.0	534848	PASS
199	198	5	9	6.6	35155	PASS
275	198	10	60	26.6	142376	PASS
365	198	1	100	3.9	20651	PASS
441	198	0.01	100	12.5	66987	PASS
442	442	50	100	100.0	424149	PASS
443	442	15	24	18.4	78027	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041124\
Data File : BN030845.D
Acq On : 11 Apr 2024 17:00
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 12 01:44:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 12 01:44:27 2024
Response via : Initial Calibration

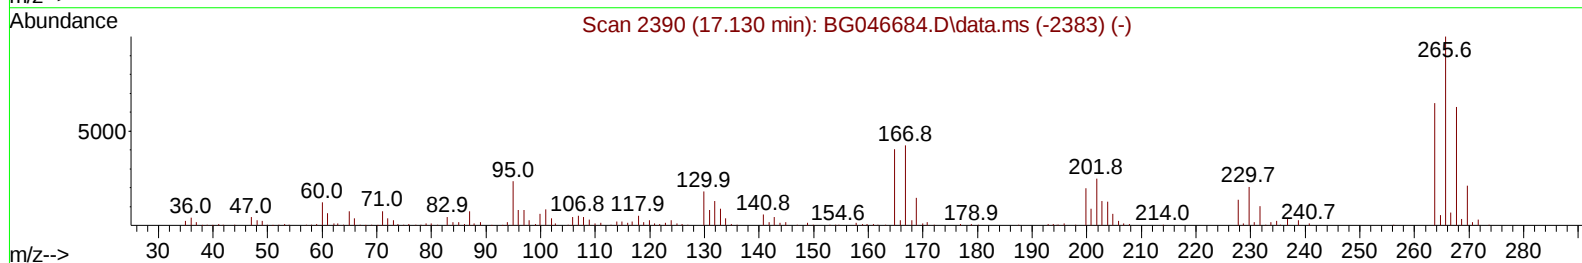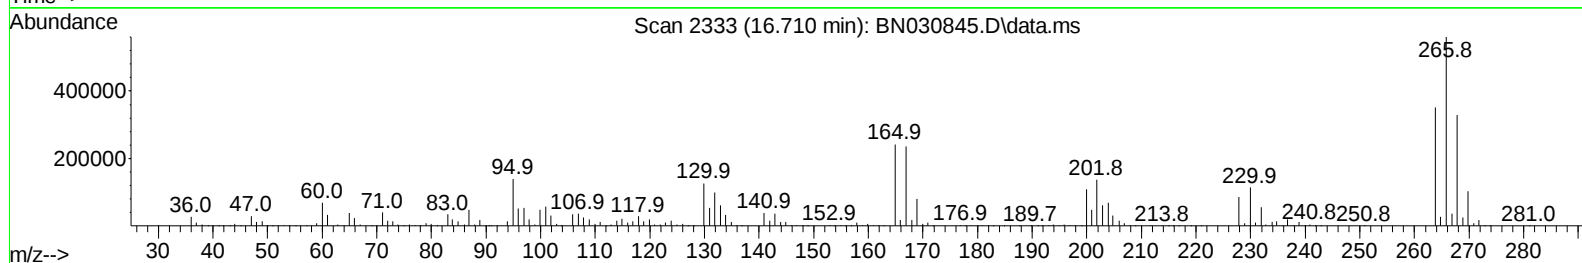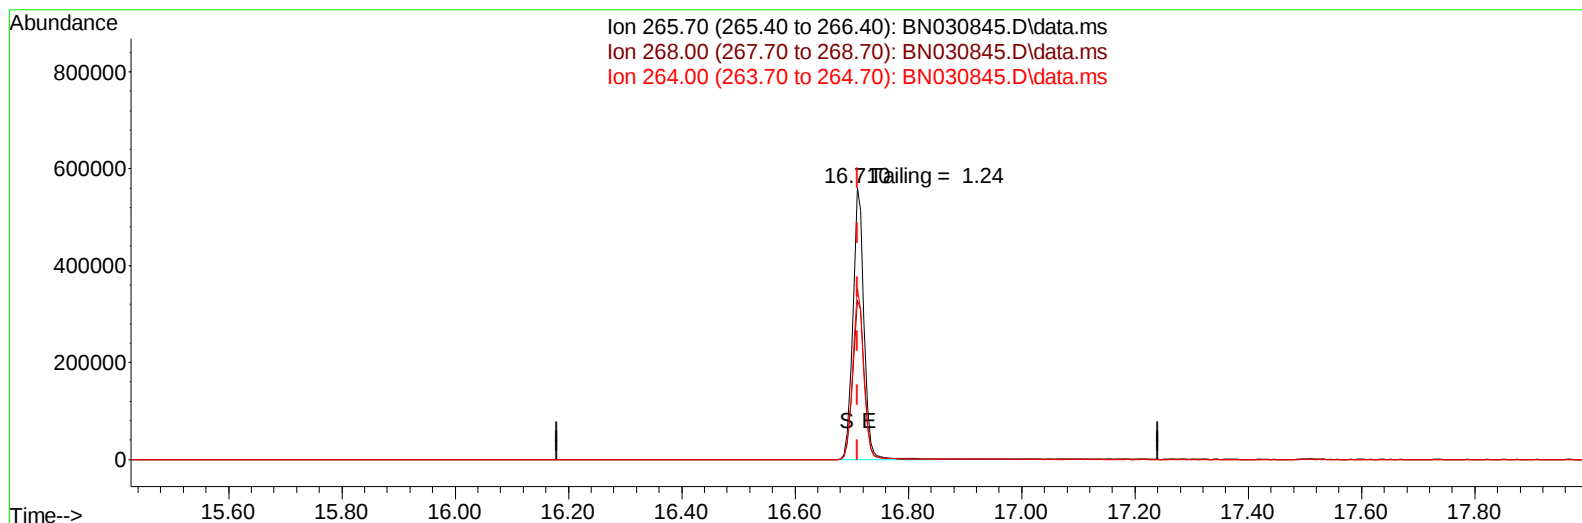

TIC: BN030845.D\data.ms

(70) Pentachlorophenol (C)

16.710min (0.000) 27669.81 ng




response 769130

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.55
264.00	61.60	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041124\
Data File : BN030845.D
Acq On : 11 Apr 2024 17:00
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 12 01:44:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 12 01:44:27 2024
Response via : Initial Calibration

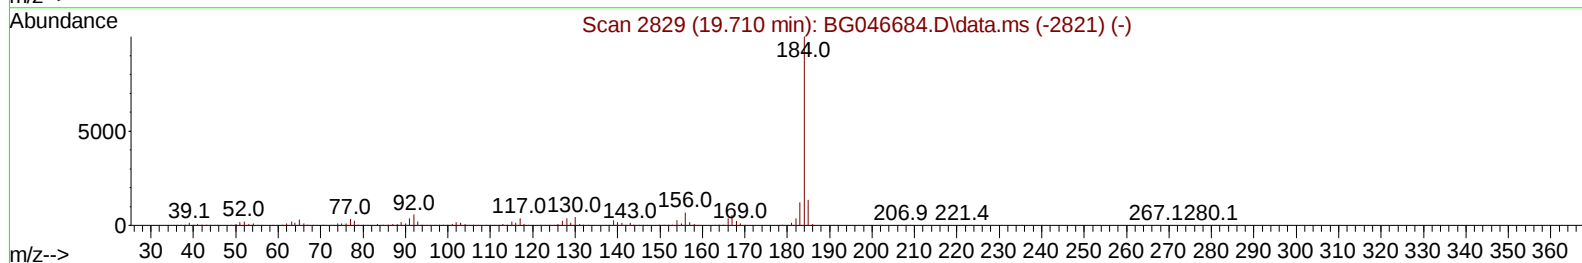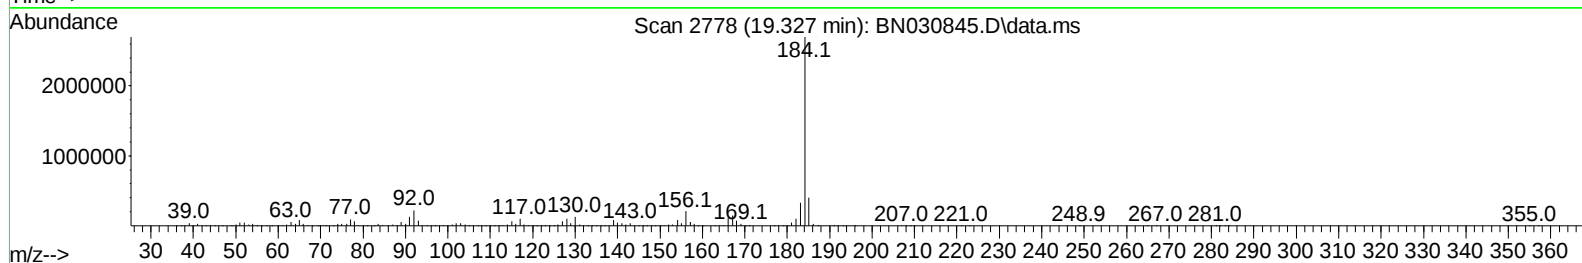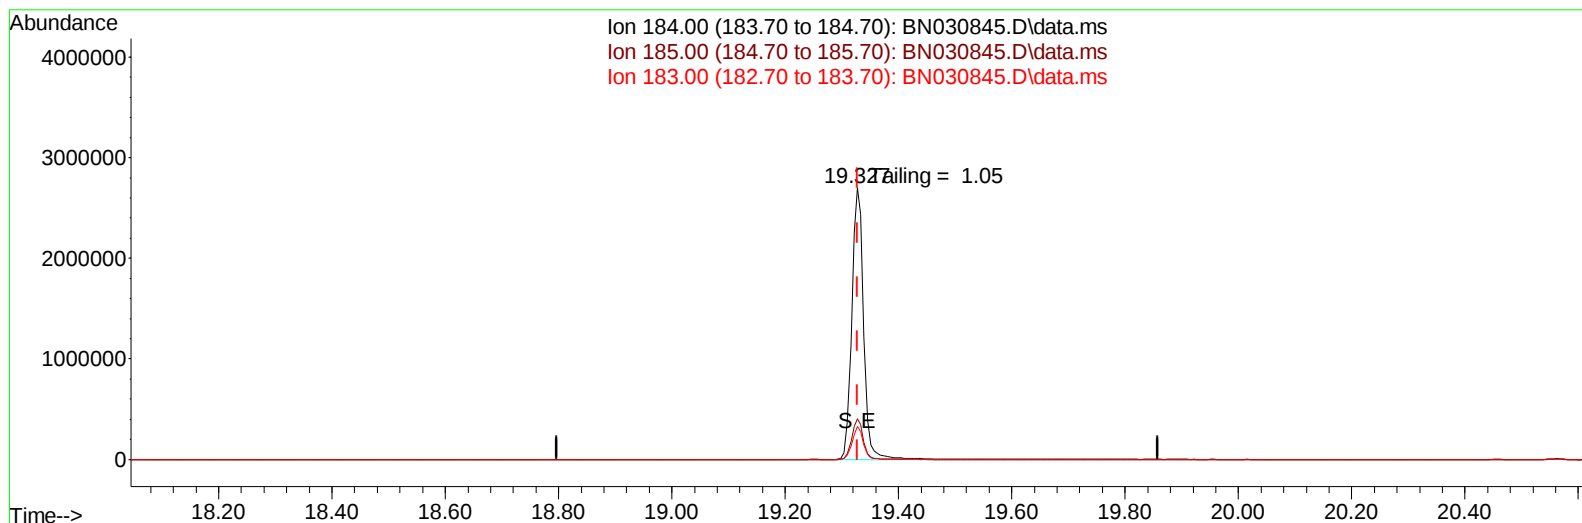

TIC: BN030845.D\data.ms

(77) Benzidine

19.327min (0.000) 0.00 ng

response 3947947

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.99
183.00	13.20	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/11/2024	BNA_N	<u>BN030845.D</u>
Compound Name	Response	Retention Time
DDT	2001225	20.563
DDD	50397	20.122
DDE	1896	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
52293	2053518	2.55

Instrument :
BNA_N
ClientSampleId :
DFTPP