
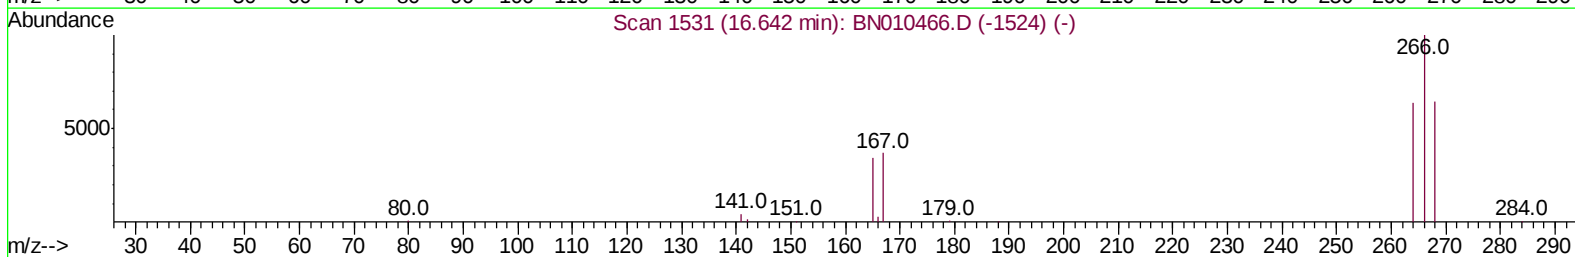
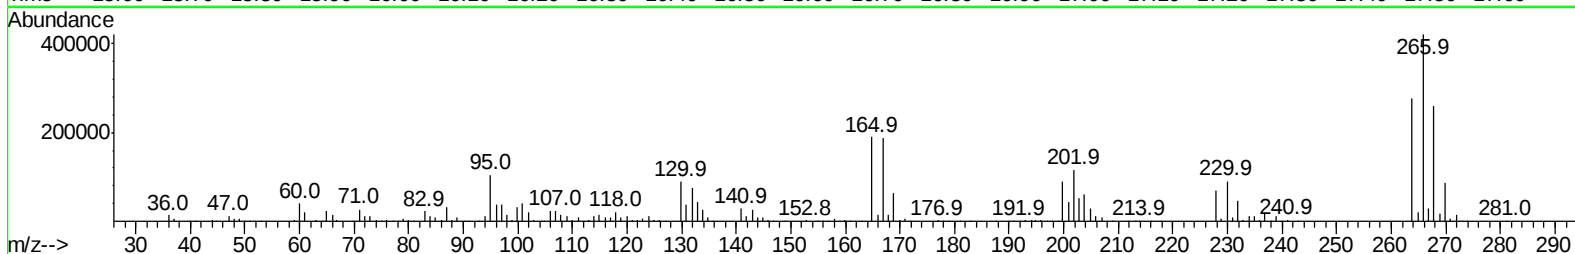


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041420\
 Data File : BN010486.D
 Acq On : 14 Apr 2020 20:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 00:05:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN041320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 13 18:04:22 2020
 Response via : Initial Calibration

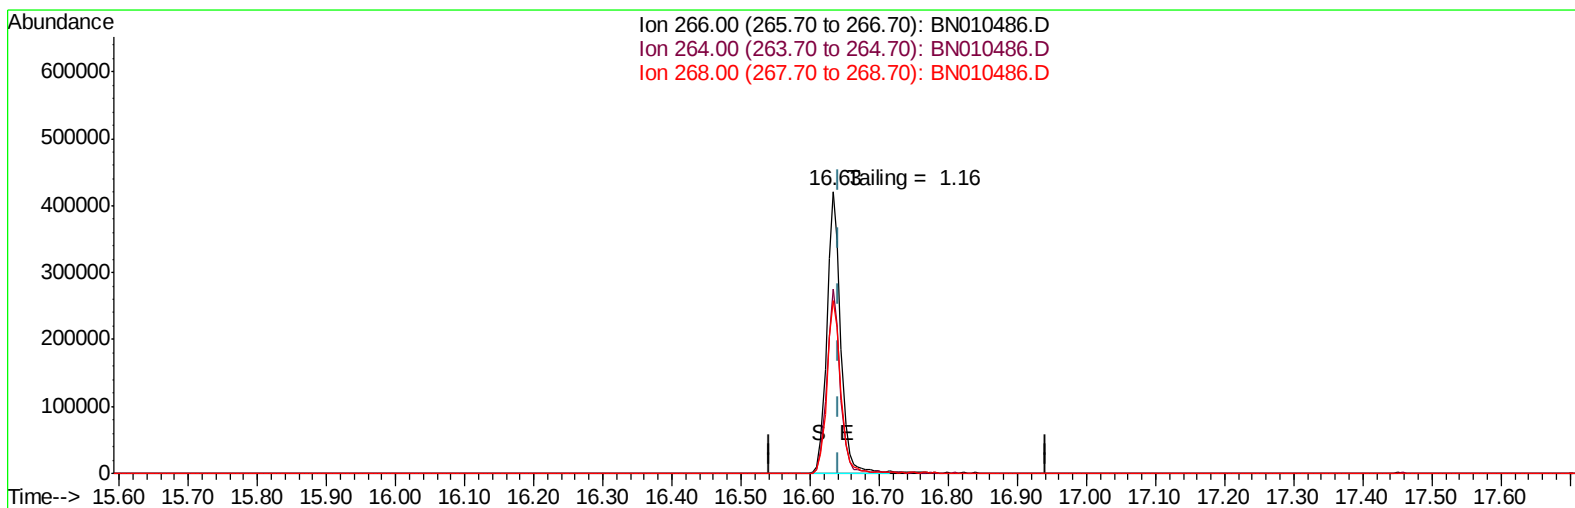

TIC: BN010486.D

(22) Pentachlorophenol

16.633min (-0.008) 0.00ng

response 582197

Ion	Exp%	Act%
266.00	100	100
264.00	64.70	65.47
268.00	67.10	61.53
0.00	0.00	0.00