


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN041420\
 Data File : BN010472.D
 Acq On : 14 Apr 2020 07:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 13 18:04:22 2020

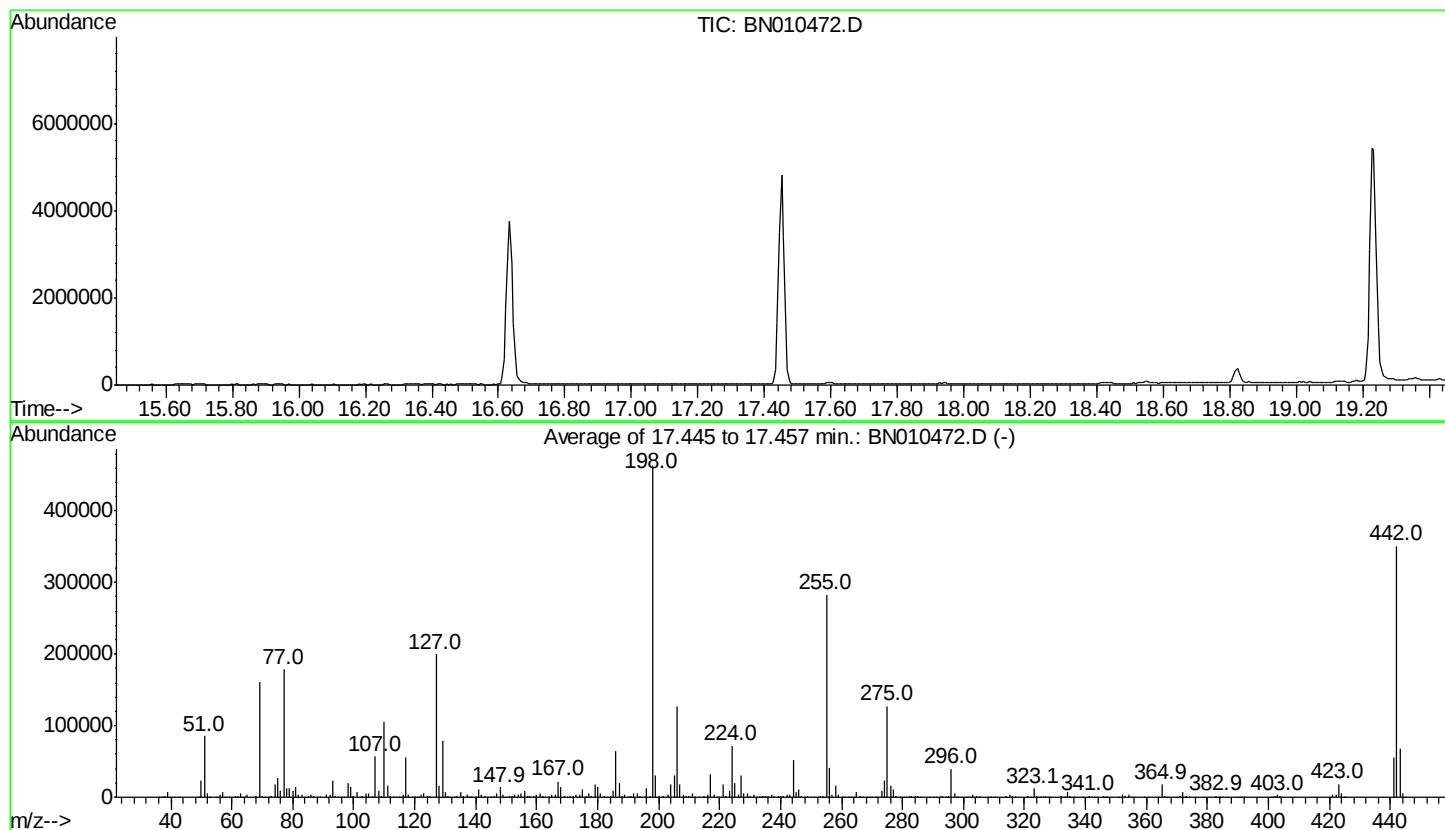

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.5	85589	PASS
68	69	0.00	2	1.6	2577	PASS
69	198	0.00	100	34.8	161106	PASS
70	69	0.00	2	0.6	971	PASS
127	198	10	80	43.1	199850	PASS
197	198	0.00	2	0.2	1113	PASS
198	198	100	100	100.0	463168	PASS
199	198	5	9	6.6	30800	PASS
275	198	10	60	27.5	127317	PASS
365	198	1	100	3.8	17569	PASS
441	198	0.01	100	12.0	55482	PASS
442	198	50	100	75.8	350954	PASS
443	442	15	24	19.5	68394	PASS