


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN041420\
 Data File : BN010486.D
 Acq On : 14 Apr 2020 20:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 13 18:04:22 2020

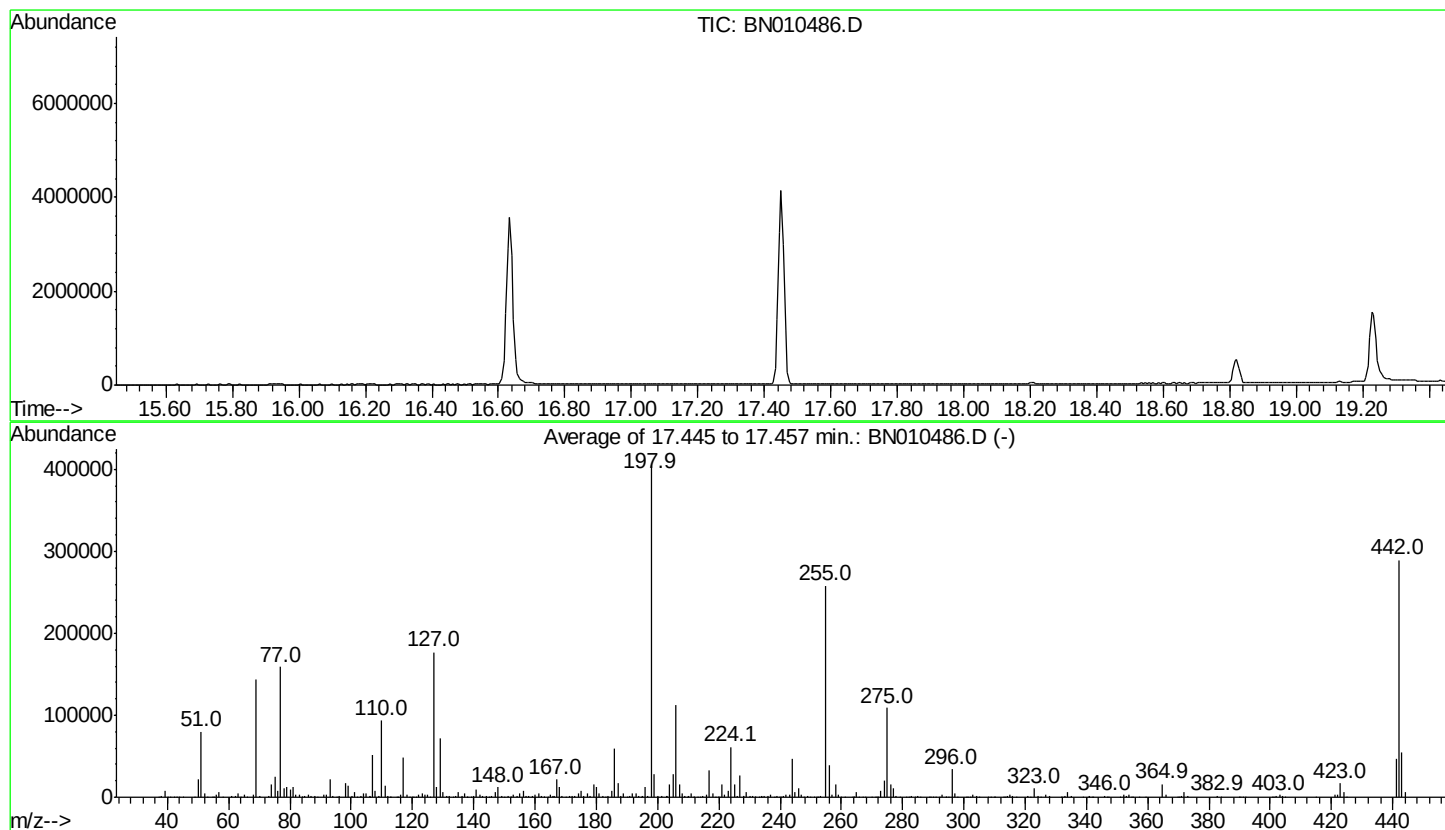

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.8	79938	PASS
68	69	0.00	2	1.9	2661	PASS
69	198	0.00	100	35.4	143381	PASS
70	69	0.00	2	0.6	872	PASS
127	198	10	80	43.8	177066	PASS
197	198	0.00	2	0.2	936	PASS
198	198	100	100	100.0	404522	PASS
199	198	5	9	7.0	28274	PASS
275	198	10	60	26.9	108997	PASS
365	198	1	100	3.9	15841	PASS
441	198	0.01	100	11.7	47141	PASS
442	198	50	100	71.5	289344	PASS
443	442	15	24	18.9	54754	PASS