

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024892.D
 Acq On : 14 Apr 2023 11:34
 Operator : CG/JU
 Sample : 02252-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMEO

Quant Time: Apr 14 22:47:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 14 22:34:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	291722	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	1271257	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	781643	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.334	188	1748253	20.000	ng/ul	0.00
79) Chrysene-d12	21.528	240	1752102	20.000	ng/ul	0.00
88) Perylene-d12	23.980	264	1904265	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	34317	4.477	ng/uL	0.00
4) Pyridine-d5	3.746	84	92539	4.032	ng/ul	0.01
7) Phenol-d5	7.105	99	171408	6.027	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	868635	45.662	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	482328	23.077	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	314574	13.932	ng/ul	-0.01
21) Nitrobenzene-d5	9.111	128	315053	30.608	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	329801	29.581	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	523424	26.266	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	600692	19.863	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	1882566	31.068	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	2101248	30.261	ng/ul	0.00
54) 4-Nitrophenol-d4	14.781	143	58128	4.680	ng/ul	0.00
60) Fluorene-d10	15.575	176	1633236	31.924	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.693	200	291535	25.624	ng/ul	0.00
73) Anthracene-d10	17.428	188	2701343	32.899	ng/ul	0.00
81) Pyrene-d10	19.728	212	3329023	32.720	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.827	264	3440830	34.558	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.128	94	252629	8.529	ng/ul	99
12) 2-Chlorophenol	7.499	128	98907	4.531	ng/ul	99
32) 4-Chloroaniline	10.916	127	88210	2.881	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024892.D
Acq On : 14 Apr 2023 11:34
Operator : CG/JU
Sample : 02252-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COME0

Quant Time: Apr 14 22:47:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 14 22:34:56 2023
Response via : Initial Calibration




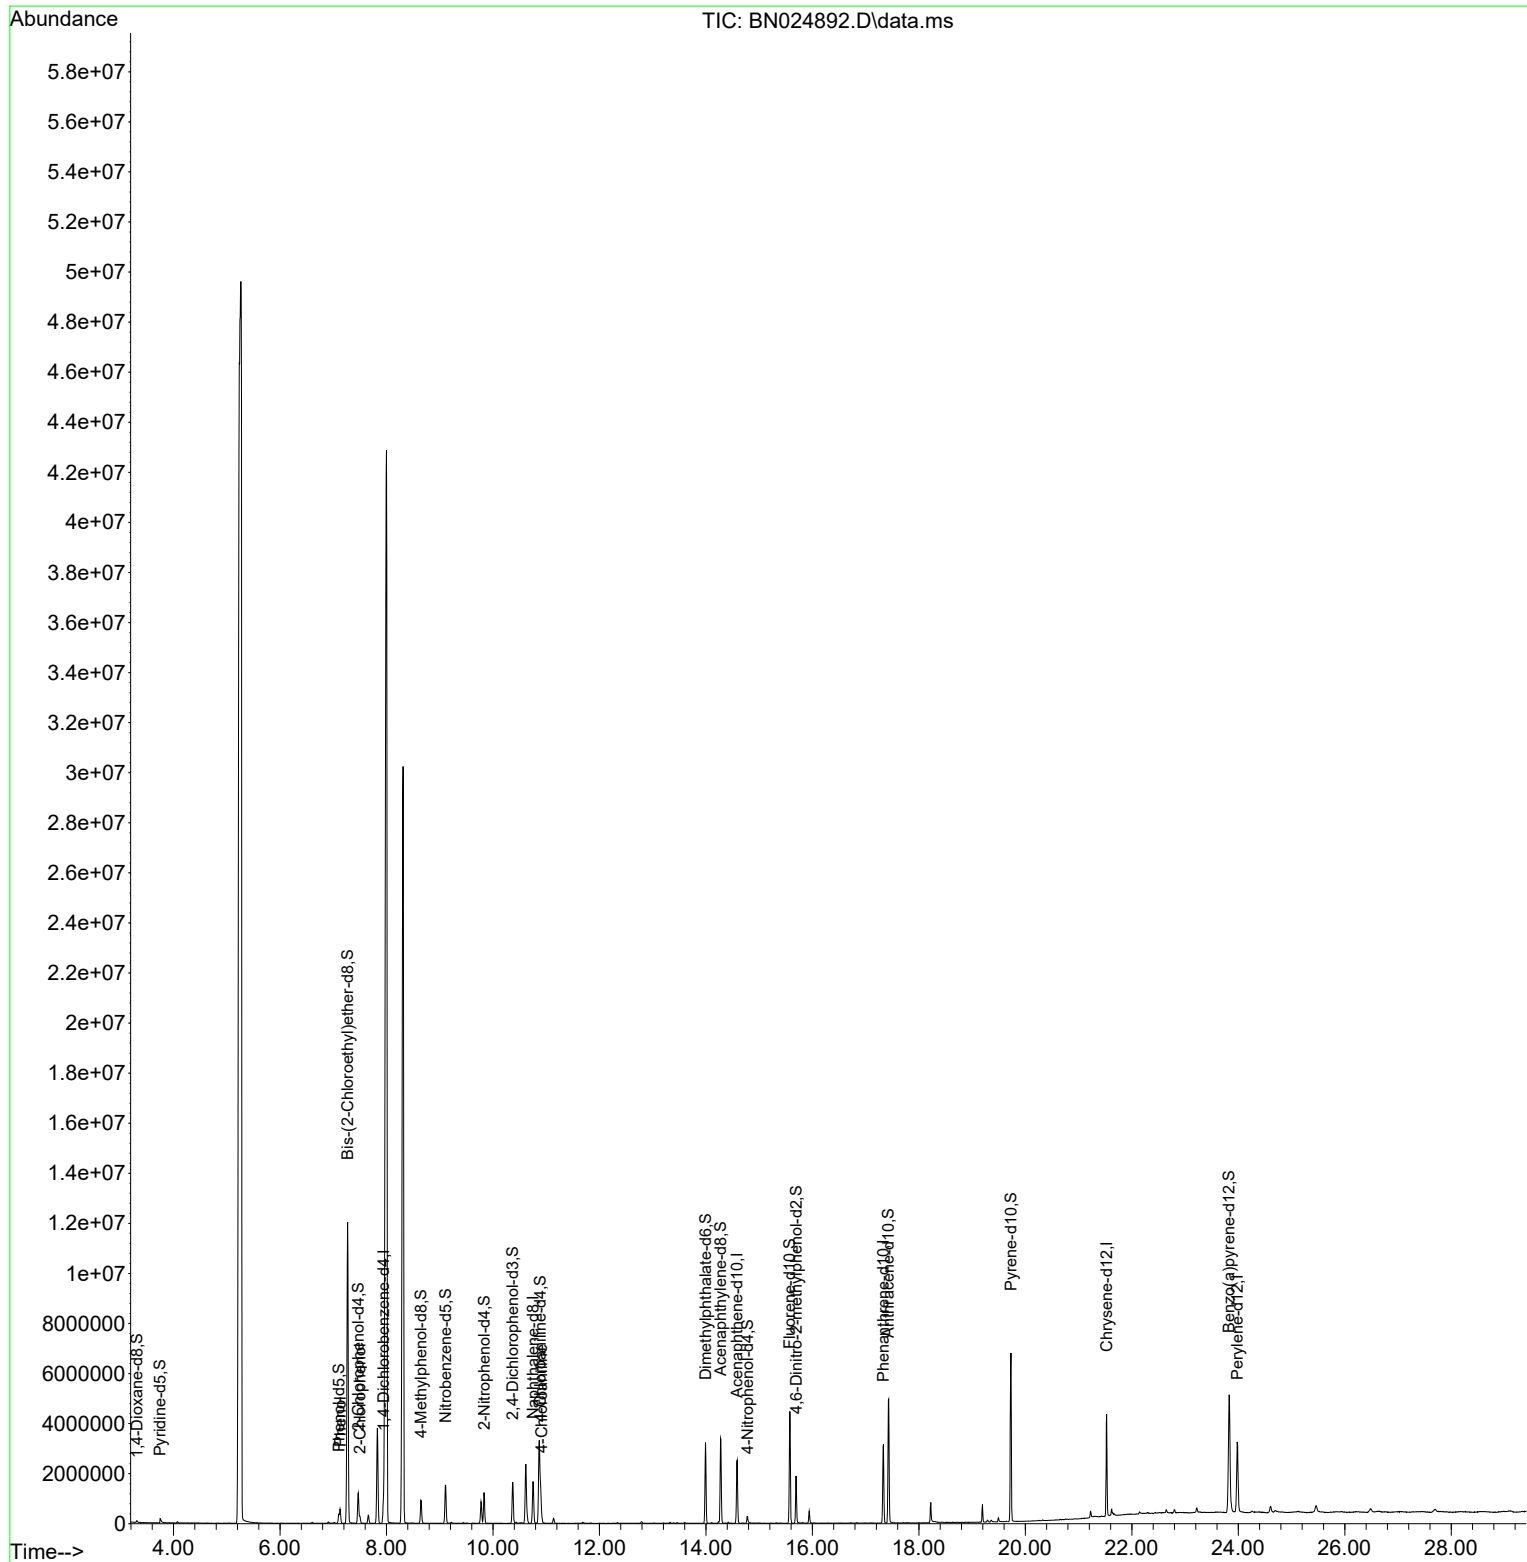


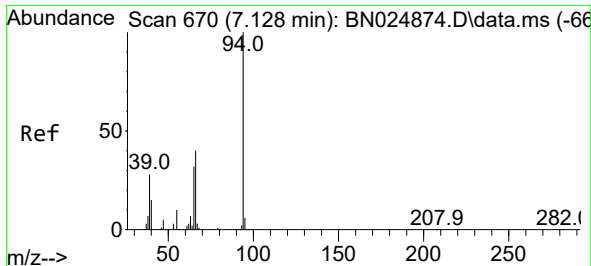

#8
Phenol
Concen: 8.529 ng/ul
RT: 7.128 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN024892.D
Acq: 14 Apr 2023 11:34




Instrument :
BNA_N
ClientSampleId :
COMEO


Tgt Ion: 94 Resp: 252629
Ion Ratio Lower Upper
94 100
65 32.2 25.1 37.7
66 40.0 31.9 47.9

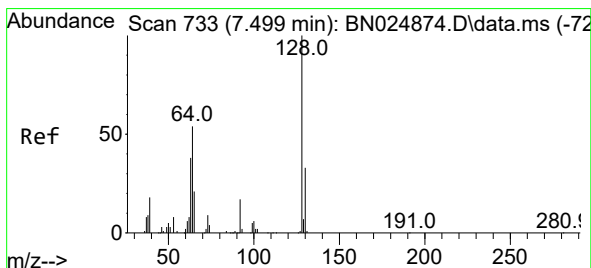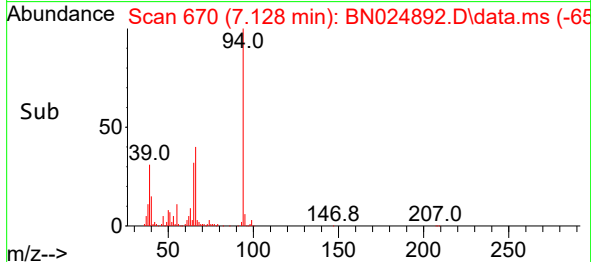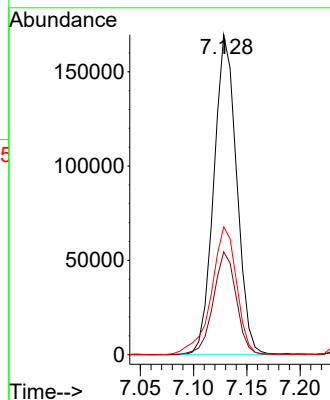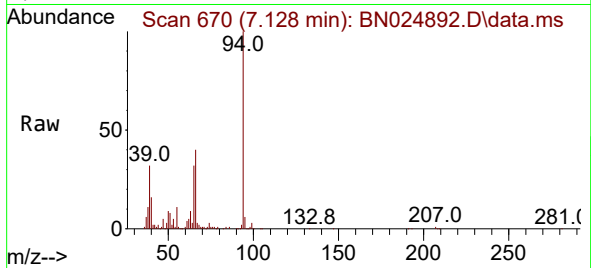

#12
2-Chlorophenol
Concen: 4.531 ng/ul
RT: 7.499 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN024892.D
Acq: 14 Apr 2023 11:34

Tgt Ion: 128 Resp: 98907
Ion Ratio Lower Upper
128 100
64 56.7 44.8 67.2
130 32.4 26.6 39.8

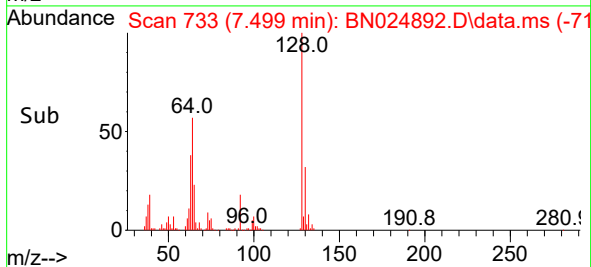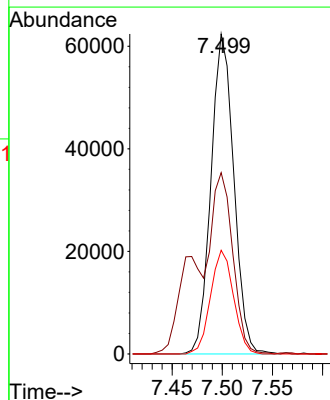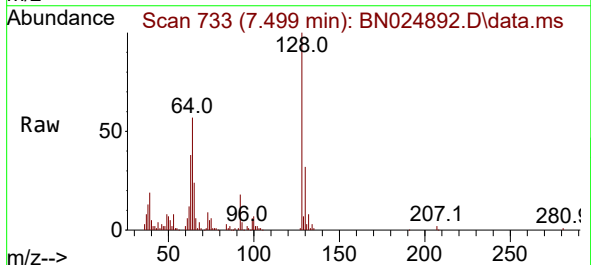

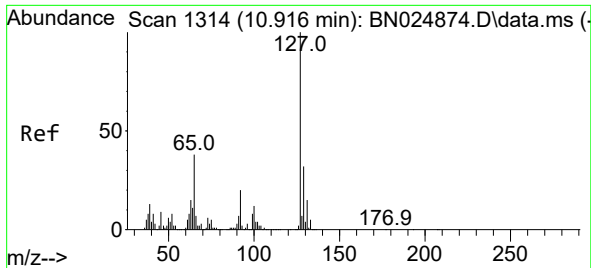

#32
 4-Chloroaniline
 Concen: 2.881 ng/ul
 RT: 10.916 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN024892.D
 Acq: 14 Apr 2023 11:34

Instrument :
 BNA_N
 ClientSampleId :
 COME0

Tgt Ion:127 Resp: 88210
 Ion Ratio Lower Upper
 127 100
 129 31.3 25.5 38.3

