

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024910.D
 Acq On : 14 Apr 2023 23:21
 Operator : CG/JU
 Sample : 02252-14
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMF0

Quant Time: Apr 15 00:03:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 15 00:01:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	296701	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	1386309	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	869686	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.334	188	1920210	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	1864765	20.000	ng/ul	0.00
88) Perylene-d12	23.951	264	1950222	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	33785	4.334	ng/uL	0.00
4) Pyridine-d5	3.746	84	128350	5.498	ng/ul	0.01
7) Phenol-d5	7.099	99	140014	4.840	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	524323	27.100	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	427851	20.127	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	297529	12.956	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	311234	27.728	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	323693	26.624	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	528561	24.322	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	623996	18.921	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	2044909	30.331	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	2266305	29.334	ng/ul	0.00
54) 4-Nitrophenol-d4	14.781	143	49714	3.597	ng/ul	0.00
60) Fluorene-d10	15.575	176	1766049	31.025	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	301430	24.121	ng/ul	0.00
73) Anthracene-d10	17.428	188	2859985	31.712	ng/ul	0.00
81) Pyrene-d10	19.722	212	3401413	31.412	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.798	264	3374544	33.093	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.034	107	31489	1.231	ng/ul	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024910.D
Acq On : 14 Apr 2023 23:21
Operator : CG/JU
Sample : 02252-14
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMF0

Quant Time: Apr 15 00:03:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

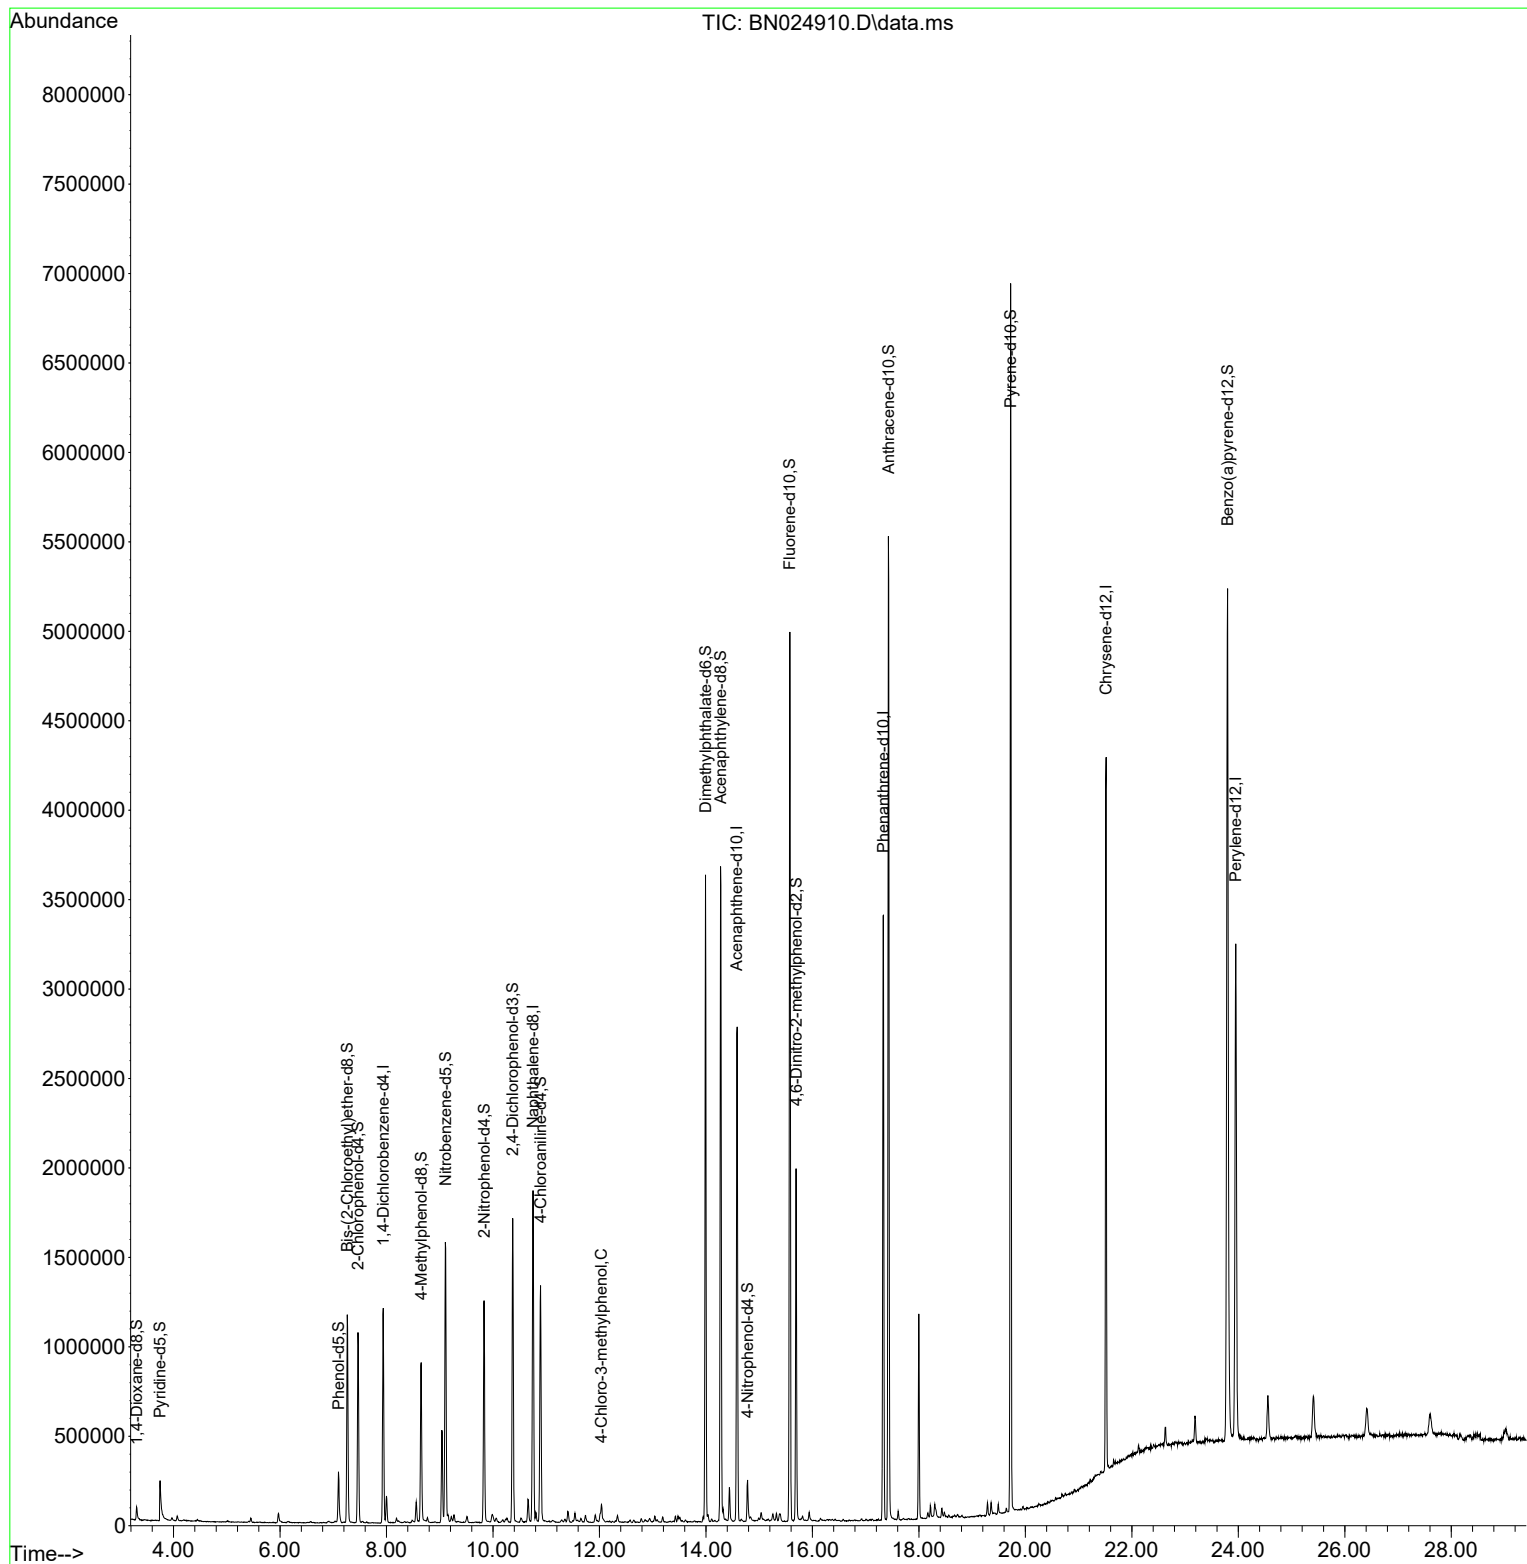

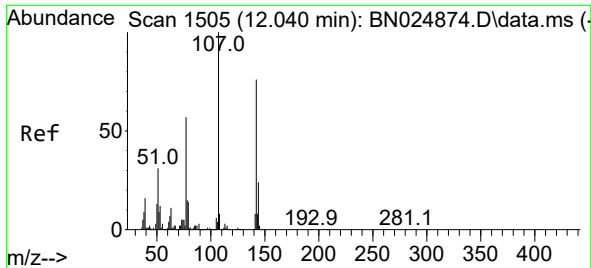

#35
 4-Chloro-3-methylphenol
 Concen: 1.231 ng/ul
 RT: 12.034 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BN024910.D
 Acq: 14 Apr 2023 23:21

Instrument :
 BNA_N
 ClientSampleId :
 COMF0

Tgt Ion:107 Resp: 31489

Ion	Ratio	Lower	Upper
107	100		
144	26.7	19.6	29.4
142	70.5	60.7	91.1

