

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024928.D
 Acq On : 15 Apr 2023 11:00
 Operator : CG/JU
 Sample : 02254-13
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB5

Quant Time: Apr 17 03:01:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 17 02:58:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	313735	20.000	ng/u1	0.00
20) Naphthalene-d8	10.746	136	1380231	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	877807	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.328	188	1940369	20.000	ng/u1	0.00
79) Chrysene-d12	21.522	240	1847868	20.000	ng/u1	0.00
88) Perylene-d12	23.974	264	1934588	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	29237	3.547	ng/uL	0.00
4) Pyridine-d5	3.746	84	125646	5.090	ng/u1	0.01
7) Phenol-d5	7.093	99	207818	6.794	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	586929	28.689	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	530886	23.618	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	374926	15.440	ng/u1	0.00
21) Nitrobenzene-d5	9.105	128	335168	29.991	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	362291	29.929	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	576684	26.654	ng/u1	0.00
31) 4-Chloroaniline-d4	10.887	131	616961	18.790	ng/u1	0.00
46) Dimethylphthalate-d6	13.993	166	2168467	31.866	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	2374031	30.444	ng/u1	0.00
54) 4-Nitrophenol-d4	14.775	143	71896	5.154	ng/u1	0.00
60) Fluorene-d10	15.575	176	1835035	31.939	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	354793	28.096	ng/u1	0.00
73) Anthracene-d10	17.428	188	3181960	34.916	ng/u1	0.00
81) Pyrene-d10	19.722	212	3768129	35.117	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.821	264	3697171	36.550	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.340	88	257372	28.932	ng/uL	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024928.D
Acq On : 15 Apr 2023 11:00
Operator : CG/JU
Sample : 02254-13
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB5

Quant Time: Apr 17 03:01:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 17 02:58:51 2023
Response via : Initial Calibration

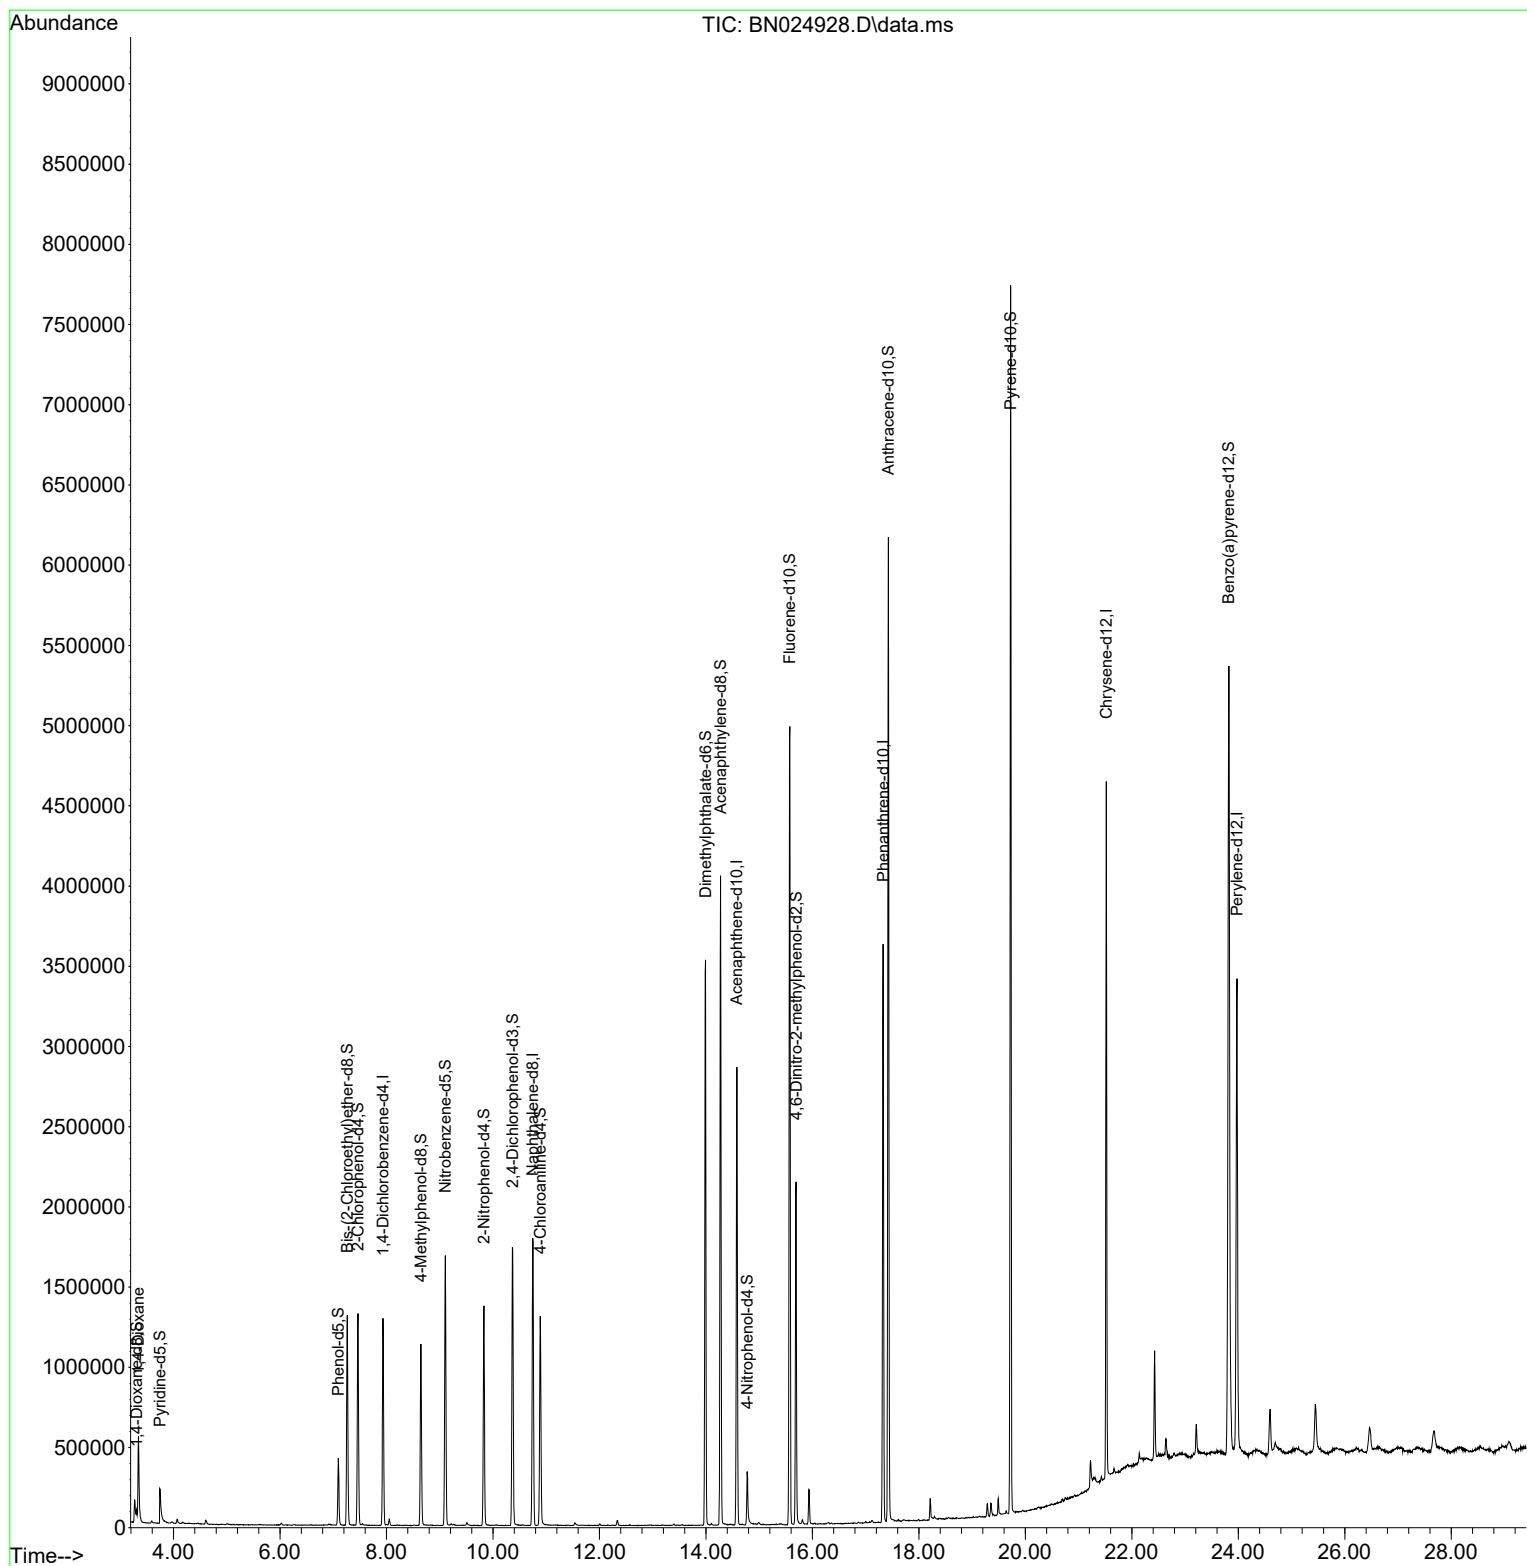

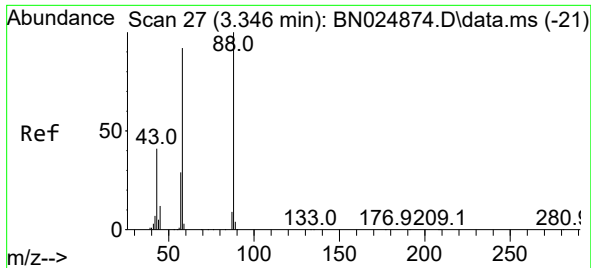

#2
 1,4-Dioxane
 Concen: 28.932 ng/uL
 RT: 3.340 min Scan# 20
 Delta R.T. 0.000 min
 Lab File: BN024928.D
 Acq: 15 Apr 2023 11:00

Instrument :
 BNA_N
 ClientSampleId :
 C0AB5

Tgt Ion: 88 Resp: 257372

Ion	Ratio	Lower	Upper
88	100		
43	39.6	33.0	49.4
58	85.9	72.3	108.5

