

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024932.D
 Acq On : 15 Apr 2023 13:26
 Operator : CG/JU
 Sample : 02254-16
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA6

Quant Time: Apr 17 03:02:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 17 02:58:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	284330	20.000	ng/u1	0.00
20) Naphthalene-d8	10.746	136	1242912	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	777551	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.328	188	1725772	20.000	ng/u1	0.00
79) Chrysene-d12	21.527	240	1776865	20.000	ng/u1	0.00
88) Perylene-d12	23.974	264	1952814	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	34114	4.566	ng/uL	0.00
4) Pyridine-d5	3.740	84	168845	7.548	ng/u1	0.00
7) Phenol-d5	7.093	99	174119	6.281	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	529563	28.562	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	457048	22.436	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	313029	14.224	ng/u1	0.00
21) Nitrobenzene-d5	9.104	128	291911	29.006	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	305972	28.069	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	500567	25.692	ng/u1	0.00
31) 4-Chloroaniline-d4	10.887	131	665780	22.517	ng/u1	0.00
46) Dimethylphthalate-d6	13.992	166	1839487	30.517	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	2062652	29.862	ng/u1	0.00
54) 4-Nitrophenol-d4	14.781	143	55675	4.506	ng/u1	0.00
60) Fluorene-d10	15.575	176	1624401	31.918	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	271523	24.176	ng/u1	0.00
73) Anthracene-d10	17.428	188	2719691	33.554	ng/u1	0.00
81) Pyrene-d10	19.722	212	3139386	30.426	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.821	264	3370012	33.005	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.340	88	829618	102.905	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024932.D
Acq On : 15 Apr 2023 13:26
Operator : CG/JU
Sample : 02254-16
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA6

Quant Time: Apr 17 03:02:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 17 02:58:51 2023
Response via : Initial Calibration

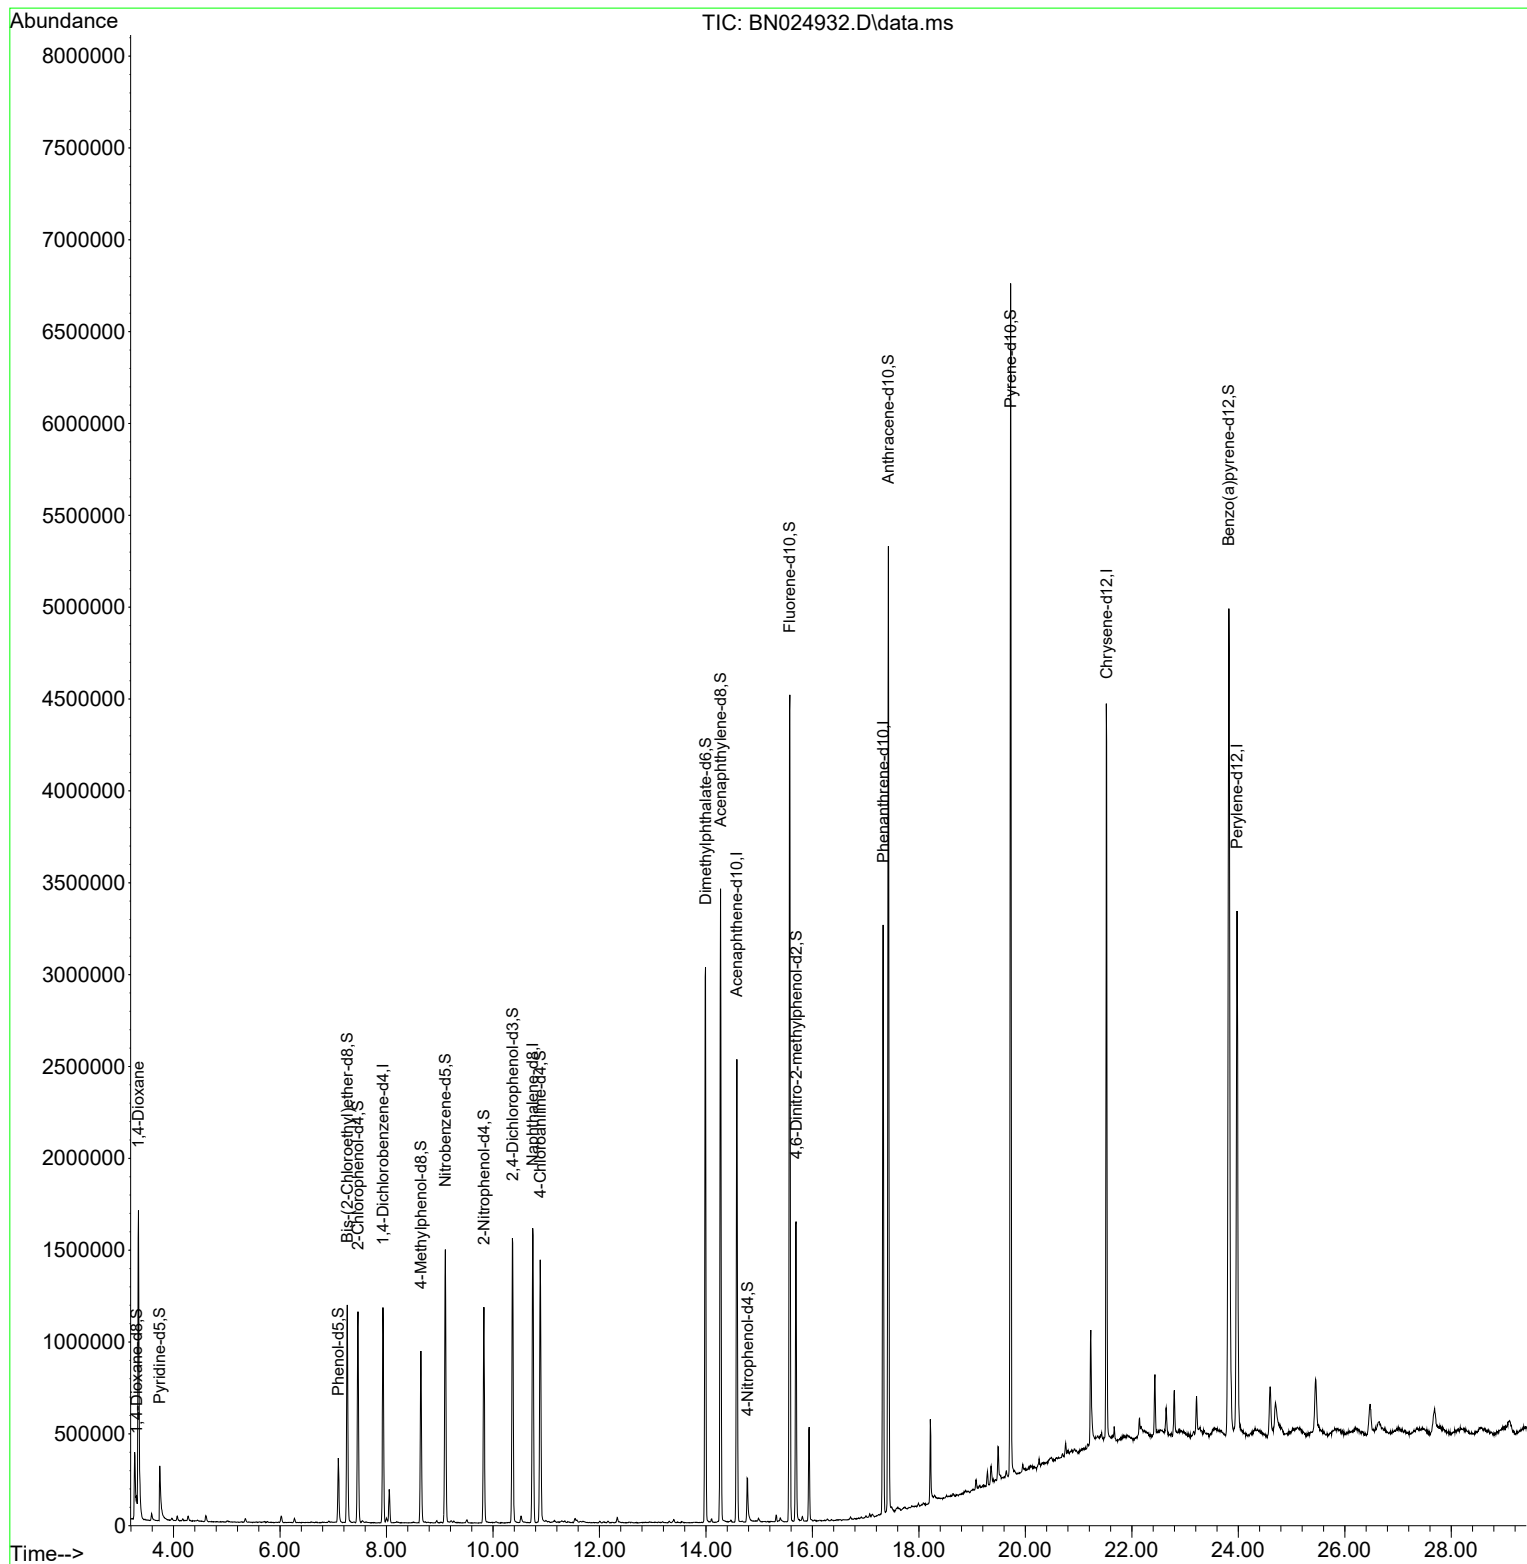

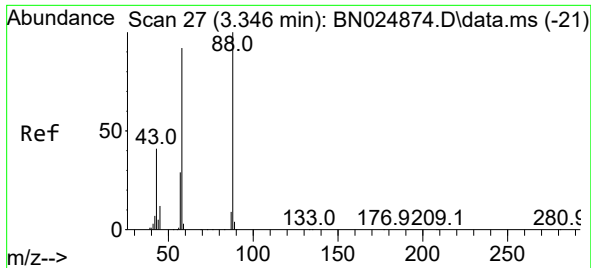

#2
 1,4-Dioxane
 Concen: 102.905 ng/uL
 RT: 3.340 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: BN024932.D
 Acq: 15 Apr 2023 13:26

Instrument :
 BNA_N
 ClientSampleId :
 C0AA6

Tgt Ion: 88 Resp: 829618
 Ion Ratio Lower Upper
 88 100
 43 39.7 33.0 49.4
 58 89.3 72.3 108.5

