

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024936.D
 Acq On : 15 Apr 2023 15:52
 Operator : CG/JU
 Sample : 02254-20
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Quant Time: Apr 17 03:02:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 17 02:58:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	293313	20.000	ng/u1	0.00
20) Naphthalene-d8	10.745	136	1297122	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.580	164	823193	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.327	188	1882030	20.000	ng/u1	0.00
79) Chrysene-d12	21.521	240	1840963	20.000	ng/u1	0.00
88) Perylene-d12	23.974	264	1970261	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.304	96	32389	4.203	ng/uL	0.00
4) Pyridine-d5	3.740	84	177924	7.710	ng/u1	0.00
7) Phenol-d5	7.092	99	174444	6.100	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	530016	27.711	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	453515	21.580	ng/u1	0.00
15) 4-Methylphenol-d8	8.645	113	319752	14.085	ng/u1	0.00
21) Nitrobenzene-d5	9.104	128	295229	28.110	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	305526	26.857	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	513229	25.241	ng/u1	0.00
31) 4-Chloroaniline-d4	10.886	131	745295	24.153	ng/u1	0.00
46) Dimethylphthalate-d6	13.992	166	2064260	32.347	ng/u1	0.00
49) Acenaphthylene-d8	14.274	160	2184553	29.873	ng/u1	0.00
54) 4-Nitrophenol-d4	14.774	143	68655	5.248	ng/u1	0.00
60) Fluorene-d10	15.574	176	1801186	33.430	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	330507	26.984	ng/u1	0.00
73) Anthracene-d10	17.427	188	3090341	34.962	ng/u1	0.00
81) Pyrene-d10	19.721	212	3692685	34.543	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.821	264	3714340	36.055	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.340	88	206116	24.783	ng/uL 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024936.D
Acq On : 15 Apr 2023 15:52
Operator : CG/JU
Sample : 02254-20
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD3

Quant Time: Apr 17 03:02:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 17 02:58:51 2023
Response via : Initial Calibration

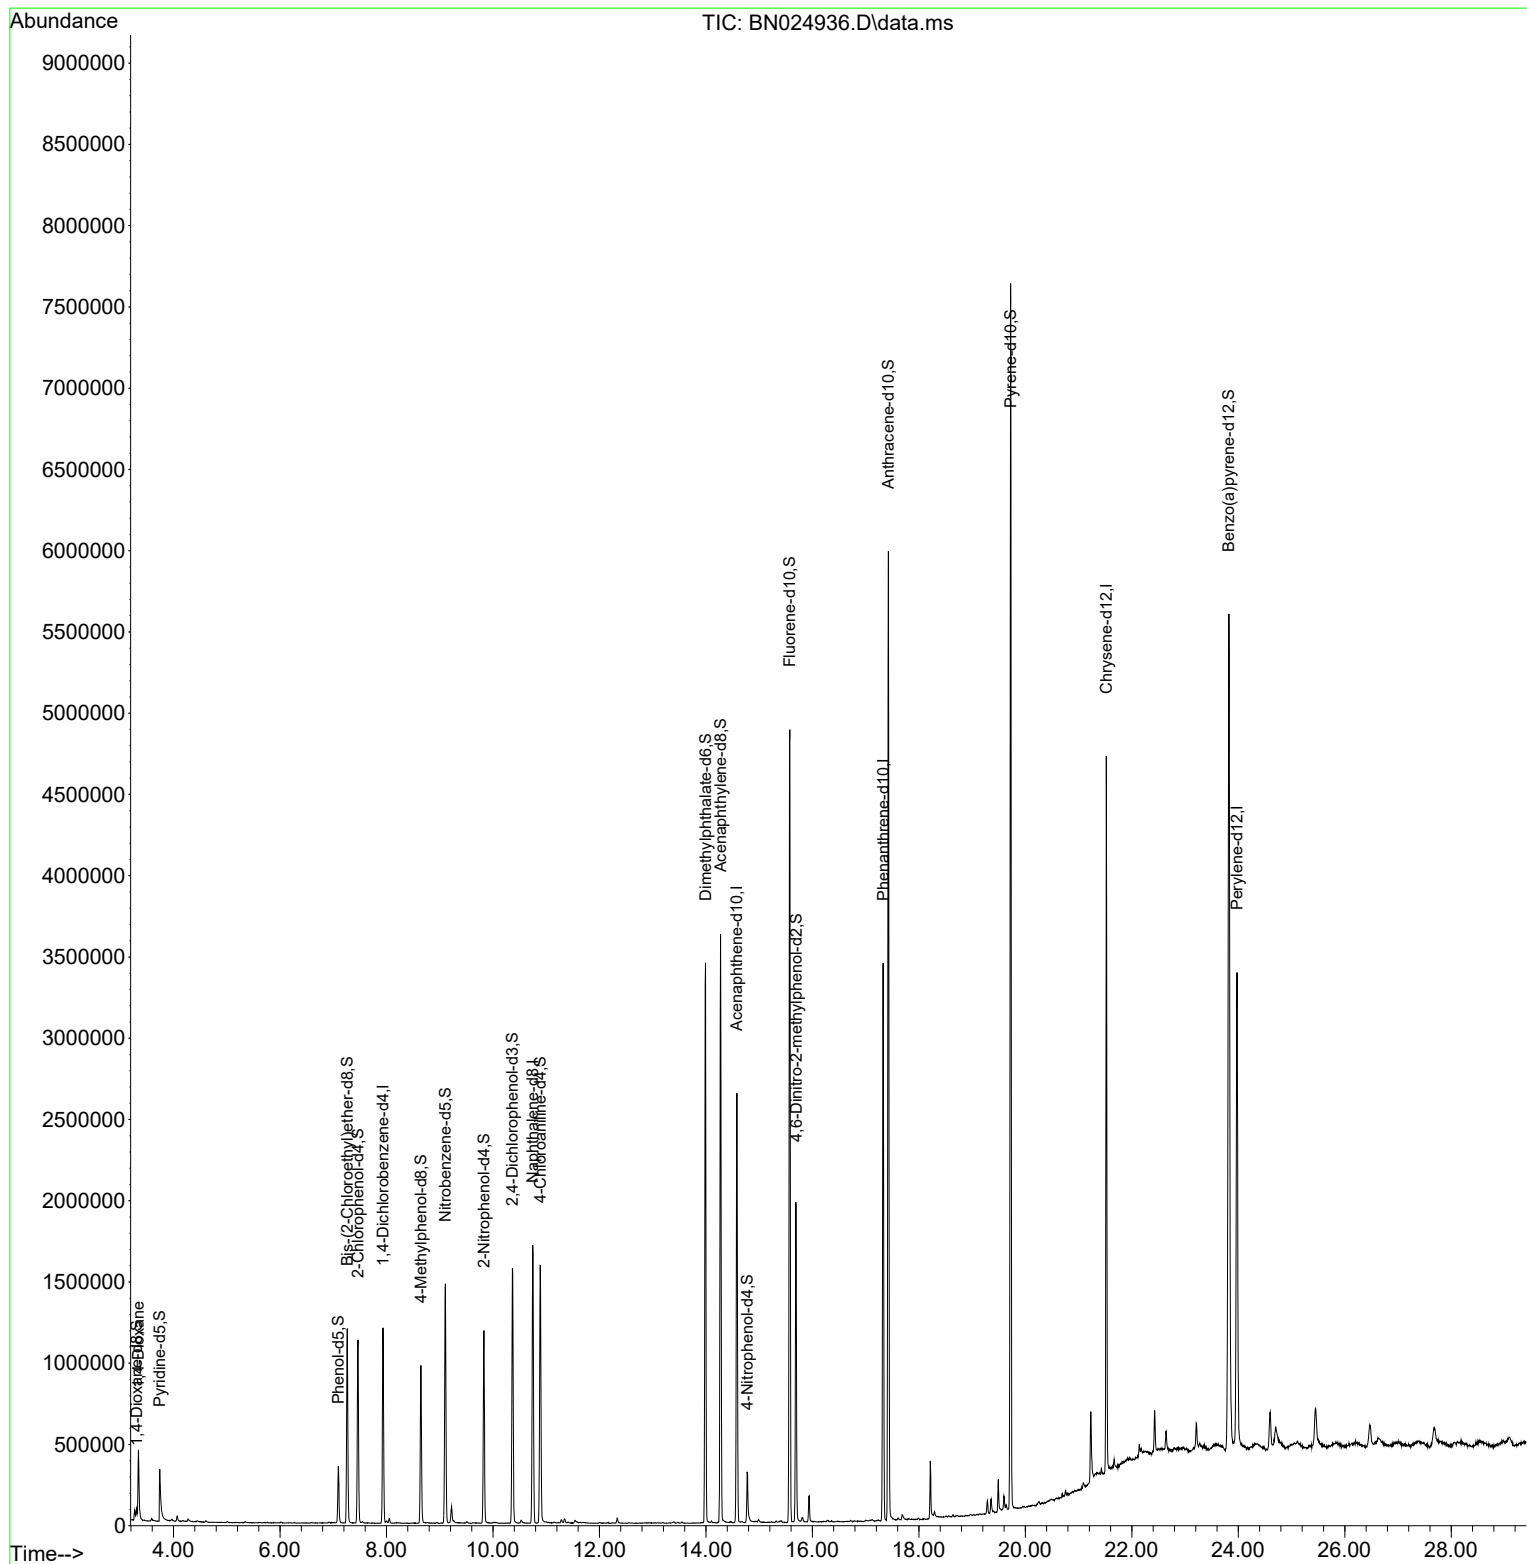

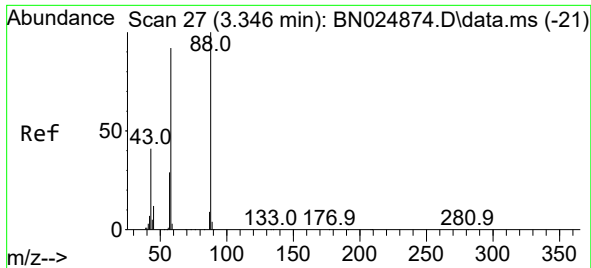

#2
 1,4-Dioxane
 Concen: 24.783 ng/uL
 RT: 3.340 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: BN024936.D
 Acq: 15 Apr 2023 15:52

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Tgt Ion: 88 Resp: 206116
 Ion Ratio Lower Upper
 88 100
 43 38.6 33.0 49.4
 58 86.3 72.3 108.5

