




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024880.D
 Acq On : 14 Apr 2023 04:18
 Operator : CG/JU
 Sample : 02275-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ1

Manual IntegrationsAPPROVED

Quant Time: Apr 14 04:54:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 14 03:27:44 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/14/2023
 Supervised By :Jagrut Upadhyay 04/14/2023

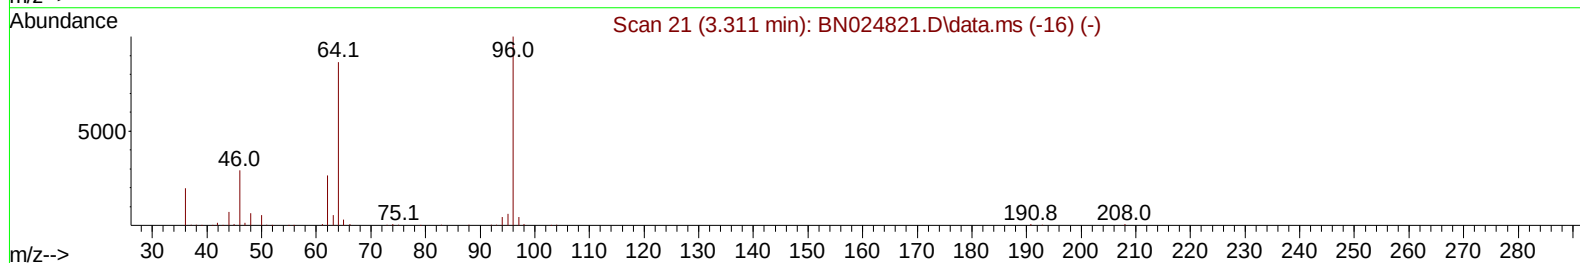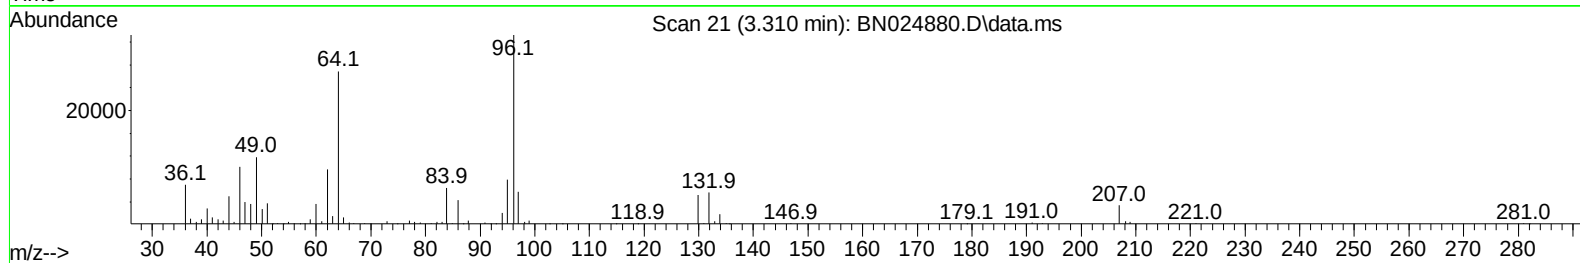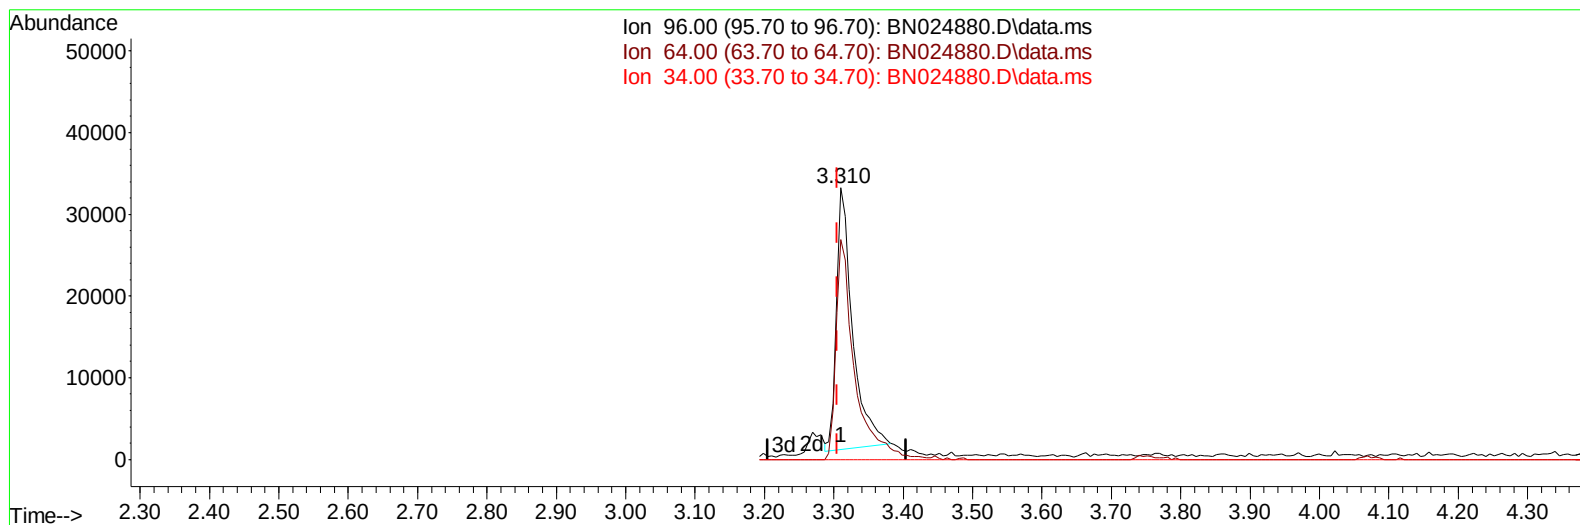

TIC: BN024880.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.310min (+ 0.006) 4.40 ng/uL

response 51725

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	86.20	80.89
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024880.D
 Acq On : 14 Apr 2023 04:18
 Operator : CG/JU
 Sample : 02275-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ1

Manual IntegrationsAPPROVED

Quant Time: Apr 14 04:54:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 14 03:27:44 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/14/2023
 Supervised By :Jagrut Upadhyay 04/14/2023

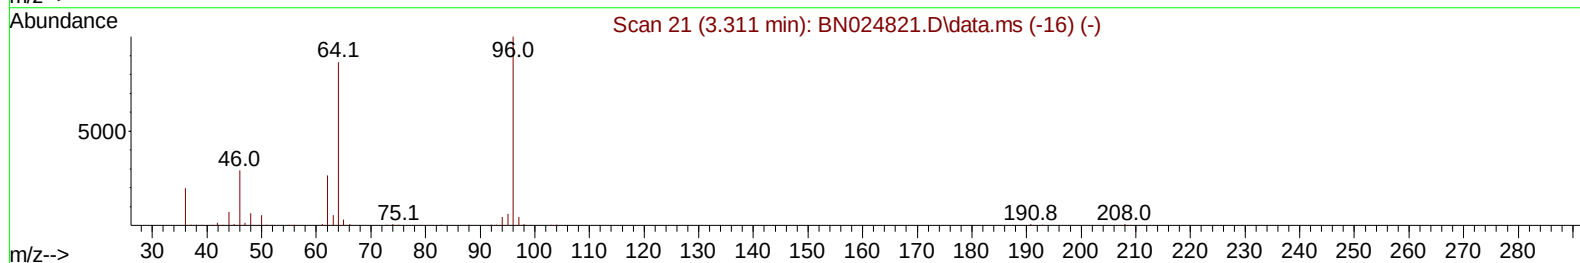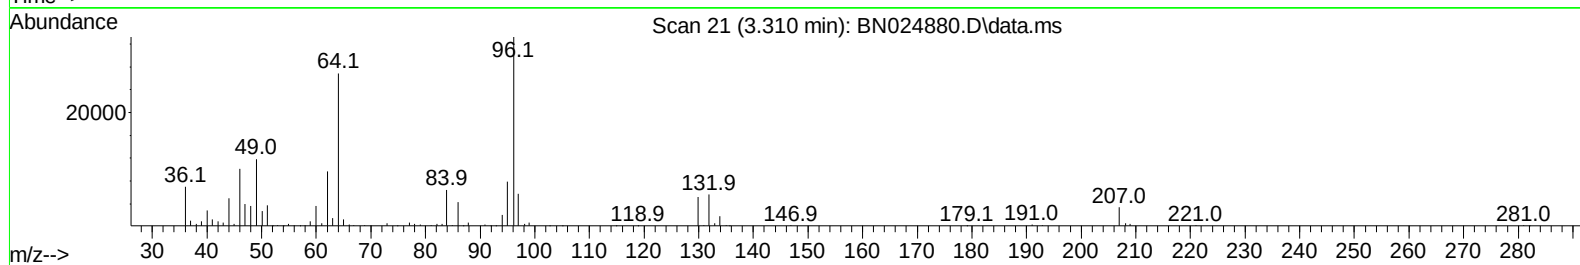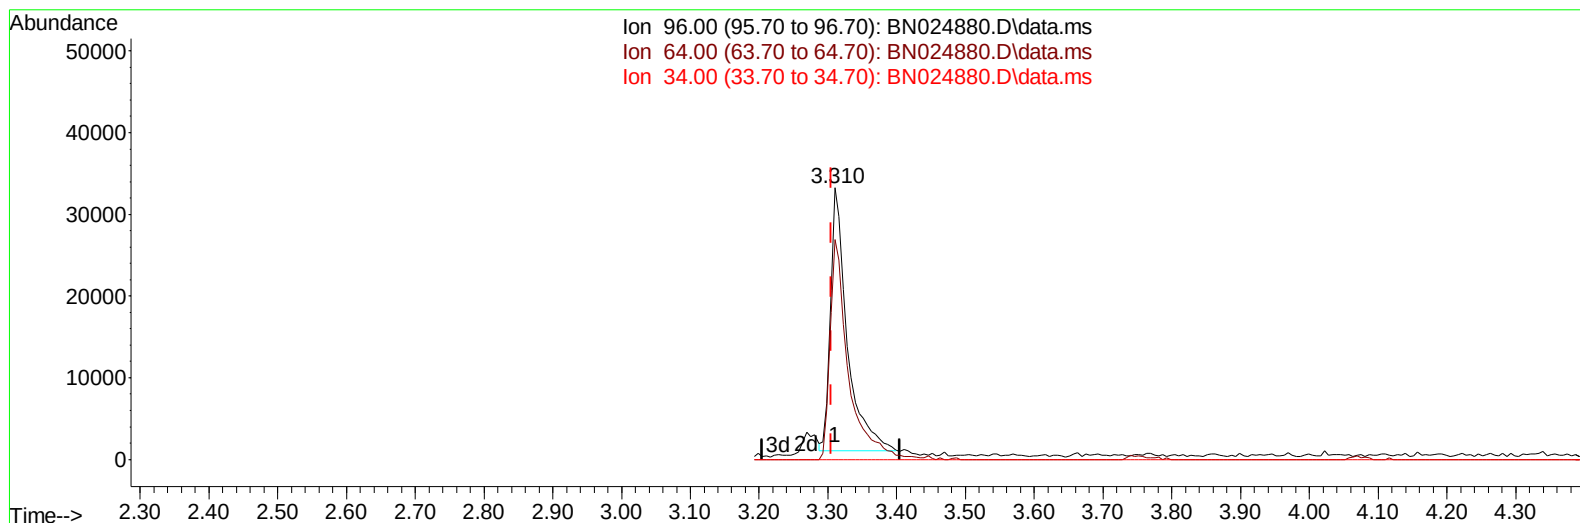

TIC: BN024880.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.310min (+ 0.006) 4.64 ng/uL m

response 54600

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	86.20	80.89
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024880.D
 Acq On : 14 Apr 2023 04:18
 Operator : CG/JU
 Sample : 02275-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ1

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/14/2023
 Supervised By :Jagrut Upadhyay 04/14/2023

Quant Time: Apr 14 04:54:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 14 03:27:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	447630	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136	1937672	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	1200013	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.333	188	2631801	20.000	ng/ul	0.00
79) Chrysene-d12	21.521	240	2533418	20.000	ng/ul	0.00
88) Perylene-d12	23.962	264	2932995	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.310	96	54600m	4.642	ng/uL	0.00
4) Pyridine-d5	3.746	84	304086	8.634	ng/ul	0.01
7) Phenol-d5	7.098	99	326820	7.489	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	1058904	36.277	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	889069	27.721	ng/ul	0.00
15) 4-Methylphenol-d8	8.651	113	595854	17.199	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	562966	35.883	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	628753	36.999	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	988186	32.534	ng/ul	0.00
31) 4-Chloroaniline-d4	10.892	131	1357801	29.456	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	3551216	38.174	ng/ul	0.00
49) Acenaphthylene-d8	14.280	160	4055121	38.039	ng/ul	0.00
54) 4-Nitrophenol-d4	14.780	143	118835	6.232	ng/ul	0.00
60) Fluorene-d10	15.574	176	2994224	38.122	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	575027	33.573	ng/ul	0.00
73) Anthracene-d10	17.433	188	4882132	39.498	ng/ul	0.00
81) Pyrene-d10	19.727	212	5710391	38.817	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.809	264	6201291	40.437	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024880.D
Acq On : 14 Apr 2023 04:18
Operator : CG/JU
Sample : 02275-05
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDZ1

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/14/2023
Supervised By :Jagrut Upadhyay 04/14/2023

Quant Time: Apr 14 04:54:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 14 03:27:44 2023
Response via : Initial Calibration

