




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024911.D
Acq On : 14 Apr 2023 23:58
Operator : CG/JU
Sample : 02252-15
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMF1

Manual IntegrationsAPPROVED

Quant Time: Apr 15 00:37:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

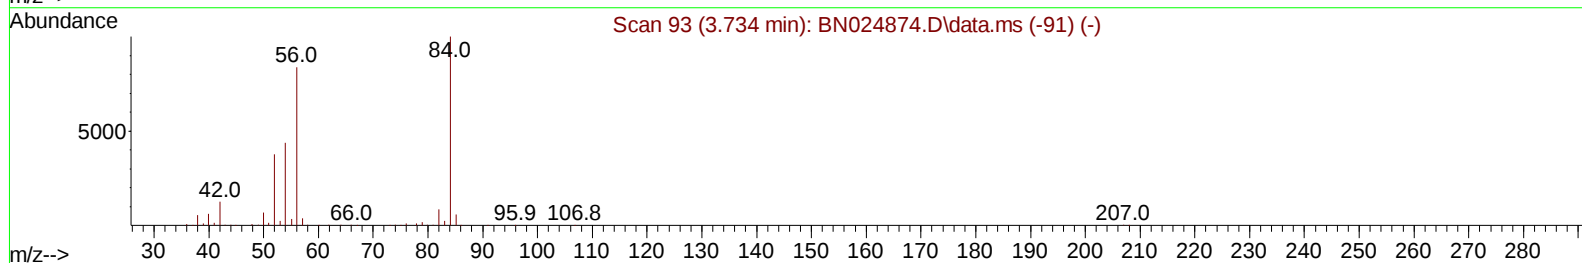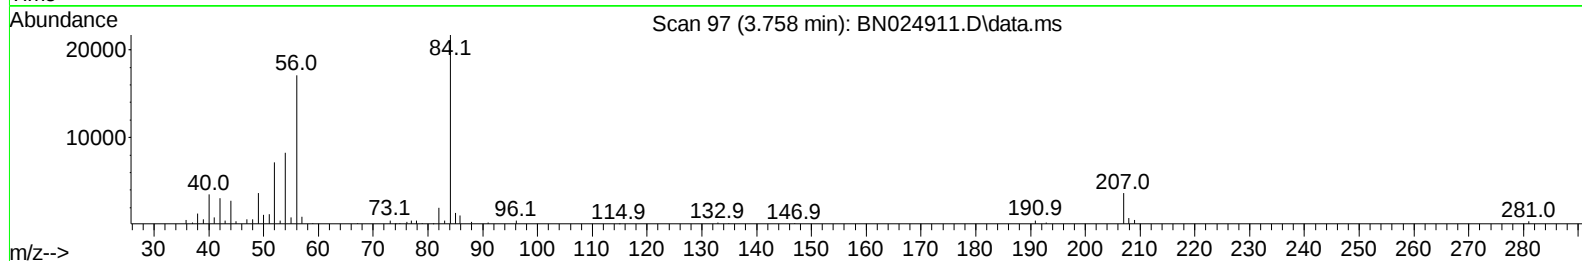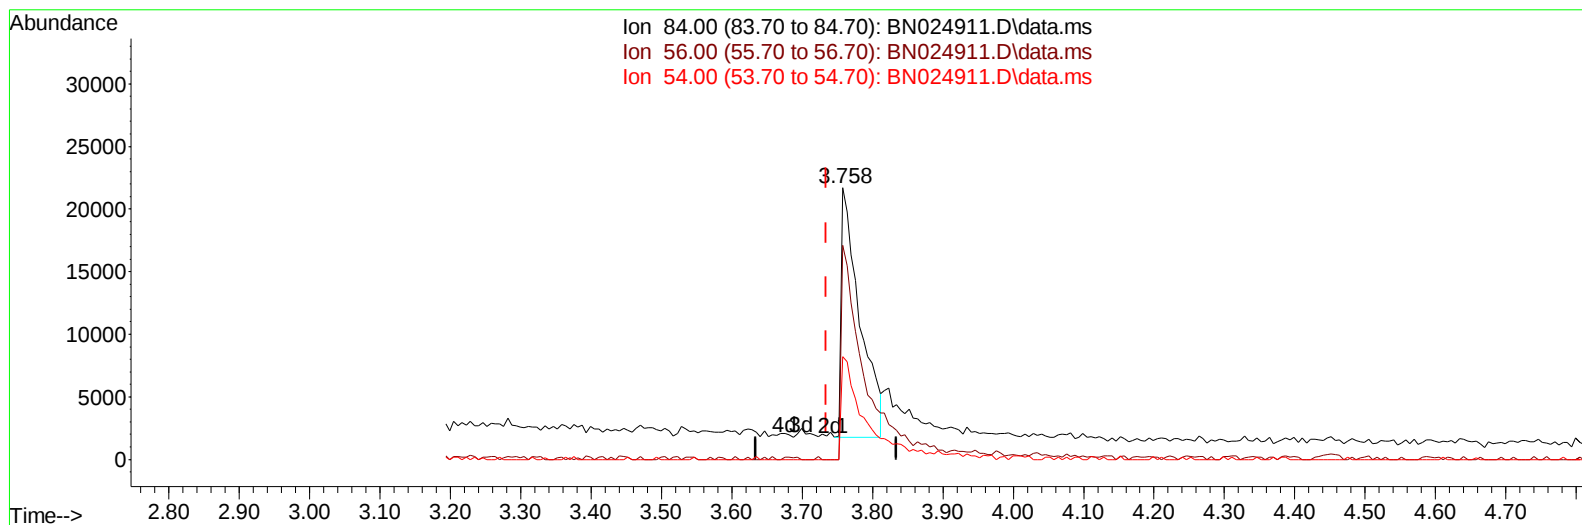

TIC: BN024911.D\data.ms

(4) Pyridine-d5 (S)

3.758min (+ 0.024) 1.58 ng/u1

response 36105

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	82.10	78.86
54.00	40.20	37.96
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024911.D
 Acq On : 14 Apr 2023 23:58
 Operator : CG/JU
 Sample : 02252-15
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMF1

Manual IntegrationsAPPROVED

Quant Time: Apr 15 00:37:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 15 00:01:14 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/17/2023
 Supervised By :Jagrut Upadhyay 04/17/2023

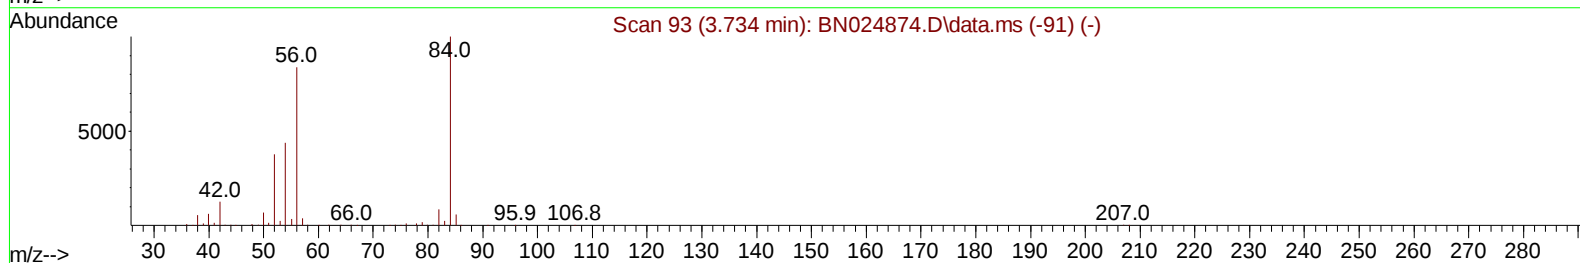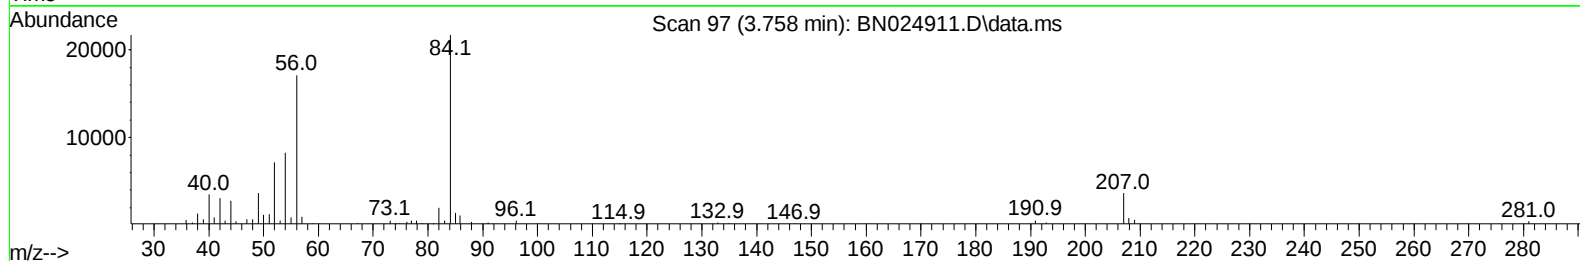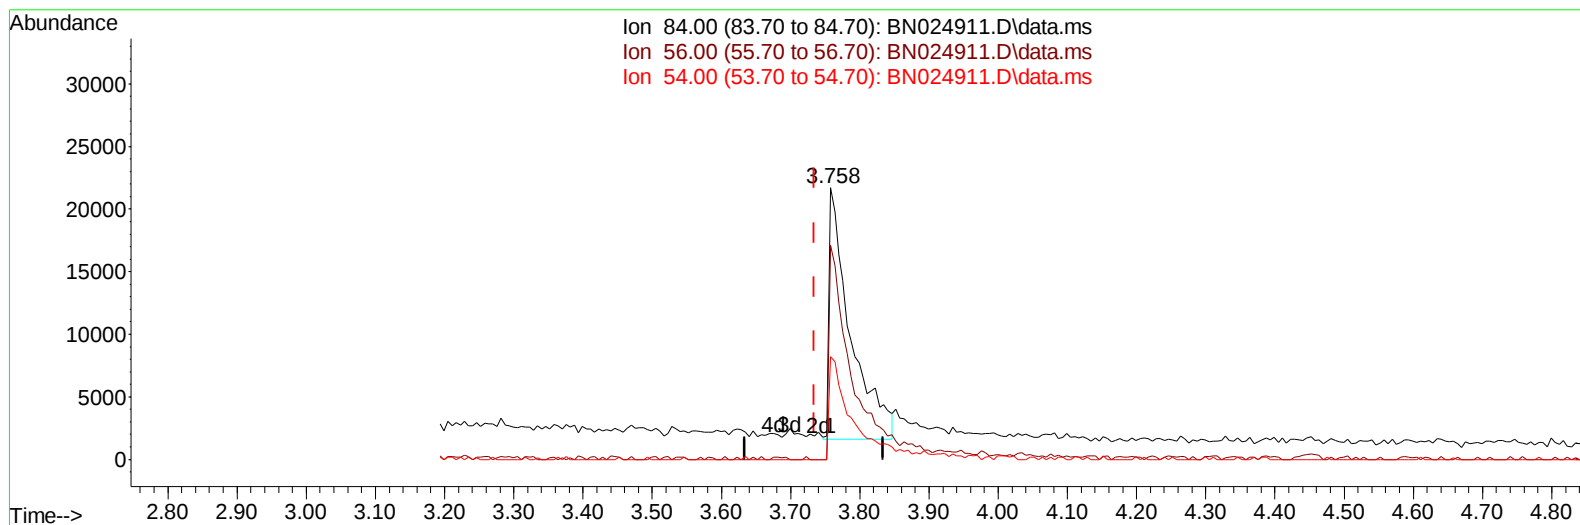

TIC: BN024911.D\data.ms

(4) Pyridine-d5 (S)

3.758min (+ 0.024) 1.88 ng/ul m

response 42842

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	82.10	78.86
54.00	40.20	37.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024911.D
 Acq On : 14 Apr 2023 23:58
 Operator : CG/JU
 Sample : 02252-15
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMF1

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
 Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 00:37:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 15 00:01:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	289612	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	1239812	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	794466	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	1764748	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	1682036	20.000	ng/ul	0.00
88) Perylene-d12	23.963	264	1859814	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	29999	3.942	ng/uL	0.00
4) Pyridine-d5	3.758	84	42842m	1.880	ng/ul	0.02
7) Phenol-d5	7.099	99	131618	4.661	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.264	67	511988	27.110	ng/ul	0.00
11) 2-Chlorophenol-d4	7.464	132	414660	19.984	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	262054	11.691	ng/ul	0.00
21) Nitrobenzene-d5	9.111	128	277724	27.666	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	283883	26.108	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	464101	23.880	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	372764	12.639	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	1772741	28.784	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	1981068	28.070	ng/ul	0.00
54) 4-Nitrophenol-d4	14.781	143	40920	3.241	ng/ul	0.00
60) Fluorene-d10	15.575	176	1573016	30.250	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.693	200	274596	23.909	ng/ul	0.00
73) Anthracene-d10	17.428	188	2686431	32.412	ng/ul	0.00
81) Pyrene-d10	19.722	212	3186790	32.627	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.804	264	3053707	31.403	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024911.D
Acq On : 14 Apr 2023 23:58
Operator : CG/JU
Sample : 02252-15
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMF1

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 00:37:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

