




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024912.D
Acq On : 15 Apr 2023 00:36
Operator : CG/JU
Sample : 02335-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMH0

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 01:31:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

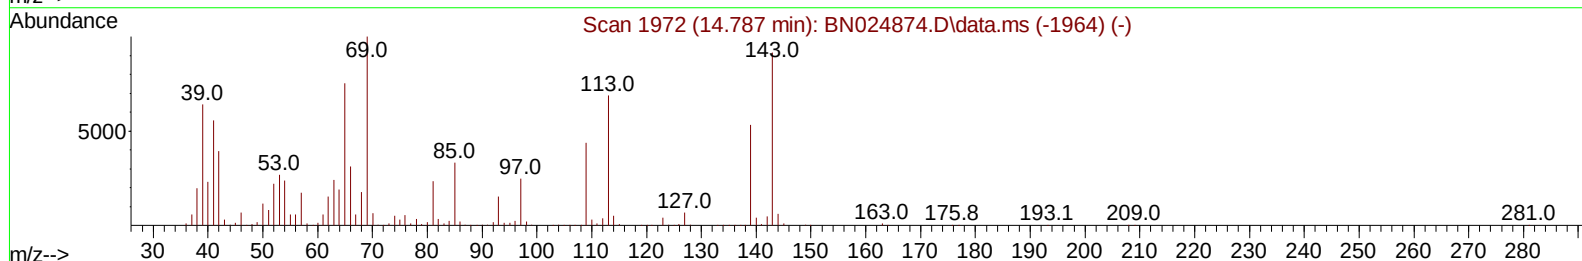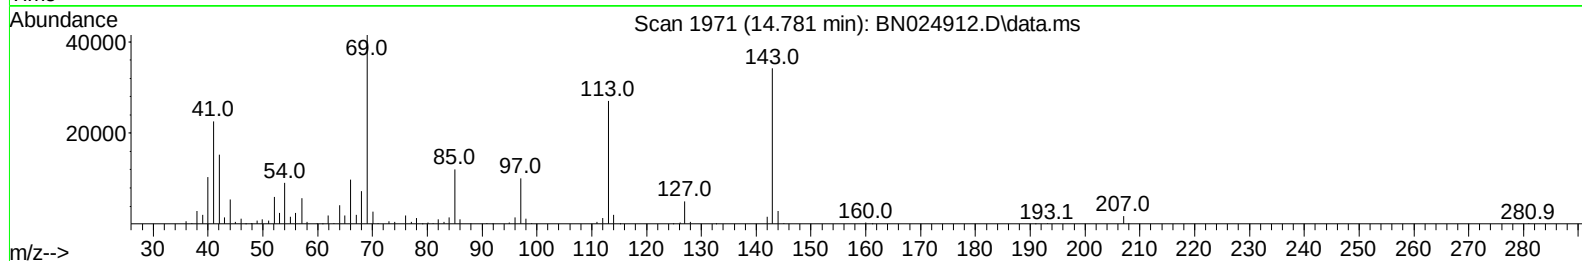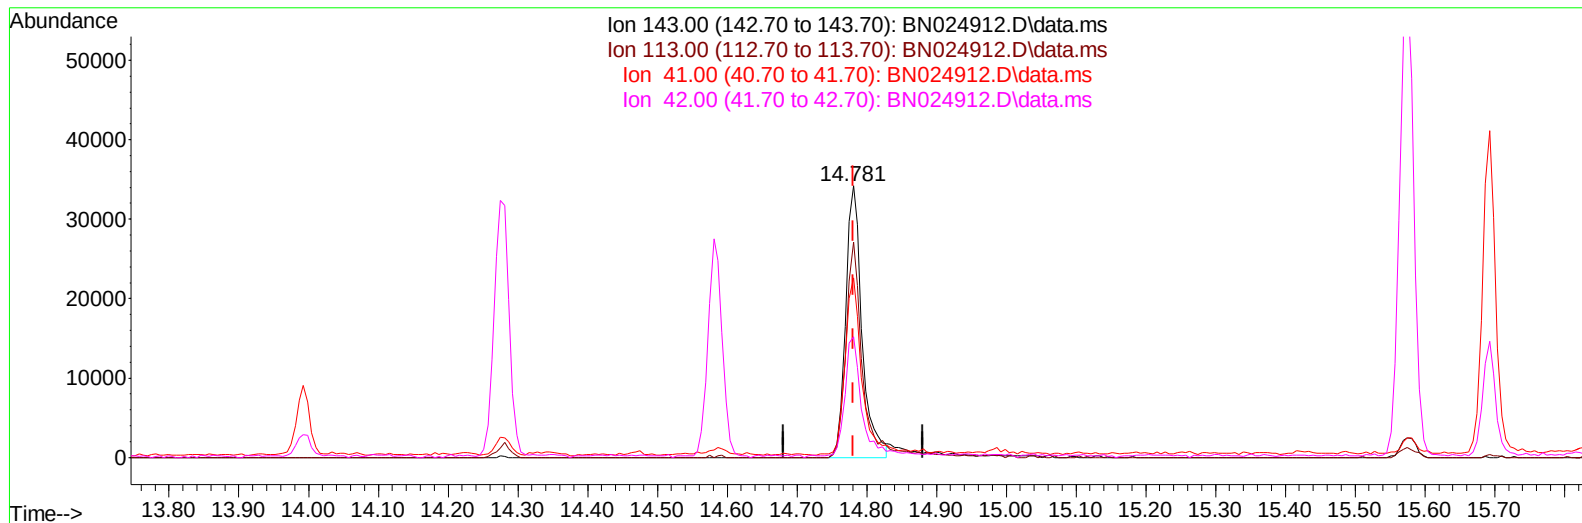

TIC: BN024912.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.781min (-0.000) 4.17 ng/u1

response 55672

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.00	79.27
41.00	60.30	66.09
42.00	40.40	44.56




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024912.D
Acq On : 15 Apr 2023 00:36
Operator : CG/JU
Sample : 02335-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMH0

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 01:31:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

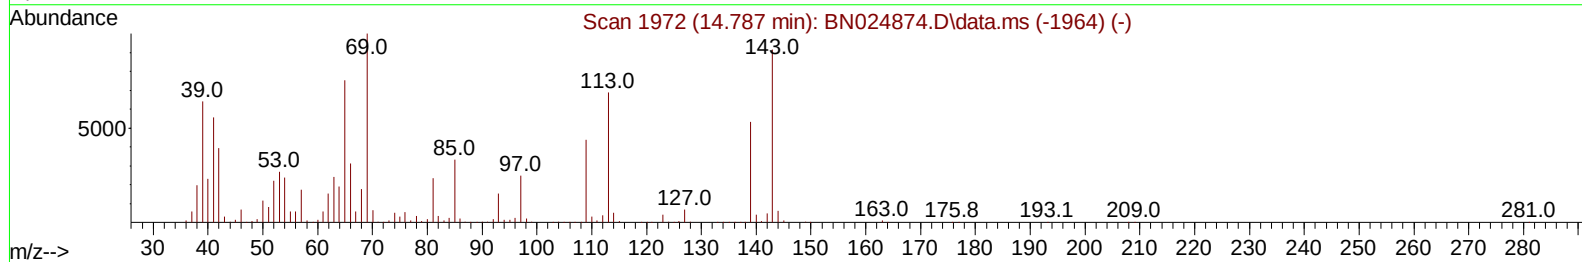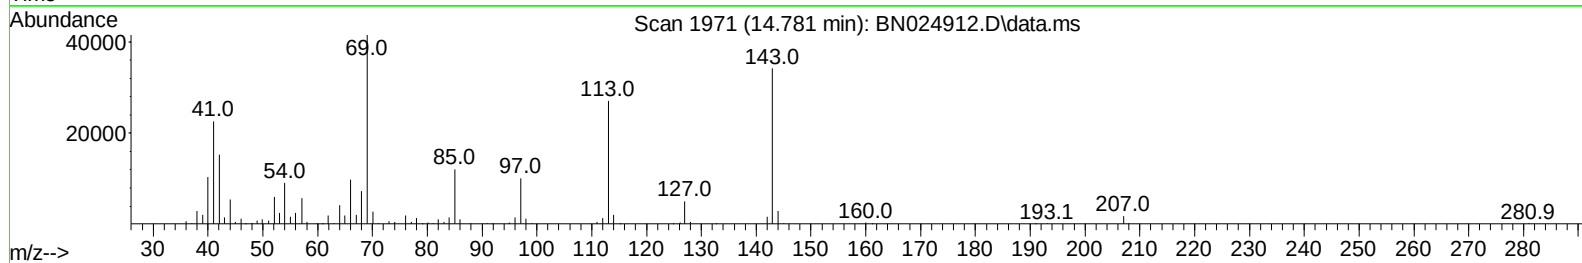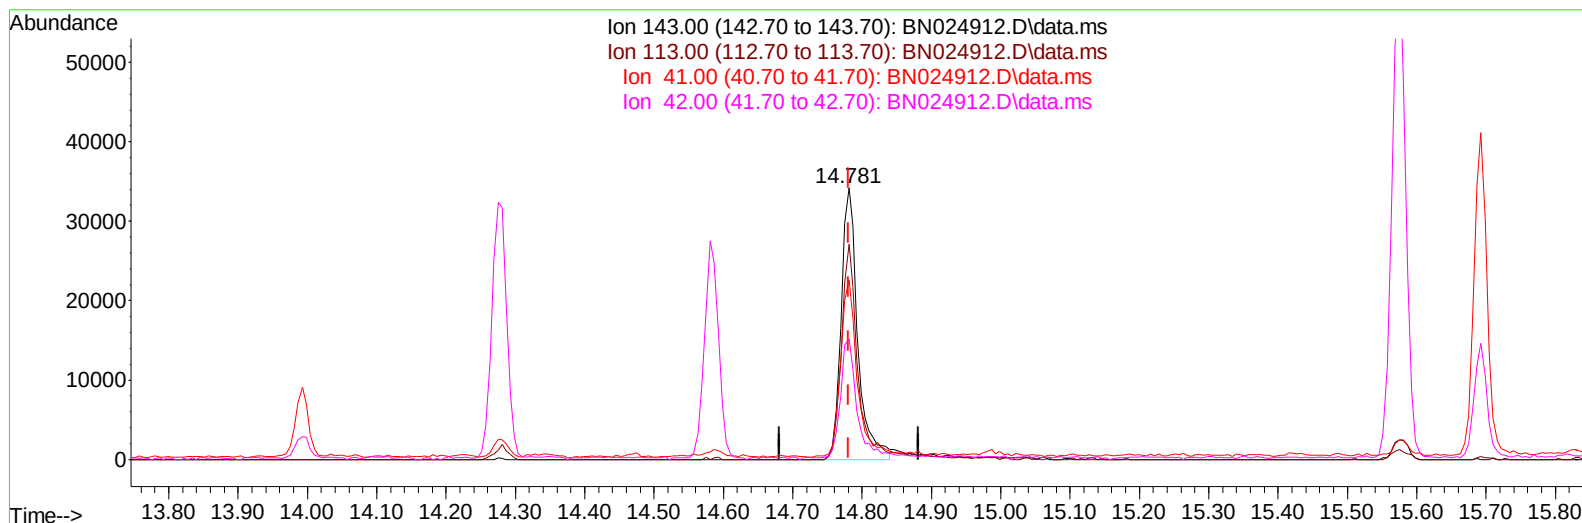

TIC: BN024912.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.781min (-0.000) 4.24 ng/ul m

response 56687

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.00	79.27
41.00	60.30	66.09
42.00	40.40	44.56

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024912.D
 Acq On : 15 Apr 2023 00:36
 Operator : CG/JU
 Sample : 02335-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMH0

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
 Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 01:31:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 15 00:01:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	323750	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	1414585	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	841133	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	1961218	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	1886293	20.000	ng/ul	0.00
88) Perylene-d12	23.957	264	1999780	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	39497	4.643	ng/uL	0.00
4) Pyridine-d5	3.740	84	212078	8.326	ng/ul	0.00
7) Phenol-d5	7.099	99	189300	5.997	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	722525	34.224	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	582032	25.092	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	372553	14.868	ng/ul	0.00
21) Nitrobenzene-d5	9.105	128	397619	34.715	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	416515	33.573	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	660488	29.786	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	879683	26.141	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	2326842	35.684	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	2642526	35.365	ng/ul	0.00
54) 4-Nitrophenol-d4	14.781	143	56687m	4.241	ng/ul	0.00
60) Fluorene-d10	15.575	176	2152633	39.100	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	388291	30.422	ng/ul	0.00
73) Anthracene-d10	17.428	188	3603002	39.116	ng/ul	0.00
81) Pyrene-d10	19.722	212	4219591	38.523	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.816	264	4066372	38.890	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024912.D
Acq On : 15 Apr 2023 00:36
Operator : CG/JU
Sample : 02335-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMH0

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 01:31:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

