




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024913.D
Acq On : 15 Apr 2023 01:13
Operator : CG/JU
Sample : 02335-02
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMH2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 01:42:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

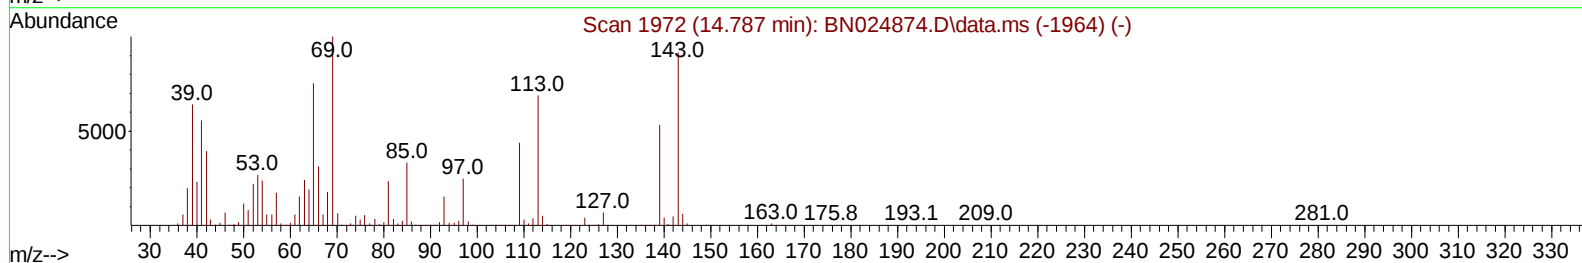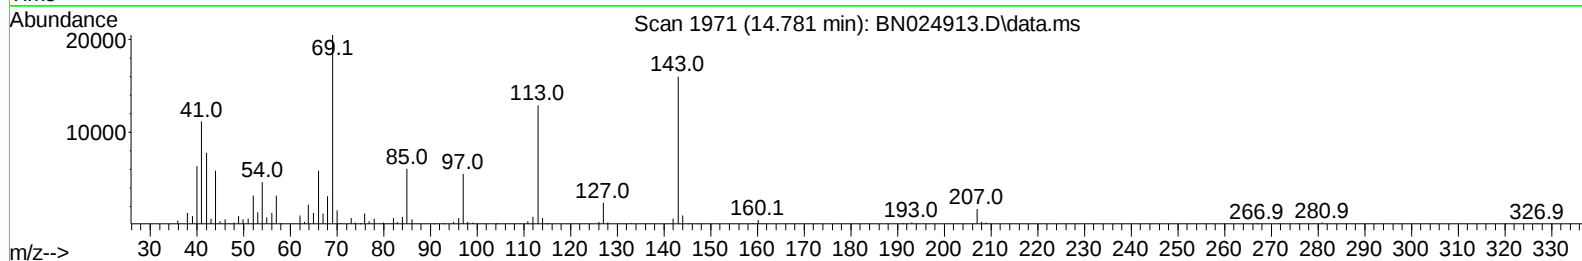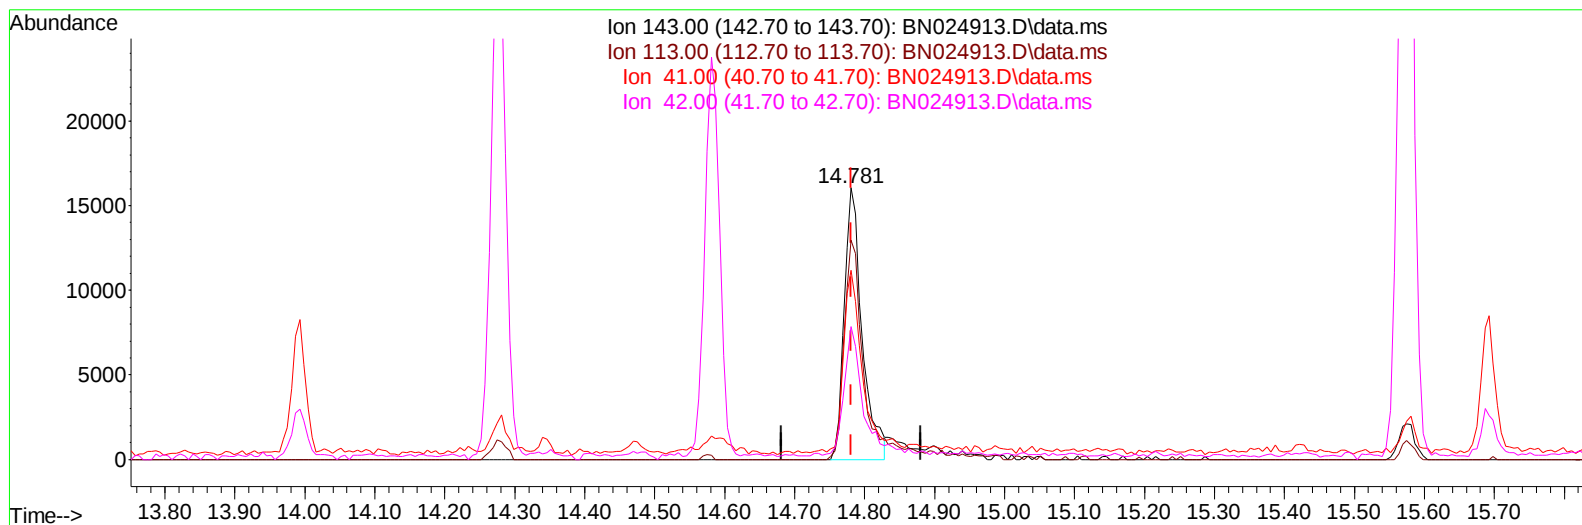

TIC: BN024913.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.781min (-0.000) 2.48 ng/u1

response 28355

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.00	80.66
41.00	60.30	69.61
42.00	40.40	48.90#




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024913.D
Acq On : 15 Apr 2023 01:13
Operator : CG/JU
Sample : 02335-02
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMH2

Manual IntegrationsAPPROVED

Quant Time: Apr 15 01:42:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

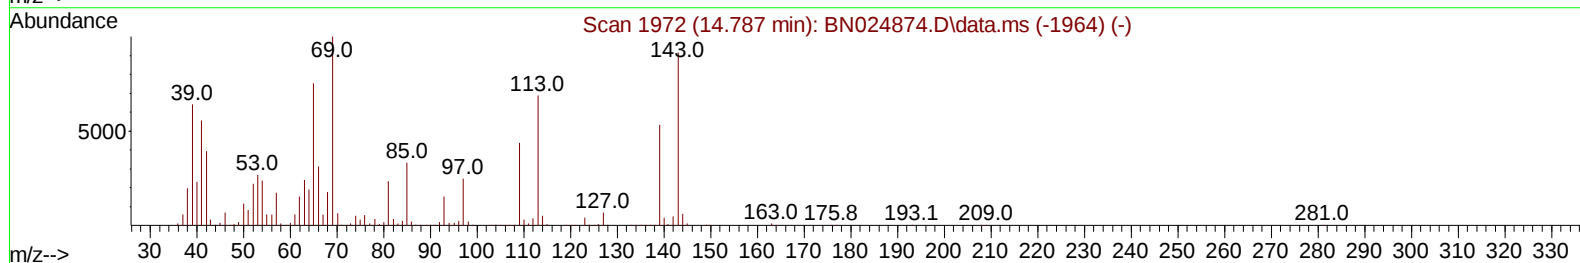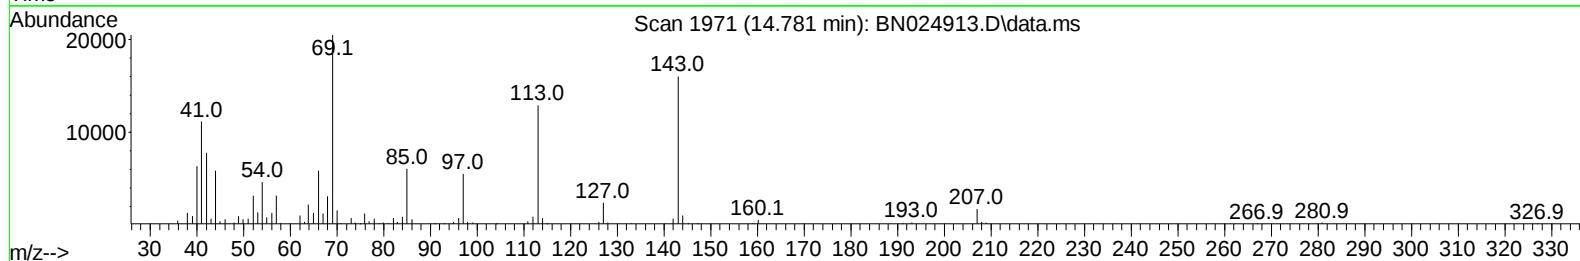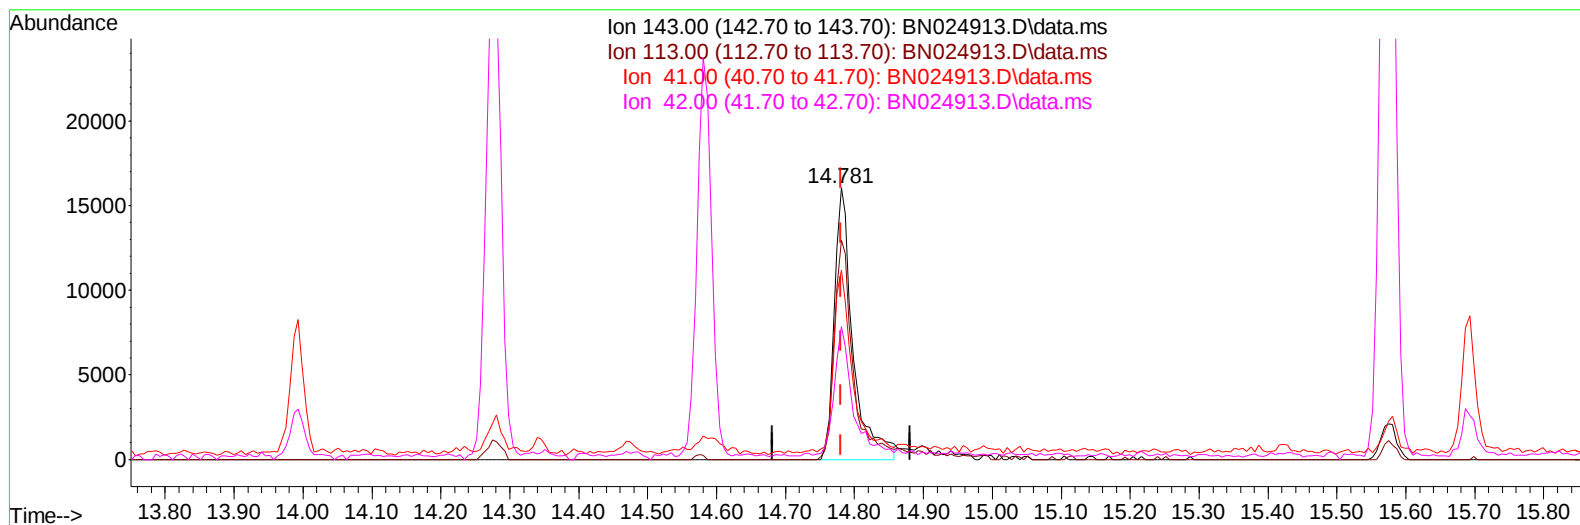

TIC: BN024913.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.781min (-0.000) 2.65 ng/ul m

response 30311

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.00	80.66
41.00	60.30	69.61
42.00	40.40	48.90#

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024913.D
 Acq On : 15 Apr 2023 01:13
 Operator : CG/JU
 Sample : 02335-02
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMH2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
 Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 01:42:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 15 00:01:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	262578	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	1158756	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	719329	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	1566170	20.000	ng/ul	0.00
79) Chrysene-d12	21.522	240	1514235	20.000	ng/ul	0.00
88) Perylene-d12	23.974	264	1695427	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	32319	4.684	ng/uL	0.00
4) Pyridine-d5	3.740	84	233412	11.299	ng/ul	0.00
7) Phenol-d5	7.099	99	155639	6.080	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.264	67	627005	36.619	ng/ul	0.00
11) 2-Chlorophenol-d4	7.464	132	490404	26.067	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	321432	15.816	ng/ul	0.00
21) Nitrobenzene-d5	9.105	128	344704	36.740	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	285349	28.079	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	543546	29.924	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	838810	30.429	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	1973246	35.386	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	2366796	37.038	ng/ul	0.00
54) 4-Nitrophenol-d4	14.781	143	30311m	2.652	ng/ul	0.00
60) Fluorene-d10	15.575	176	1875071	39.826	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.693	200	71867	7.051	ng/ul	0.00
73) Anthracene-d10	17.428	188	3050707	41.474	ng/ul	0.00
81) Pyrene-d10	19.722	212	3547394	40.344	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.816	264	3602663	40.640	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024913.D
Acq On : 15 Apr 2023 01:13
Operator : CG/JU
Sample : 02335-02
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMH2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 01:42:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

