




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024914.D
Acq On : 15 Apr 2023 01:50
Operator : CG/JU
Sample : 02335-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMH9

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 02:28:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

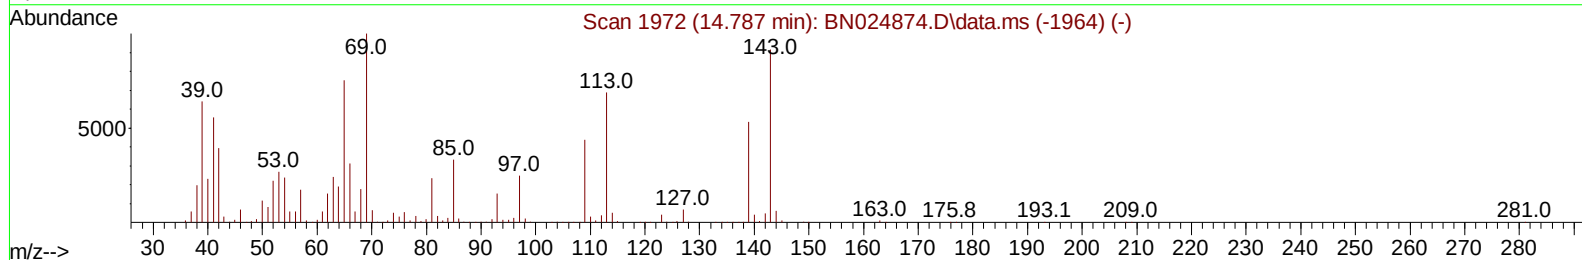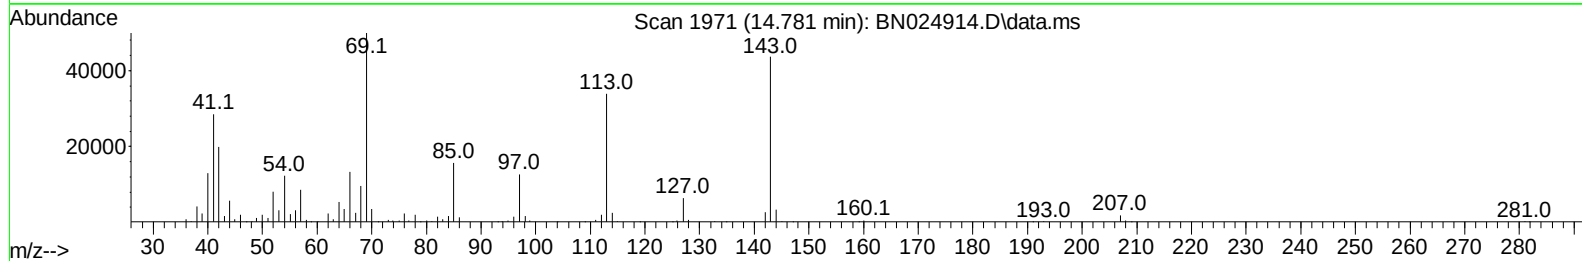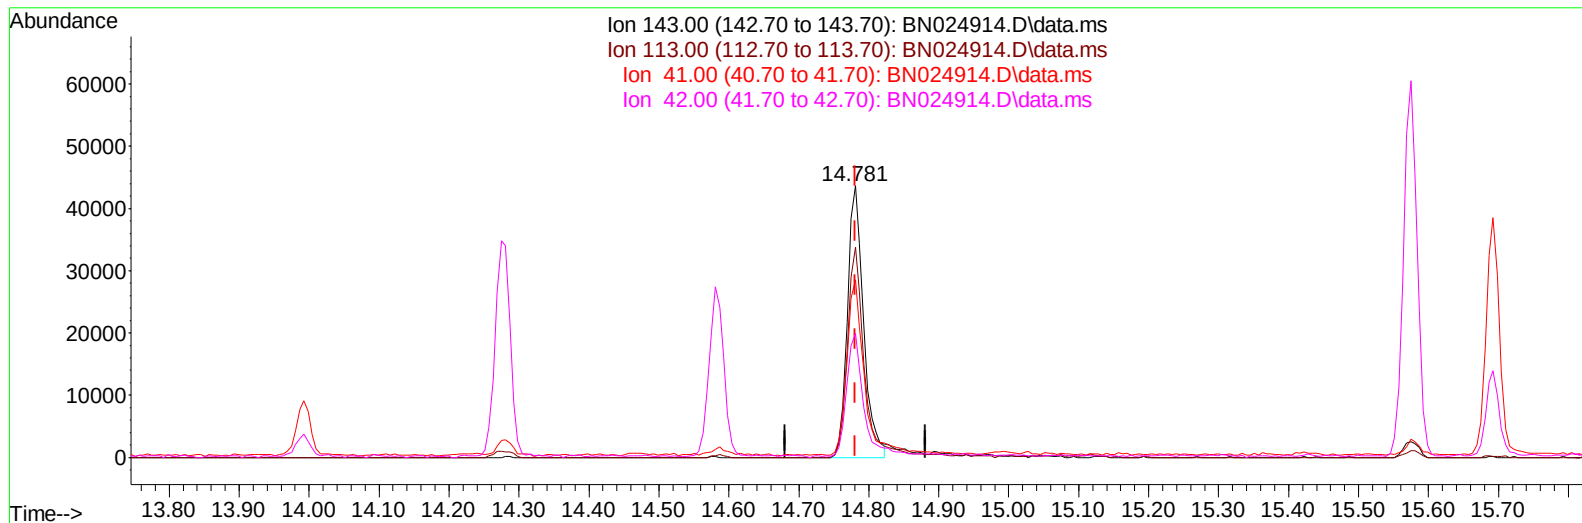

TIC: BN024914.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.781min (-0.000) 5.34 ng/u1

response 69237

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.00	77.55
41.00	60.30	65.34
42.00	40.40	45.74




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024914.D
Acq On : 15 Apr 2023 01:50
Operator : CG/JU
Sample : 02335-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMH9

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 02:28:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

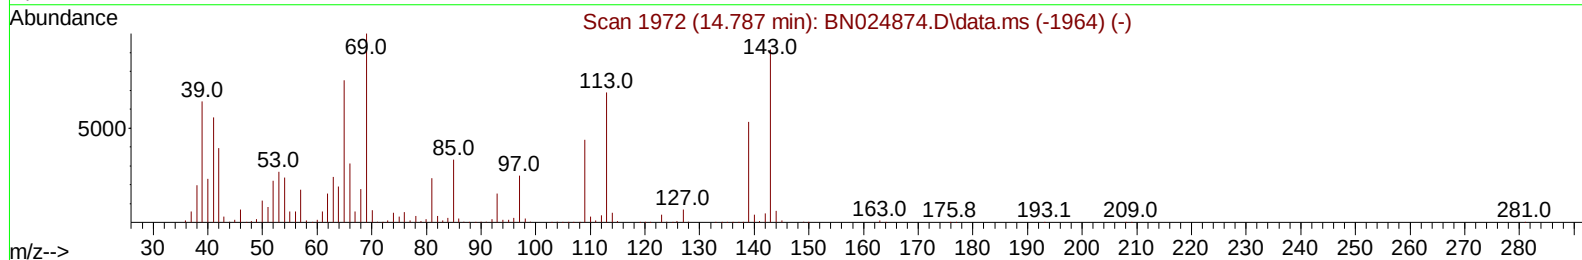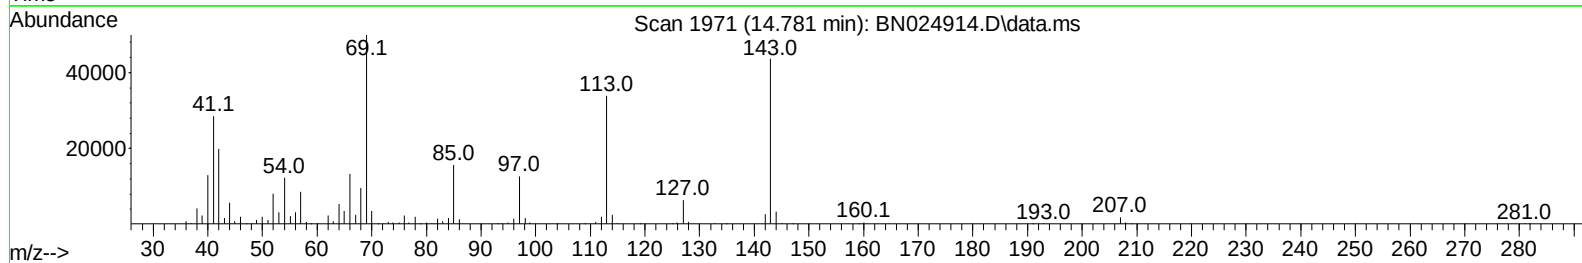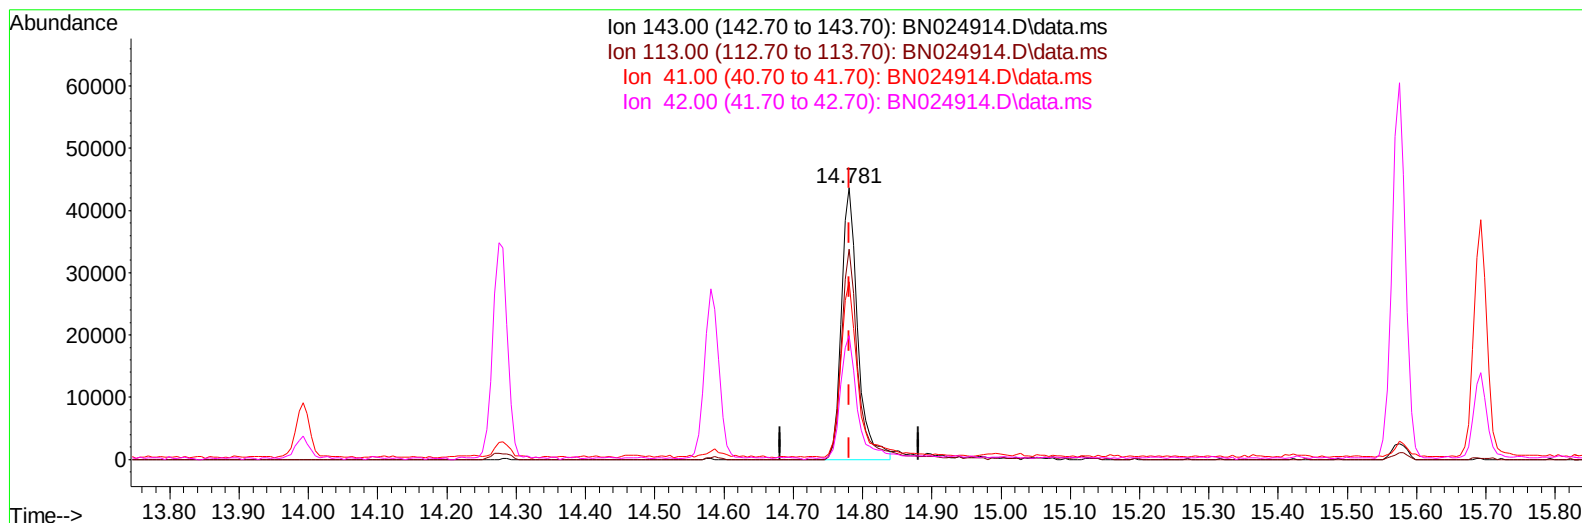

TIC: BN024914.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.781min (-0.000) 5.48 ng/ul m

response 71011

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.00	77.55
41.00	60.30	65.34
42.00	40.40	45.74

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024914.D
 Acq On : 15 Apr 2023 01:50
 Operator : CG/JU
 Sample : 02335-03
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMH9

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
 Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 02:28:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 15 00:01:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	294848	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	1313753	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	816016	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	1803409	20.000	ng/ul	0.00
79) Chrysene-d12	21.522	240	1736445	20.000	ng/ul	0.00
88) Perylene-d12	23.974	264	1893542	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	41887	5.407	ng/uL	0.00
4) Pyridine-d5	3.740	84	175108	7.549	ng/ul	0.00
7) Phenol-d5	7.099	99	219731	7.644	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	692479	36.016	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	597624	28.290	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	402319	17.630	ng/ul	0.00
21) Nitrobenzene-d5	9.105	128	370184	34.801	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	404985	35.149	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	663021	32.195	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	760537	24.335	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	2322861	36.720	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	2666565	36.785	ng/ul	0.00
54) 4-Nitrophenol-d4	14.781	143	71011m	5.476	ng/ul	0.00
60) Fluorene-d10	15.575	176	2074682	38.844	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	370780	31.592	ng/ul	0.00
73) Anthracene-d10	17.428	188	3432749	40.529	ng/ul	0.00
81) Pyrene-d10	19.728	212	3991320	39.584	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.827	264	3984057	40.240	ng/ul	0.03

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024914.D
Acq On : 15 Apr 2023 01:50
Operator : CG/JU
Sample : 02335-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMH9

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 02:28:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

