

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024921.D
 Acq On : 15 Apr 2023 06:08
 Operator : CG/JU
 Sample : PB152117BL
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK117


Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
 Supervised By :Jagrut Upadhyay 04/17/2023


04/17/2023
 Supervised By :Jagrut
 Upadhyay

Quant Time: Apr 15 06:39:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 15 00:01:14 2023
 Response via : Initial Calibration


Ion 84.00 (83.70 to 84.70): BN024921.D\data.ms
 Ion 56.00 (55.70 to 56.70): BN024921.D\data.ms
 Ion 54.00 (53.70 to 54.70): BN024921.D\data.ms

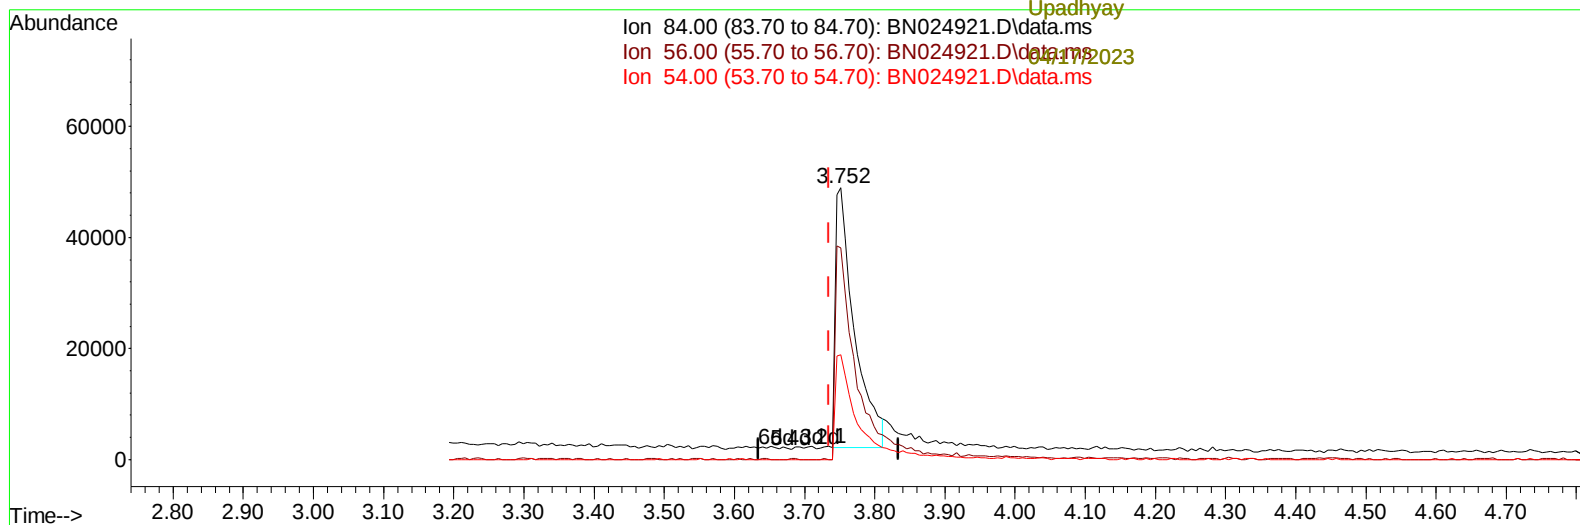

Scan 96 (3.752 min): BN024921.D\data.ms

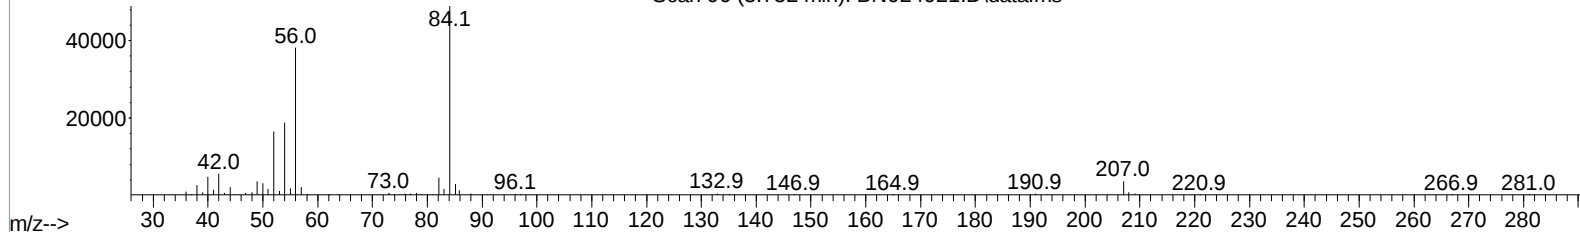

Scan 93 (3.734 min): BN024874.D\data.ms (-91) (-)

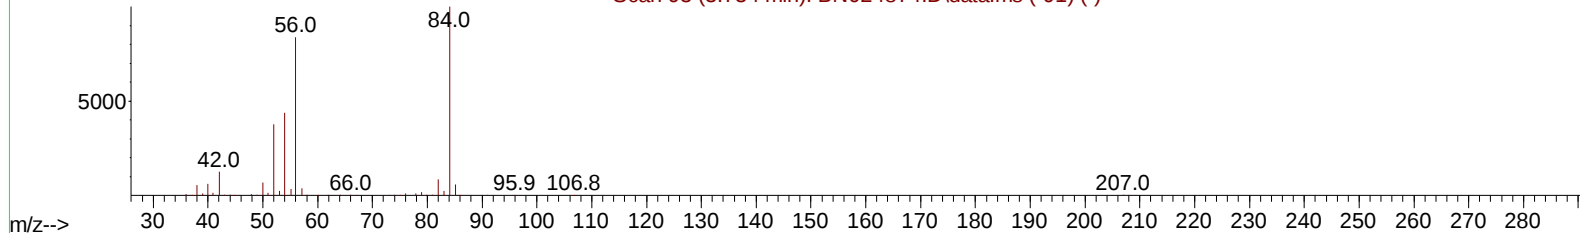

TIC: BN024921.D\data.ms

(4) Pyridine-d5 (S)

3.752min (+ 0.017) 3.69 ng/u1

response 87222

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	82.10	77.95
54.00	40.20	38.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024921.D
 Acq On : 15 Apr 2023 06:08
 Operator : CG/JU
 Sample : PB152117BL
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK117


Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
 Supervised By :Jagrut Upadhyay 04/17/2023


04/17/2023
 Supervised By :Jagrut
 Upadhyay

Quant Time: Apr 15 06:39:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 15 00:01:14 2023
 Response via : Initial Calibration


Ion 84.00 (83.70 to 84.70): BN024921.D\data.ms
 Ion 56.00 (55.70 to 56.70): BN024921.D\data.ms
 Ion 54.00 (53.70 to 54.70): BN024921.D\data.ms

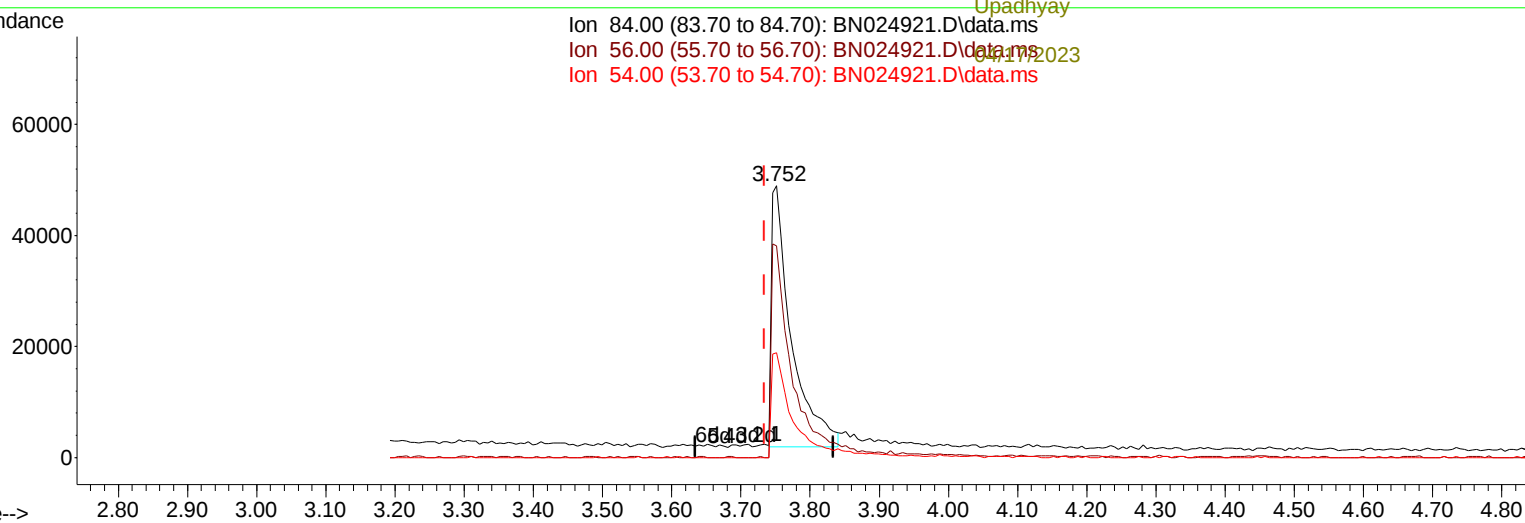

Scan 96 (3.752 min): BN024921.D\data.ms

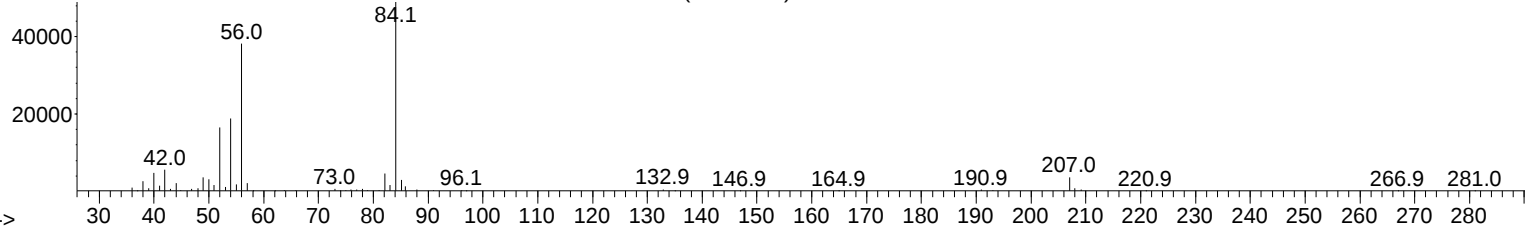

Scan 93 (3.734 min): BN024874.D\data.ms (-91) (-)

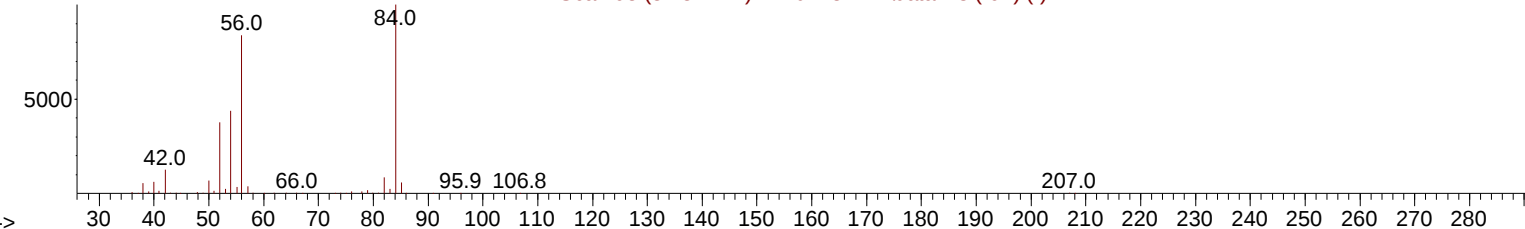

TIC: BN024921.D\data.ms

(4) Pyridine-d5 (S)

3.752min (+ 0.017) 3.99 ng/ul m

response 94244

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	82.10	77.95
54.00	40.20	38.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024921.D
Acq On : 15 Apr 2023 06:08
Operator : CG/JU
Sample : PB152117BL
Misc :
ALS Vial : 68 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
SBLK117

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 06:39:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

04/17/2023
Supervised By :Jagrut
Upadhyay

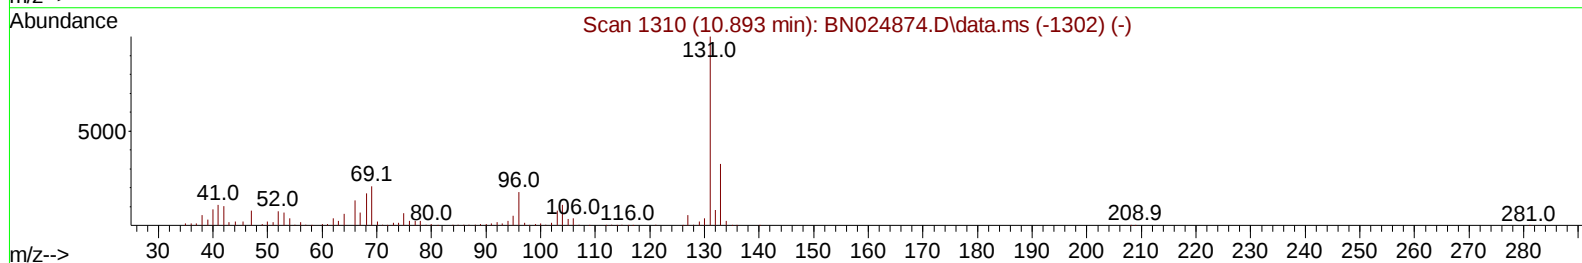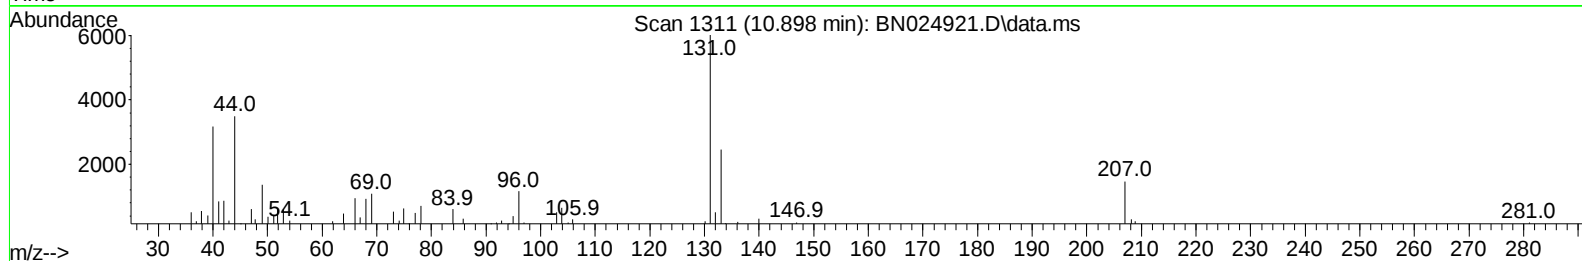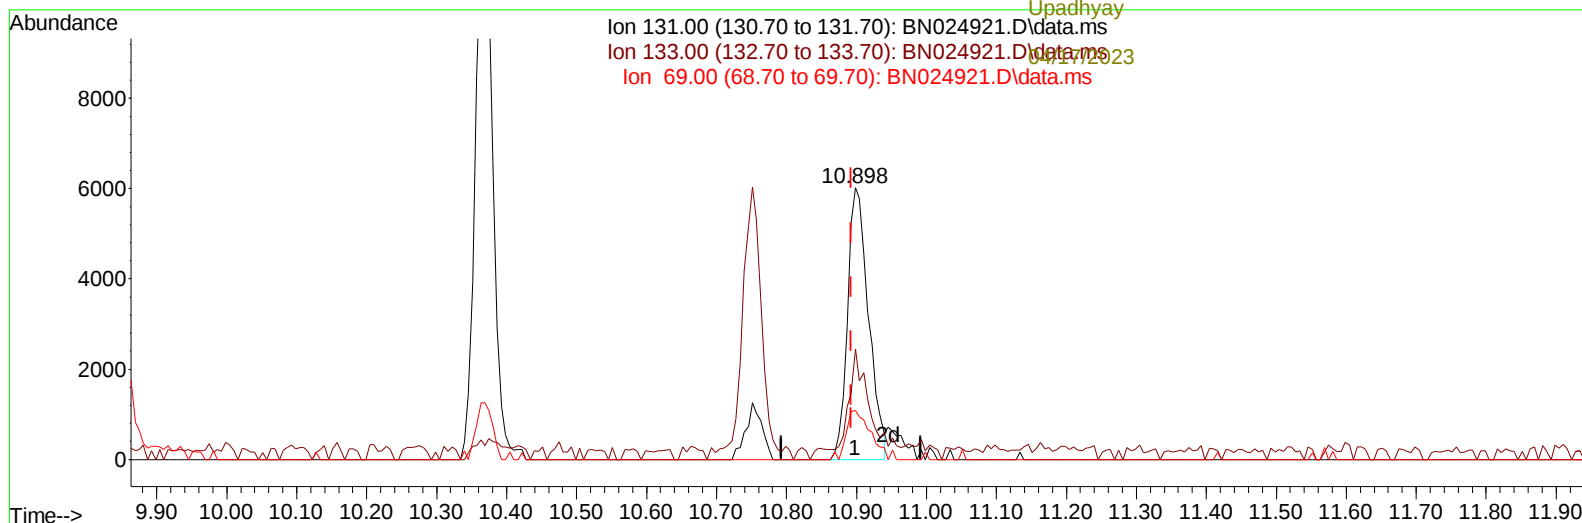

TIC: BN024921.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.898min (+ 0.006) 0.40 ng/u1

response 12492

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.00	40.78#
69.00	19.40	18.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024921.D
Acq On : 15 Apr 2023 06:08
Operator : CG/JU
Sample : PB152117BL
Misc :
ALS Vial : 68 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
SBLK117

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 06:39:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 15 00:01:14 2023
Response via : Initial Calibration

04/17/2023
Supervised By :Jagrut
Upadhyay

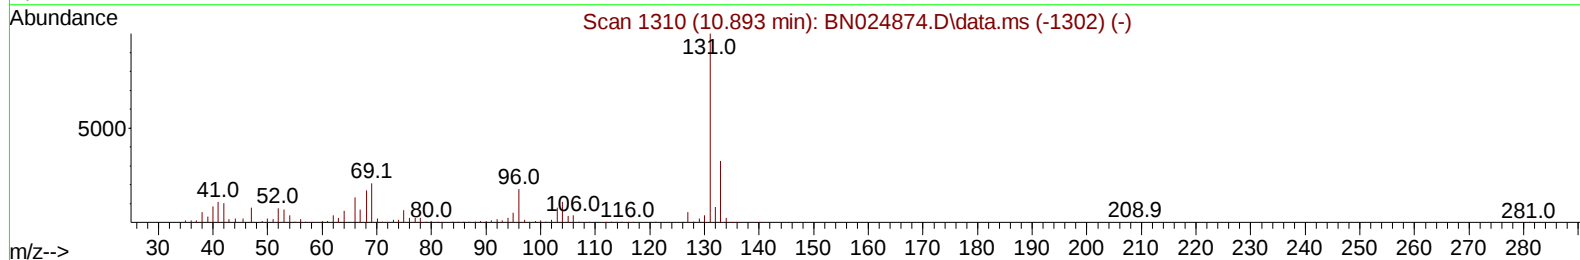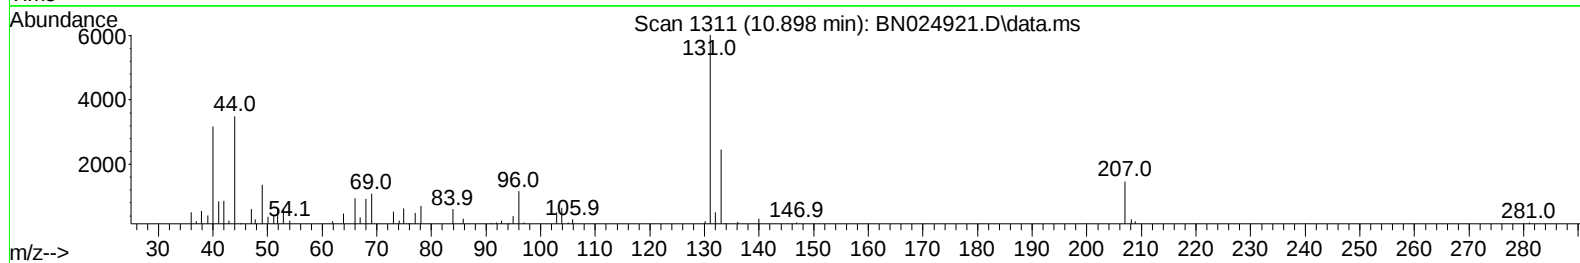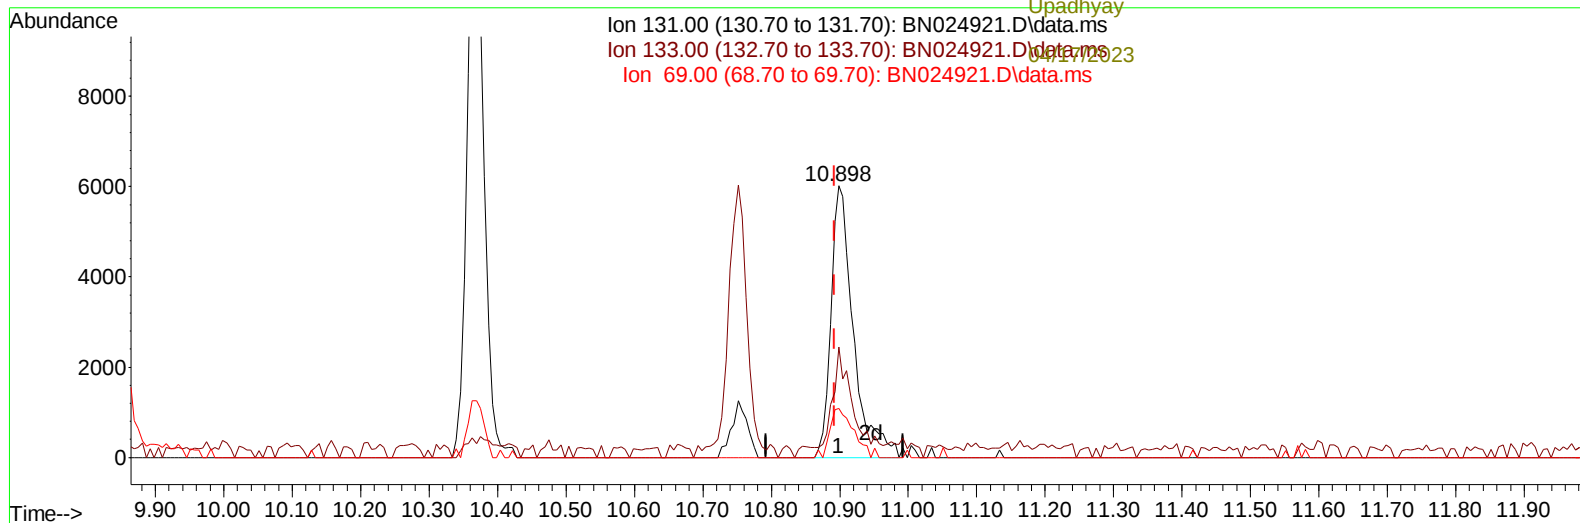

TIC: BN024921.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.898min (+ 0.006) 0.44 ng/ul m

response 13652

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.00	40.78#
69.00	19.40	18.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024921.D
 Acq On : 15 Apr 2023 06:08
 Operator : CG/JU
 Sample : PB152117BL
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK117

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
 Supervised By :Jagrut Upadhyay 04/17/2023

Quant Time: Apr 15 06:39:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 15 00:01:14 2023
 Response via : Initial Calibration

04/17/2023
 Supervised By :Jagrut
 Upadhyay

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----04/17/2023							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.934	152		300374	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136		1316187	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164		765435	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.327	188		1667233	20.000	ng/ul	0.00
79) Chrysene-d12	21.515	240		1677700	20.000	ng/ul	0.00
88) Perylene-d12	23.968	264		1776059	20.000	ng/ul	0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.305	96		52003	6.589	ng/uL	0.00
4) Pyridine-d5	3.752	84		94244m	3.988	ng/ul	0.02
7) Phenol-d5	7.099	99		771022	26.328	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67		637174	32.530	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132		690587	32.089	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113		599642	25.793	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128		349242	32.771	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143		380732	32.983	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165		642770	31.154	ng/ul	0.00
31) 4-Chloroaniline-d4	10.898	131		13652m	0.436	ng/ul	0.00
46) Dimethylphthalate-d6	13.992	166		2057997	34.683	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160		1941094	28.547	ng/ul	0.00
54) 4-Nitrophenol-d4	14.781	143		354680	29.159	ng/ul	0.00
60) Fluorene-d10	15.575	176		1678486	33.503	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200		309938	28.565	ng/ul	0.00
73) Anthracene-d10	17.427	188		2603020	33.243	ng/ul	0.00
81) Pyrene-d10	19.721	212		3180734	32.649	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.810	264		2718095	29.270	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024921.D
Acq On : 15 Apr 2023 06:08
Operator : CG/JU
Sample : PB152117BL
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK117

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

04/17/2023
Supervised By :Jagrut
Upadhyay

04/17/2023

