




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024926.D
Acq On : 15 Apr 2023 09:47
Operator : CG/JU
Sample : PB152052TB 10X
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB052

Manual IntegrationsAPPROVED

Quant Time: Apr 25 08:52:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 25 08:52:18 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/26/2023
Supervised By :Jagrut Upadhyay 04/26/2023

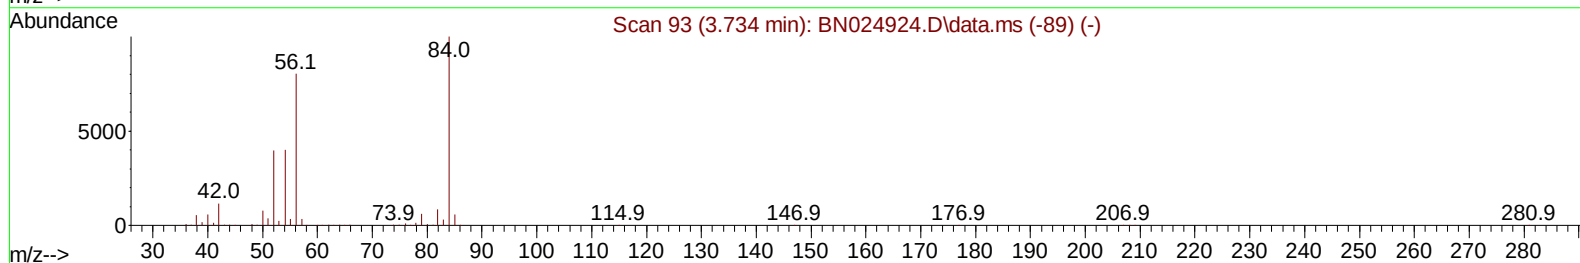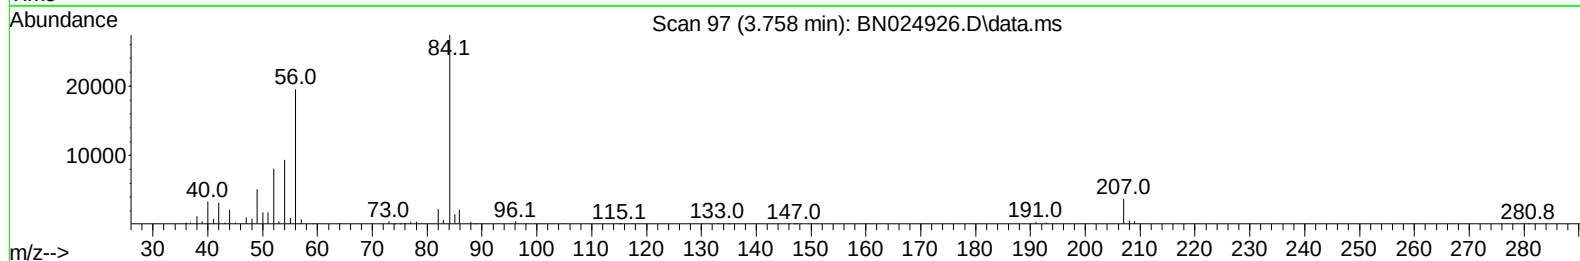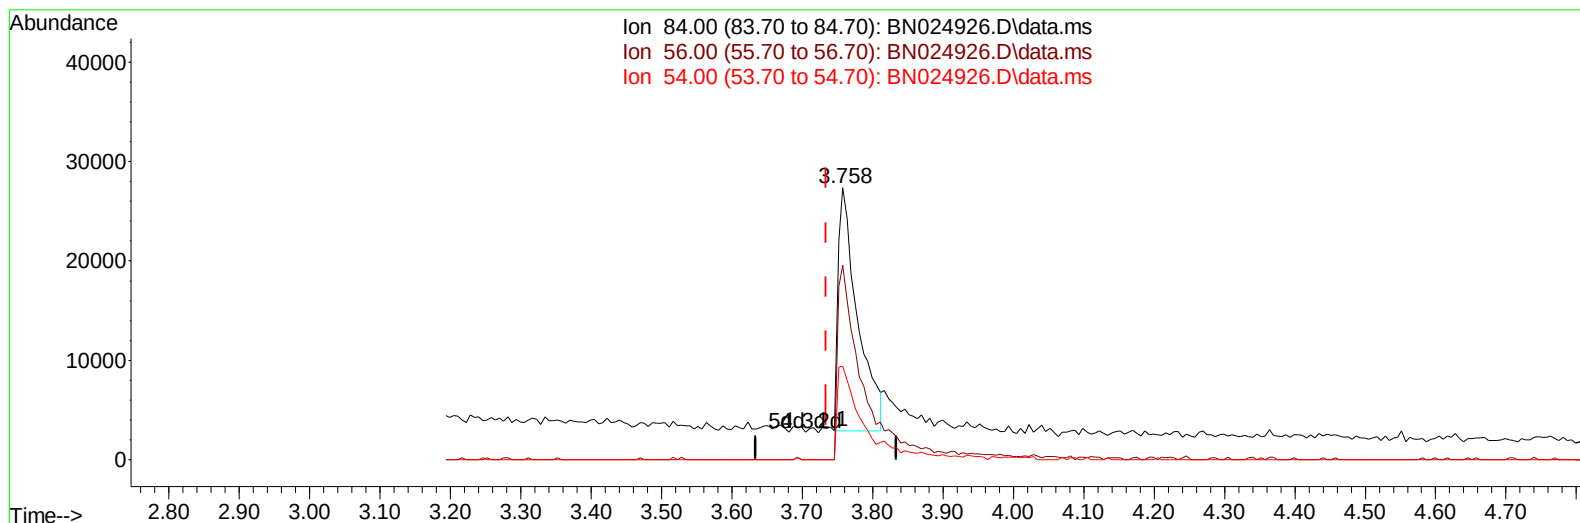

TIC: BN024926.D\data.ms

(4) Pyridine-d5 (S)

3.758min (+ 0.023) 2.07 ng/u1

response 46742

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	82.10	71.52
54.00	40.20	34.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024926.D
 Acq On : 15 Apr 2023 09:47
 Operator : CG/JU
 Sample : PB152052TB 10X
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB052

Manual IntegrationsAPPROVED

Quant Time: Apr 17 03:01:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 17 02:58:51 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/26/2023
 Supervised By :Jagrut Upadhyay 04/26/2023

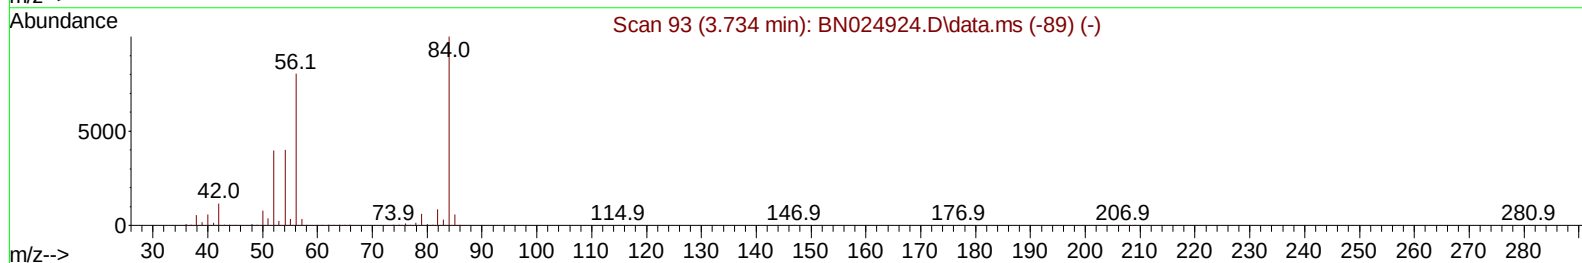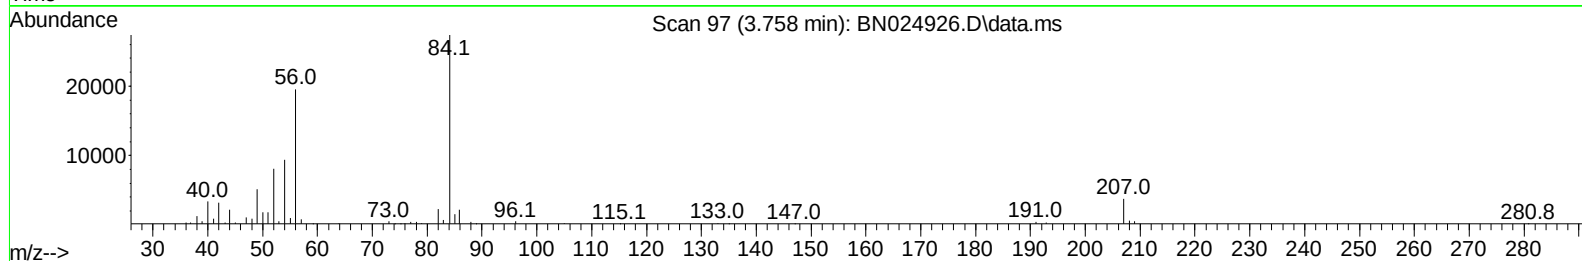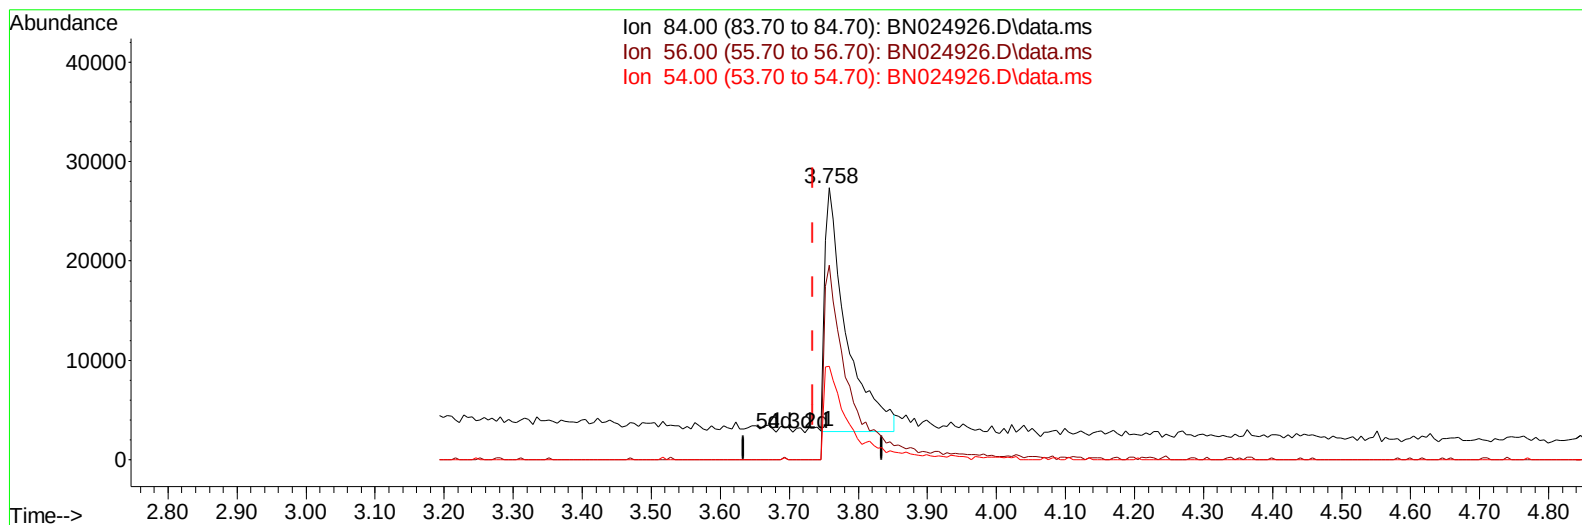

TIC: BN024926.D\data.ms

(4) Pyridine-d5 (S)

3.758min (+ 0.023) 2.37 ng/ul m

response 53502

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	82.10	71.52
54.00	40.20	34.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024926.D
Acq On : 15 Apr 2023 09:47
Operator : CG/JU
Sample : PB152052TB 10X
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB052

Manual IntegrationsAPPROVED

Quant Time: Apr 25 08:52:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 25 08:52:18 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/26/2023
Supervised By :Jagrut Upadhyay 04/26/2023

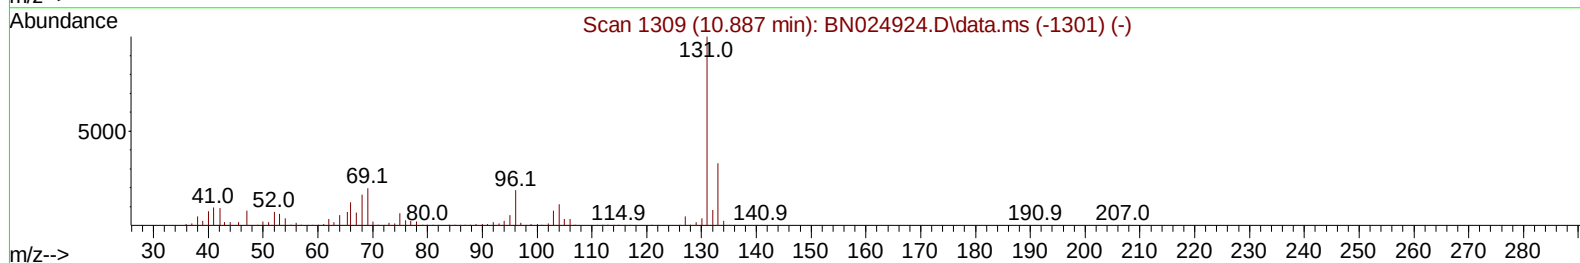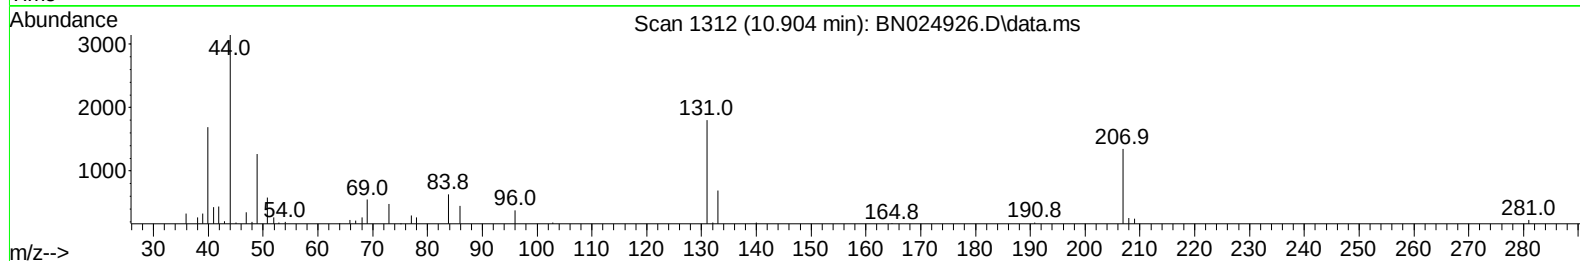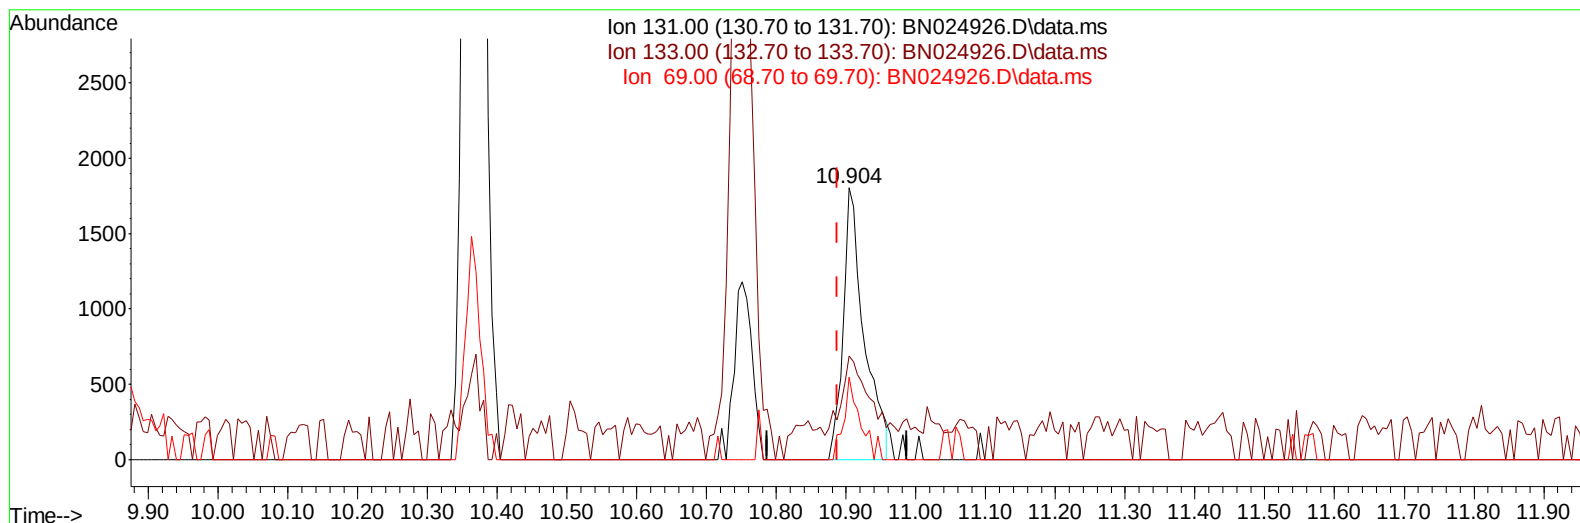

TIC: BN024926.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.904min (+ 0.018) 0.12 ng/ul

response 3757

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.00	38.16
69.00	19.40	30.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024926.D
Acq On : 15 Apr 2023 09:47
Operator : CG/JU
Sample : PB152052TB 10X
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB052

Manual IntegrationsAPPROVED

Quant Time: Apr 17 03:01:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 17 02:58:51 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/26/2023
Supervised By :Jagrut Upadhyay 04/26/2023

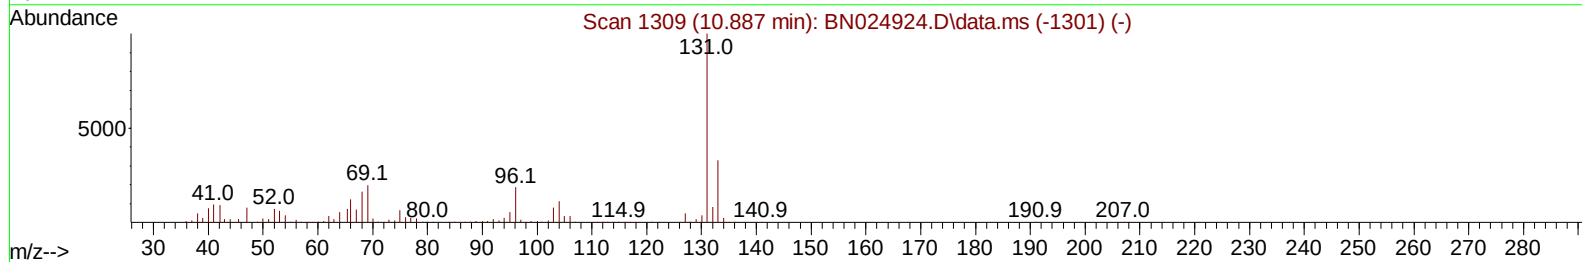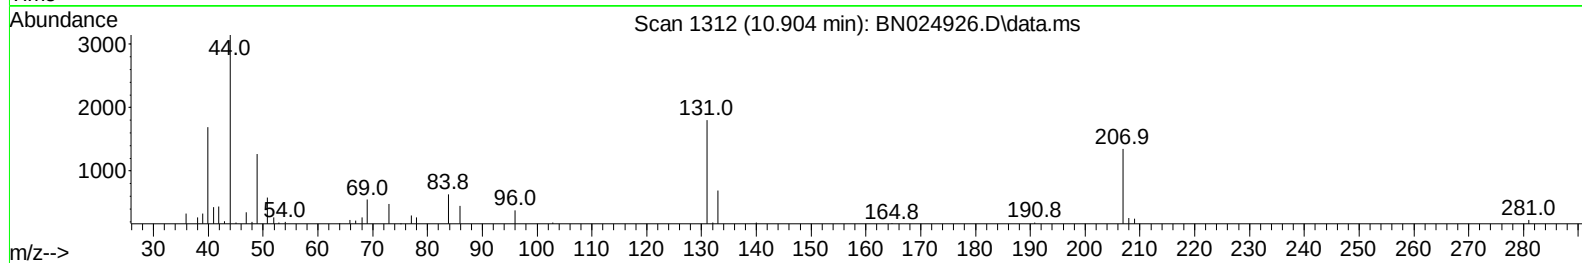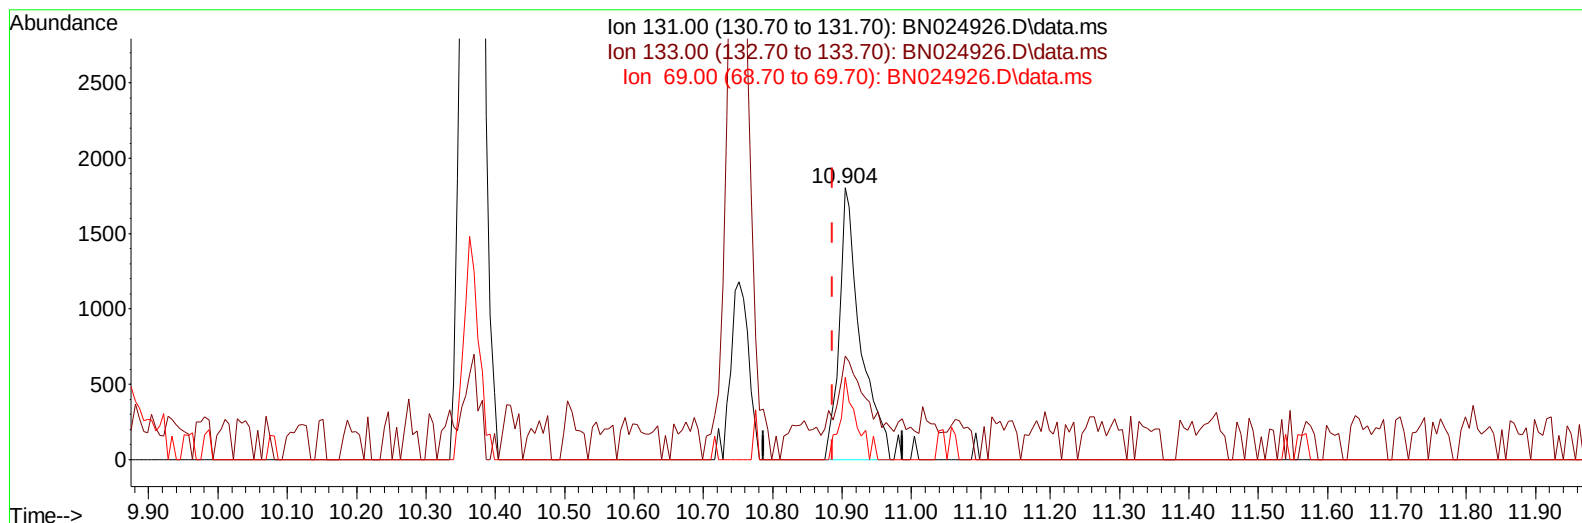

TIC: BN024926.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.904min (+ 0.018) 0.13 ng/ul m

response 3819

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.00	38.16
69.00	19.40	30.23#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024926.D
 Acq On : 15 Apr 2023 09:47
 Operator : CG/JU
 Sample : PB152052TB 10X
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB052

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/26/2023
 Supervised By :Jagrut Upadhyay 04/26/2023

Quant Time: Apr 17 03:01:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 17 02:58:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	286757	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136	1263797	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164	794082	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	1716544	20.000	ng/ul	0.00
79) Chrysene-d12	21.521	240	1676582	20.000	ng/ul	0.00
88) Perylene-d12	23.974	264	1750016	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	48095	6.383	ng/uL	0.00
4) Pyridine-d5	3.758	84	53502m	2.371	ng/ul	0.02
7) Phenol-d5	7.093	99	779262	27.873	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	611770	32.716	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	682732	33.230	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	578869	26.082	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128	344405	33.657	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	377429	34.053	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	636532	32.130	ng/ul	0.00
31) 4-Chloroaniline-d4	10.904	131	3819m	0.127	ng/ul	0.02
46) Dimethylphthalate-d6	13.992	166	2105409	34.202	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	2064576	29.267	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	378232	29.974	ng/ul	0.00
60) Fluorene-d10	15.575	176	1808777	34.801	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	336017	30.079	ng/ul	0.00
73) Anthracene-d10	17.428	188	2762364	34.264	ng/ul	0.00
81) Pyrene-d10	19.722	212	3325628	34.159	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.815	264	2747479	30.026	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024926.D
Acq On : 15 Apr 2023 09:47
Operator : CG/JU
Sample : PB152052TB 10X
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB052

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/26/2023
Supervised By :Jagrut Upadhyay 04/26/2023

Quant Time: Apr 17 03:01:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 17 02:58:51 2023
Response via : Initial Calibration

