

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024881.D
 Acq On : 14 Apr 2023 04:55
 Operator : CG/JU
 Sample : 02275-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ2

Quant Time: Apr 14 05:39:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 14 03:27:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	359625	20.000	ng/u1	0.00
20) Naphthalene-d8	10.752	136	1589403	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	987435	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.334	188	2156375	20.000	ng/u1	0.00
79) Chrysene-d12	21.522	240	2104754	20.000	ng/u1	0.00
88) Perylene-d12	23.963	264	2298889	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	43351	4.588	ng/uL	0.00
4) Pyridine-d5	3.740	84	263329	9.307	ng/u1	0.00
7) Phenol-d5	7.099	99	196362	5.601	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	644340	27.476	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	533328	20.699	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	368703	13.246	ng/u1	-0.01
21) Nitrobenzene-d5	9.110	128	349421	27.152	ng/u1	0.00
24) 2-Nitrophenol-d4	9.834	143	359014	25.756	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	594317	23.854	ng/u1	0.00
31) 4-Chloroaniline-d4	10.893	131	855114	22.616	ng/u1	0.00
46) Dimethylphthalate-d6	13.993	166	2291760	29.939	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	2500200	28.502	ng/u1	0.00
54) 4-Nitrophenol-d4	14.781	143	67707	4.315	ng/u1	0.00
60) Fluorene-d10	15.575	176	1947980	30.140	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	346297	24.676	ng/u1	0.00
73) Anthracene-d10	17.434	188	3188634	31.484	ng/u1	0.00
81) Pyrene-d10	19.722	212	3853226	31.527	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.810	264	3878193	32.264	ng/u1	-0.02
Target Compounds						
2) 1,4-Dioxane	3.346	88	13870	1.360	ng/uL	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024881.D
Acq On : 14 Apr 2023 04:55
Operator : CG/JU
Sample : 02275-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDZ2

Quant Time: Apr 14 05:39:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 14 03:27:44 2023
Response via : Initial Calibration

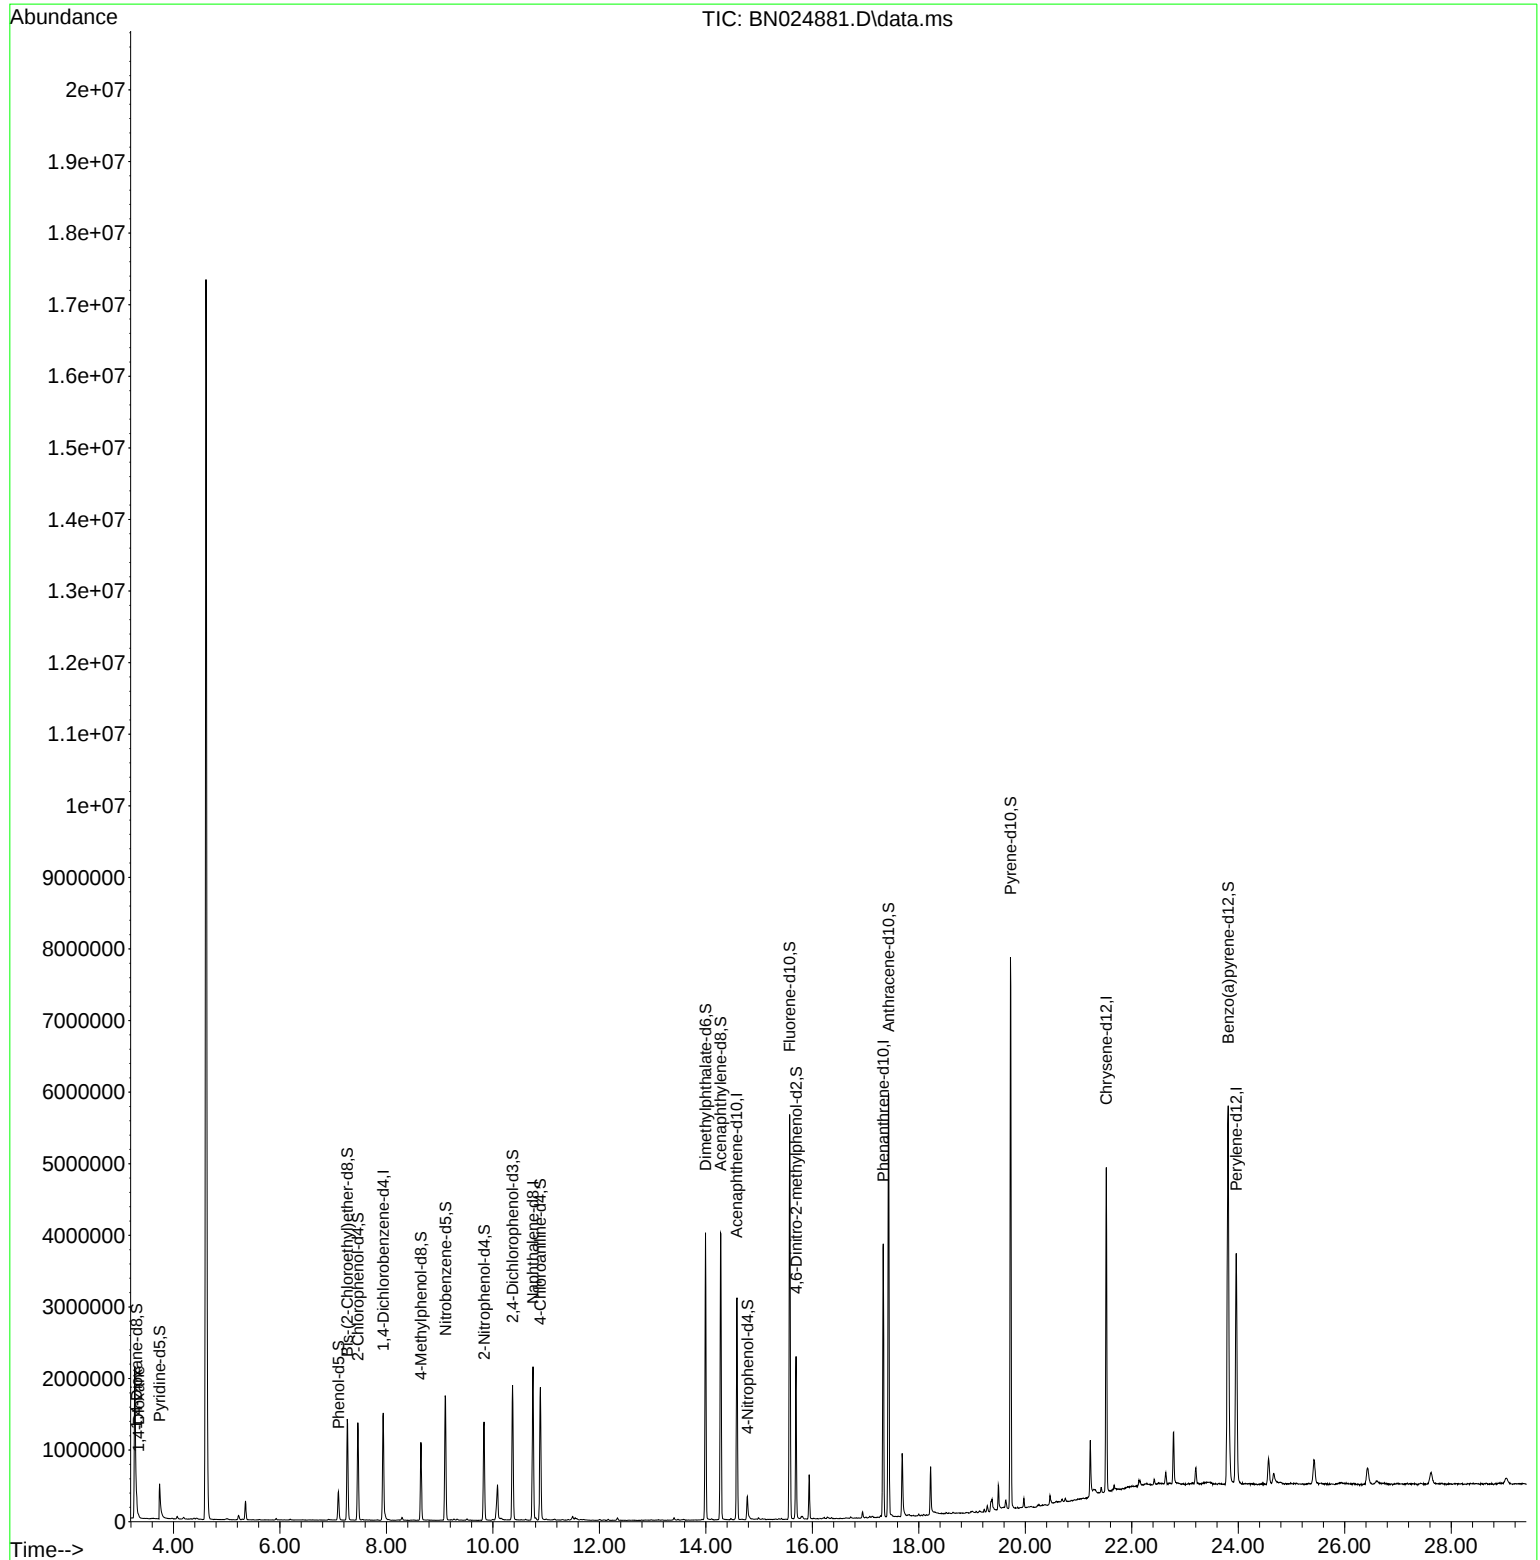

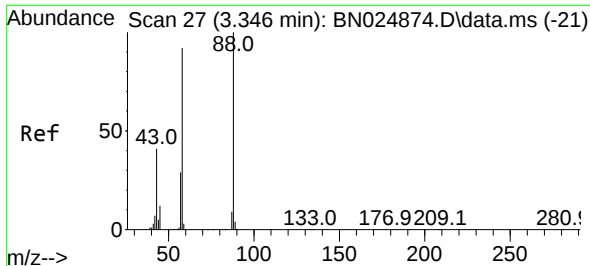

#2
 1,4-Dioxane
 Concen: 1.360 ng/uL
 RT: 3.346 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN024881.D
 Acq: 14 Apr 2023 04:55

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ2

Tgt Ion: 88 Resp: 13870
 Ion Ratio Lower Upper
 88 100
 43 45.5 33.0 49.4
 58 83.1 72.3 108.5

