

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024882.D
 Acq On : 14 Apr 2023 05:31
 Operator : CG/JU
 Sample : 02275-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ3

Quant Time: Apr 14 06:00:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 14 03:27:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	324781	20.000	ng/u1	0.00
20) Naphthalene-d8	10.751	136	1408124	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.587	164	841448	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.333	188	1948520	20.000	ng/u1	0.00
79) Chrysene-d12	21.516	240	1875205	20.000	ng/u1	-0.01
88) Perylene-d12	23.968	264	2035163	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	42419	4.971	ng/uL	0.00
4) Pyridine-d5	3.740	84	232421	9.096	ng/u1	0.00
7) Phenol-d5	7.099	99	207623	6.557	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	610678	28.835	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	538536	23.143	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	383415	15.253	ng/u1	-0.01
21) Nitrobenzene-d5	9.110	128	336499	29.514	ng/u1	0.00
24) 2-Nitrophenol-d4	9.834	143	352206	28.520	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	595022	26.957	ng/u1	0.00
31) 4-Chloroaniline-d4	10.893	131	872529	26.047	ng/u1	0.00
46) Dimethylphthalate-d6	13.992	166	2057841	31.547	ng/u1	0.00
49) Acenaphthylene-d8	14.281	160	2265521	30.308	ng/u1	0.00
54) 4-Nitrophenol-d4	14.781	143	69993	5.235	ng/u1	0.00
60) Fluorene-d10	15.575	176	1787737	32.460	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	339738	26.791	ng/u1	0.00
73) Anthracene-d10	17.428	188	3156435	34.491	ng/u1	0.00
81) Pyrene-d10	19.722	212	3722000	34.181	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.804	264	3785937	35.578	ng/u1	-0.02
Target Compounds						
2) 1,4-Dioxane	3.346	88	13009	1.413	ng/uL#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024882.D
Acq On : 14 Apr 2023 05:31
Operator : CG/JU
Sample : 02275-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDZ3


Quant Time: Apr 14 06:00:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 14 03:27:44 2023
Response via : Initial Calibration

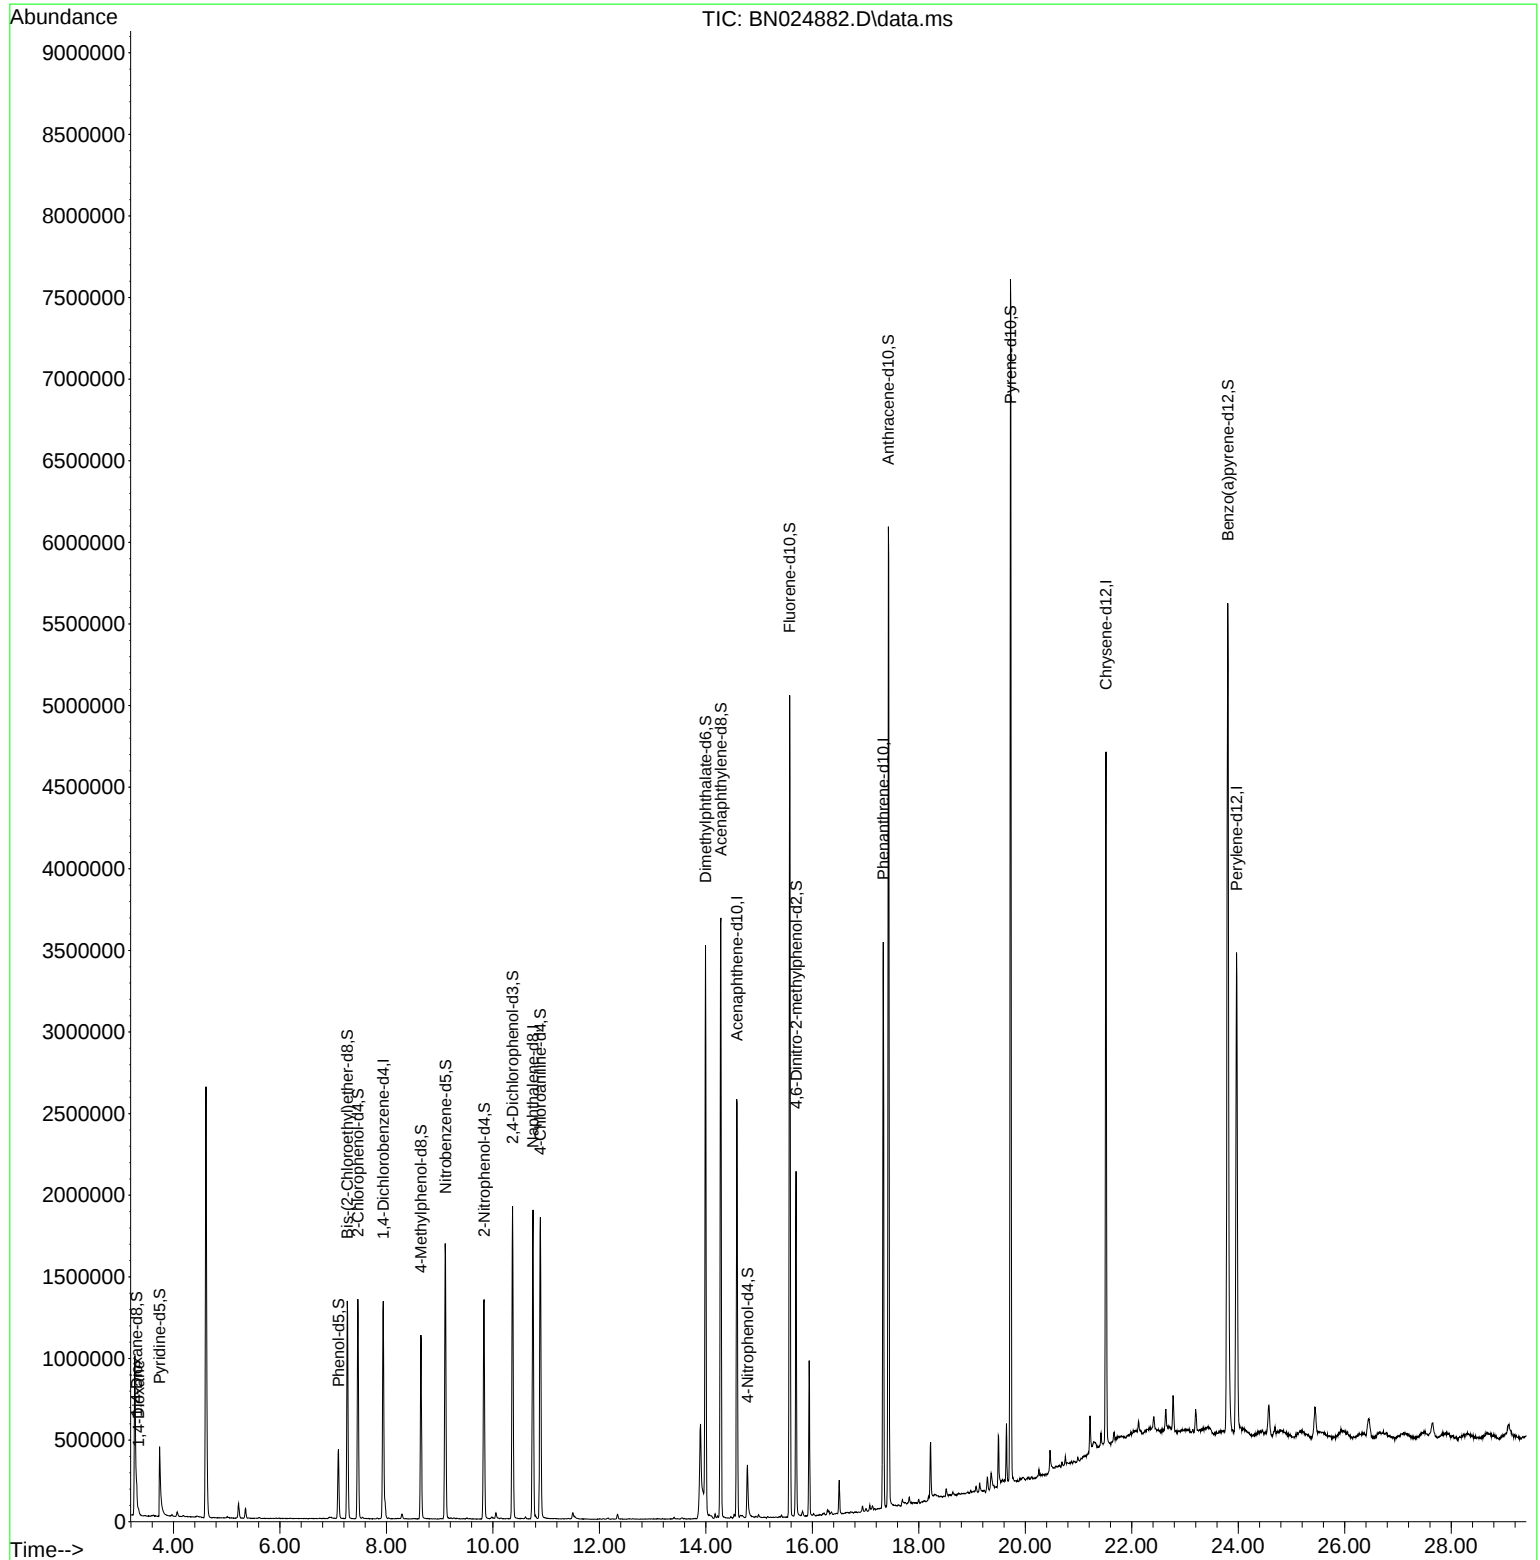

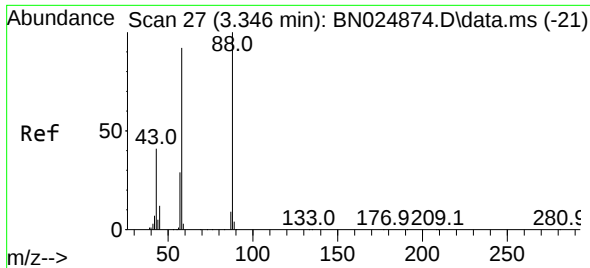

#2
 1,4-Dioxane
 Concen: 1.413 ng/uL
 RT: 3.346 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN024882.D
 Acq: 14 Apr 2023 05:31

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ3

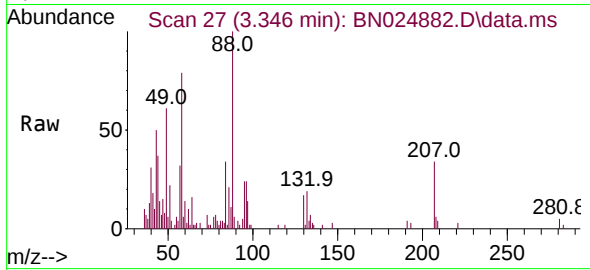

Tgt Ion:	88	Resp:	13009
Ion	Ratio	Lower	Upper
88	100		
43	50.3	33.0	49.4#
58	79.0	72.3	108.5

