

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024886.D
 Acq On : 14 Apr 2023 07:55
 Operator : CG/JU
 Sample : 02275-13
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ8

Quant Time: Apr 14 08:24:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 14 03:27:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	300612	20.000	ng/u1	0.00
20) Naphthalene-d8	10.751	136	1307010	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	816261	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.328	188	1771719	20.000	ng/u1	0.00
79) Chrysene-d12	21.521	240	1723397	20.000	ng/u1	0.00
88) Perylene-d12	23.980	264	1882271	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	57822	7.321	ng/uL	0.00
4) Pyridine-d5	3.740	84	273464	11.563	ng/u1	0.00
7) Phenol-d5	7.093	99	245642	8.381	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	716679	36.560	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	624519	28.996	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	419435	18.027	ng/u1	-0.01
21) Nitrobenzene-d5	9.104	128	375598	35.492	ng/u1	0.00
24) 2-Nitrophenol-d4	9.834	143	395581	34.510	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	663196	32.370	ng/u1	0.00
31) 4-Chloroaniline-d4	10.893	131	913522	29.381	ng/u1	0.00
46) Dimethylphthalate-d6	13.992	166	2453018	38.766	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	2665403	36.758	ng/u1	0.00
54) 4-Nitrophenol-d4	14.781	143	86953	6.704	ng/u1	0.00
60) Fluorene-d10	15.575	176	2047541	38.325	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	384010	33.305	ng/u1	0.00
73) Anthracene-d10	17.428	188	3293675	39.582	ng/u1	0.00
81) Pyrene-d10	19.727	212	3999331	39.963	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.827	264	4120233	41.865	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.346	88	27033	3.172	ng/uL	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024886.D
Acq On : 14 Apr 2023 07:55
Operator : CG/JU
Sample : 02275-13
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDZ8

Quant Time: Apr 14 08:24:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 14 03:27:44 2023
Response via : Initial Calibration

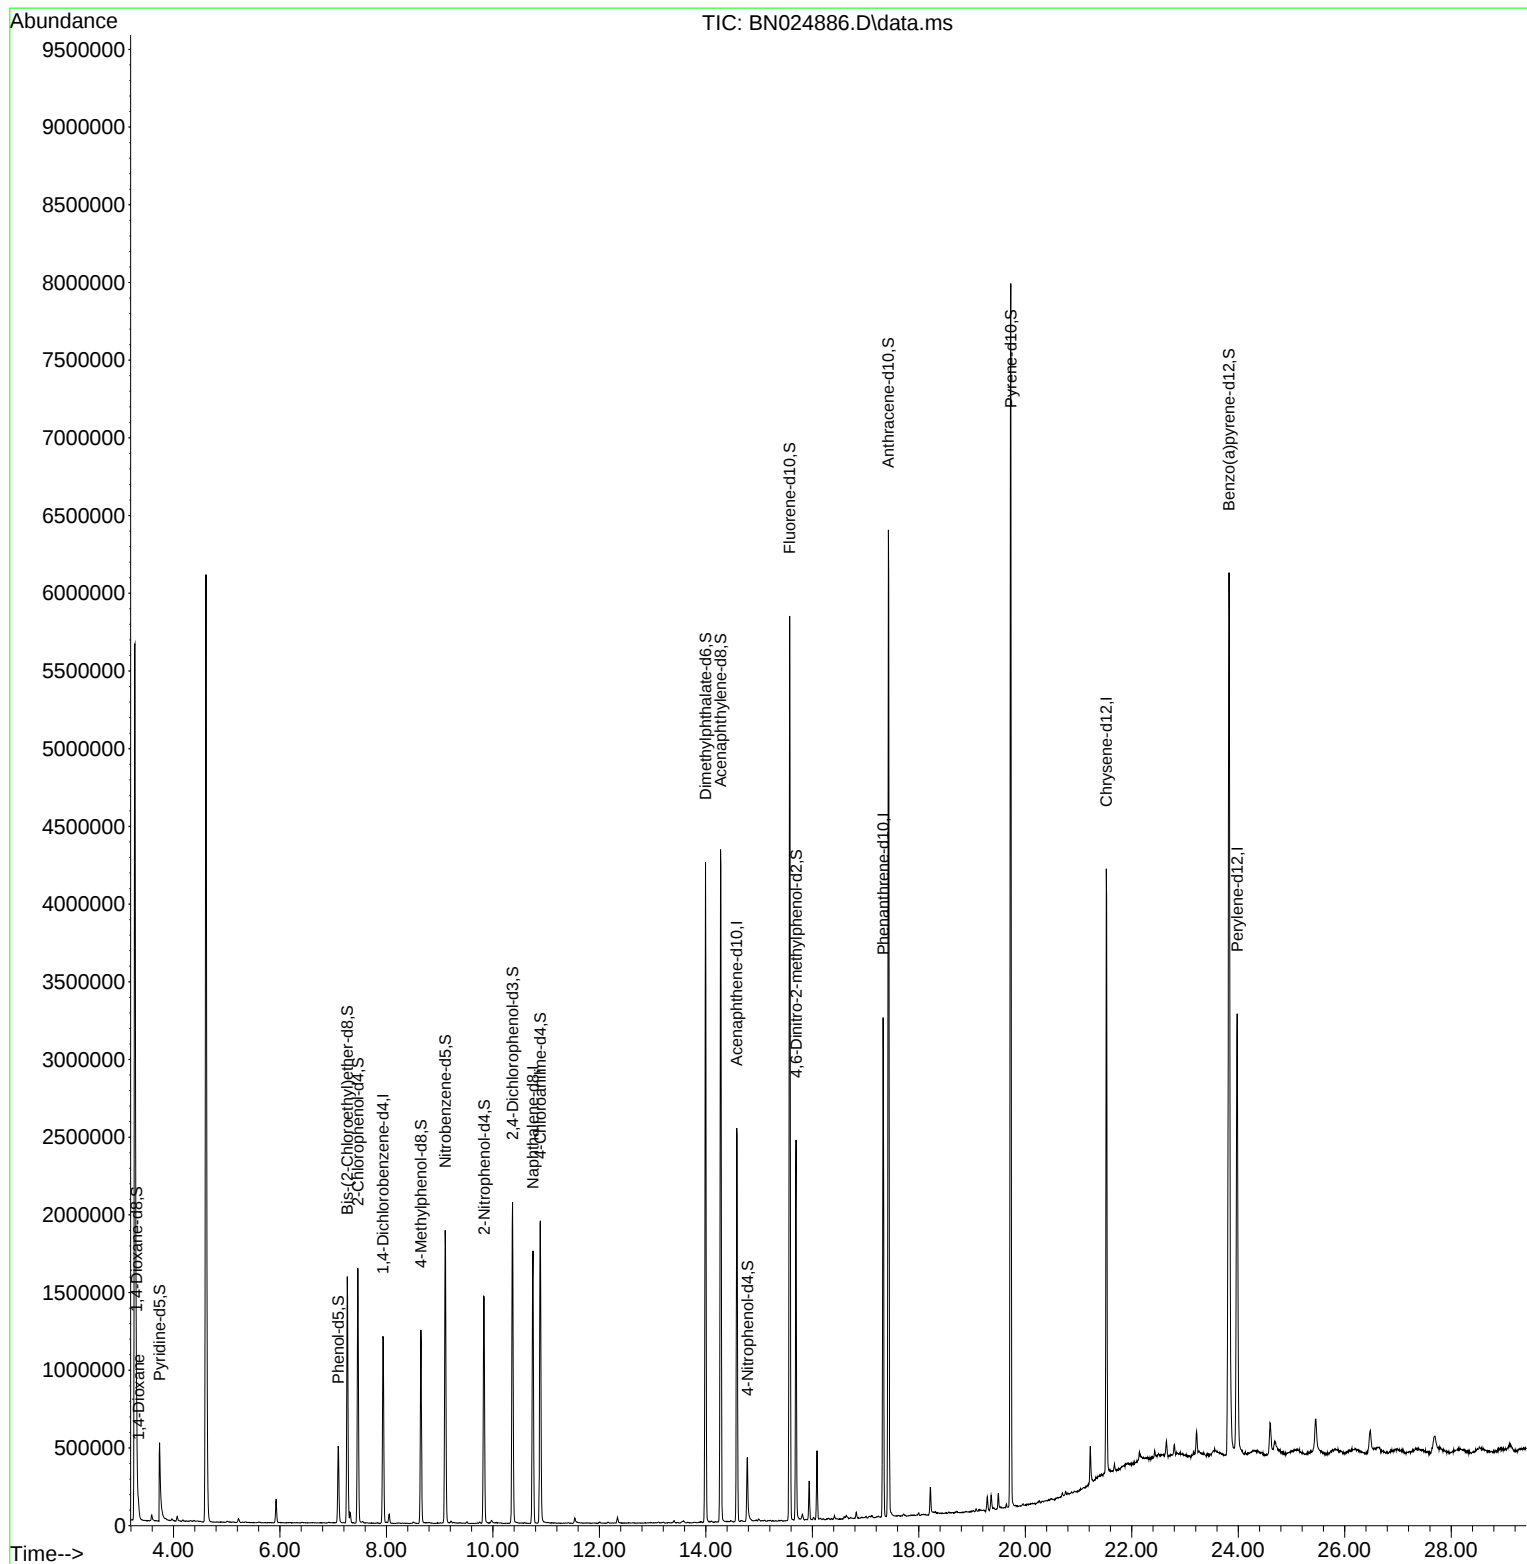

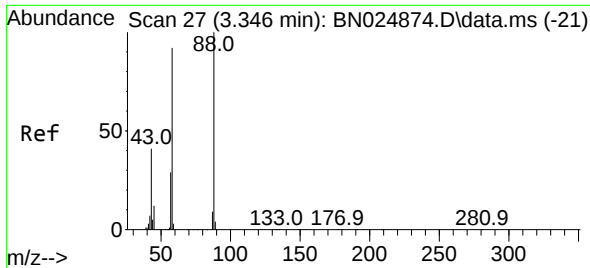

#2
 1,4-Dioxane
 Concen: 3.172 ng/uL
 RT: 3.346 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN024886.D
 Acq: 14 Apr 2023 07:55

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ8

Tgt Ion: 88 Resp: 27033
 Ion Ratio Lower Upper
 88 100
 43 44.9 33.0 49.4
 58 84.2 72.3 108.5

