

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024893.D
 Acq On : 14 Apr 2023 12:11
 Operator : CG/JU
 Sample : 02252-05
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COME1

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 04/17/2023
 Supervised By : Jagrut Upadhyay 04/17/2023

Quant Time: Apr 14 22:47:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 14 22:34:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	262923m	20.000	ng/u1	0.01
20) Naphthalene-d8	10.751	136	1177805	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.587	164	701489	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.333	188	1518744	20.000	ng/u1	0.00
79) Chrysene-d12	21.527	240	1562731	20.000	ng/u1	0.00
88) Perylene-d12	23.986	264	1677840	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	27501	3.981	ng/uL	0.00
4) Pyridine-d5	3.746	84	149282	7.217	ng/u1	0.01
7) Phenol-d5	7.105	99	133332	5.201	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	915320	53.387	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	407559	21.635	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	259517	12.753	ng/u1	0.00
21) Nitrobenzene-d5	9.110	128	272660	28.591	ng/u1	0.00
24) 2-Nitrophenol-d4	9.834	143	286722	27.758	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	465935	25.236	ng/u1	0.00
31) 4-Chloroaniline-d4	10.893	131	560493	20.004	ng/u1	0.00
46) Dimethylphthalate-d6	13.992	166	1649301	30.329	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	1841776	29.555	ng/u1	0.00
54) 4-Nitrophenol-d4	14.781	143	46607	4.181	ng/u1	0.00
60) Fluorene-d10	15.575	176	1448070	31.539	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	254988	25.798	ng/u1	0.00
73) Anthracene-d10	17.428	188	2359791	33.083	ng/u1	0.00
81) Pyrene-d10	19.727	212	2929546	32.283	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	2882194	32.853	ng/u1	0.00
Target Compounds						
8) Phenol	7.134	94	182933	6.853	ng/u1	100
12) 2-Chlorophenol	7.505	128	52278	2.657	ng/u1	96
22) Nitrobenzene	9.157	77	3592625	140.198	ng/u1	99
32) 4-Chloroaniline	10.916	127	111858	3.944	ng/u1	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024893.D
Acq On : 14 Apr 2023 12:11
Operator : CG/JU
Sample : 02252-05
Misc :
ALS Vial : 39 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
COME1

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023


Quant Time: Apr 14 22:47:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 14 22:34:56 2023
Response via : Initial Calibration

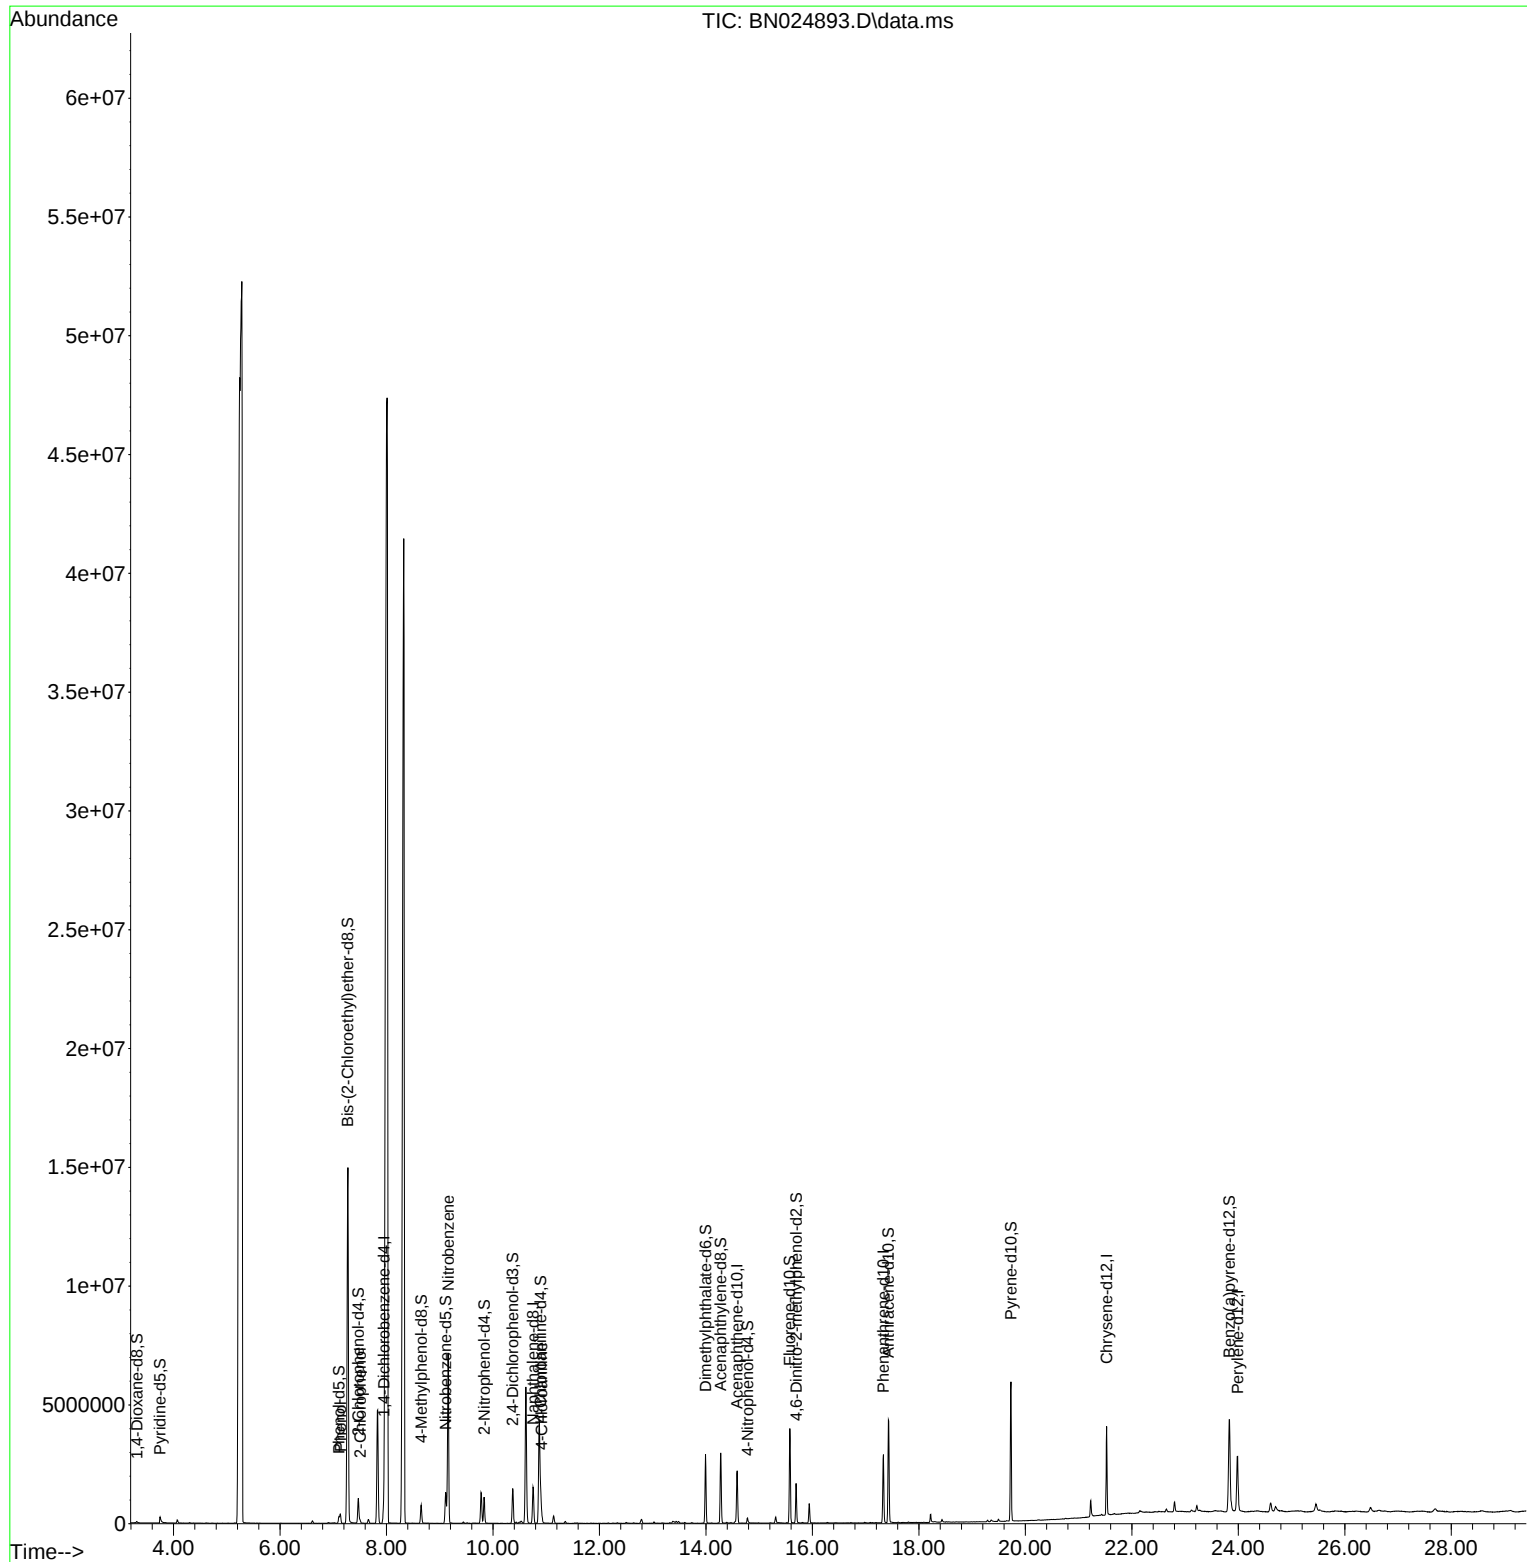

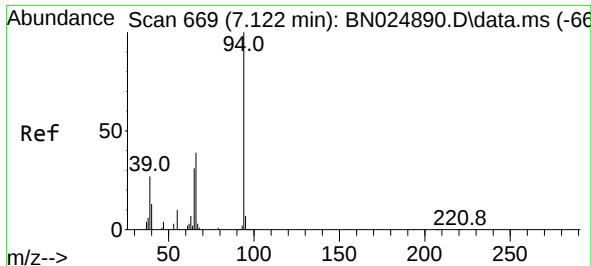

#8
Phenol
Concen: 6.853 ng/u1
RT: 7.134 min Scan# 669
Delta R.T. 0.006 min
Lab File: BN024893.D
Acq: 14 Apr 2023 12:11




Instrument :
BNA_N
ClientSampleId :
COME1

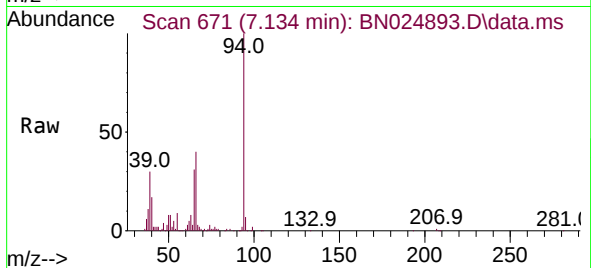

Tgt Ion: 94 Resp: 182933
Ion Ratio Lower Upper
94 100
65 31.4 25.1 37.7
66 39.8 31.9 47.9




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

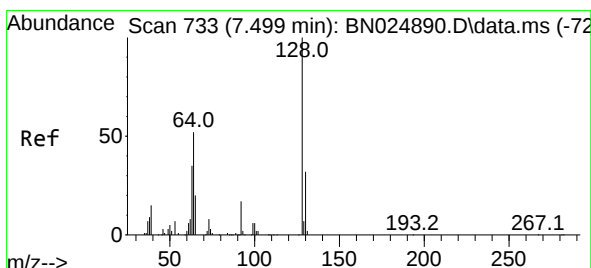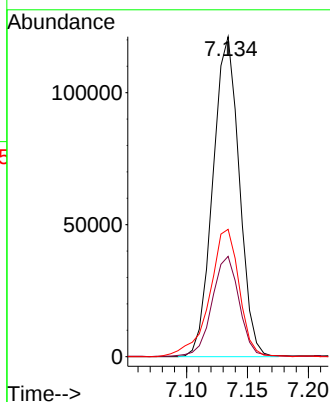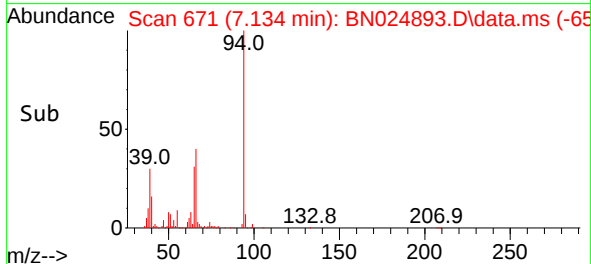

#12
2-Chlorophenol
Concen: 2.657 ng/u1
RT: 7.505 min Scan# 734
Delta R.T. 0.006 min
Lab File: BN024893.D
Acq: 14 Apr 2023 12:11


Tgt Ion:128 Resp: 52278
Ion Ratio Lower Upper
128 100
64 52.5 44.8 67.2
130 34.3 26.6 39.8

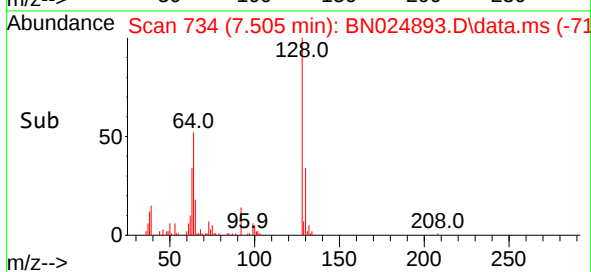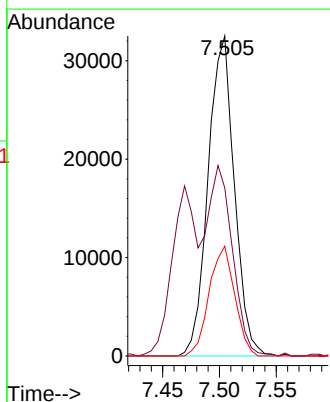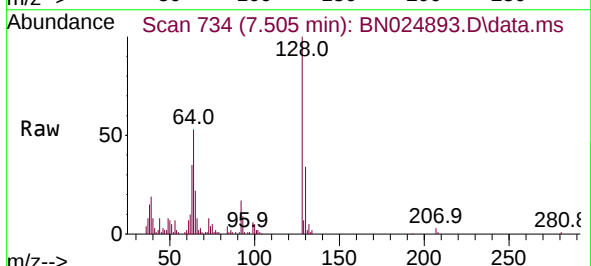

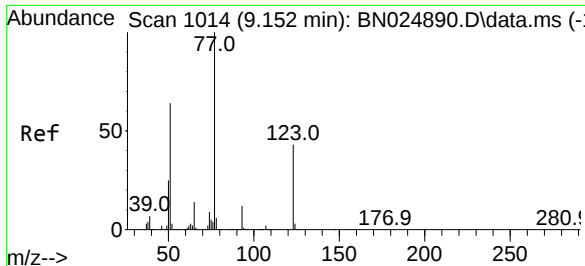

#22
Nitrobenzene
Concen: 140.198 ng/ul
RT: 9.157 min Scan# 1015
Delta R.T. 0.006 min
Lab File: BN024893.D
Acq: 14 Apr 2023 12:11




Instrument :
BNA_N
ClientSampleId :
COME1

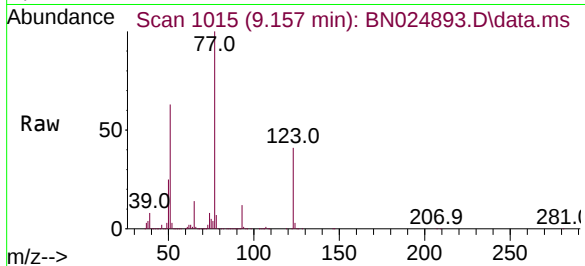

Tgt Ion: 77 Resp: 359262
Ion Ratio Lower Upper
77 100
123 41.2 33.5 50.3
65 14.3 11.8 17.8

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 04/17/2023
Supervised By :Jagrut Upadhyay 04/17/2023

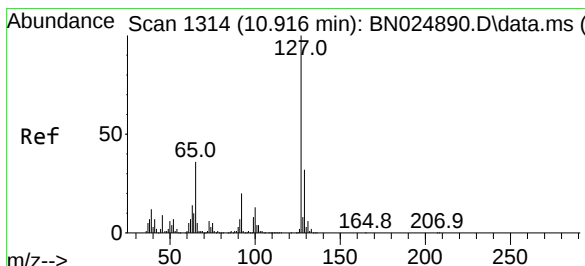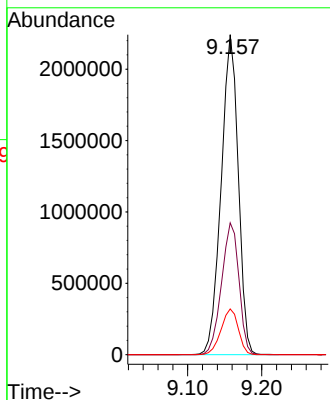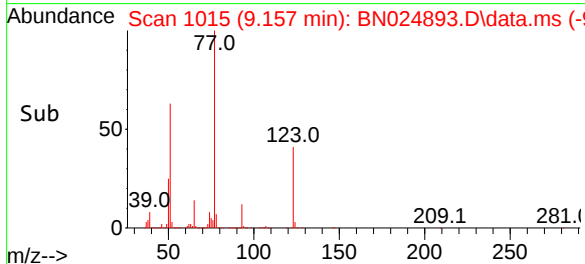

#32
4-Chloroaniline
Concen: 3.944 ng/ul
RT: 10.916 min Scan# 1314
Delta R.T. -0.000 min
Lab File: BN024893.D
Acq: 14 Apr 2023 12:11

Tgt Ion:127 Resp: 111858
Ion Ratio Lower Upper
127 100
129 30.4 25.5 38.3

