

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024895.D
 Acq On : 14 Apr 2023 13:25
 Operator : CG/JU
 Sample : 02252-17
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMF3

Quant Time: Apr 14 22:47:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 14 22:34:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	270411	20.000	ng/u1	0.00
20) Naphthalene-d8	10.752	136	1193072	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.587	164	758301	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.334	188	1631165	20.000	ng/u1	0.00
79) Chrysene-d12	21.527	240	1589041	20.000	ng/u1	0.00
88) Perylene-d12	23.968	264	1737277	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	29419	4.141	ng/uL	0.00
4) Pyridine-d5	3.746	84	75207	3.535	ng/u1	0.01
7) Phenol-d5	7.099	99	143910	5.459	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	512685	29.075	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	435252	22.465	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	284895	13.612	ng/u1	0.00
21) Nitrobenzene-d5	9.110	128	297785	30.826	ng/u1	0.00
24) 2-Nitrophenol-d4	9.834	143	317850	30.377	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	518192	27.707	ng/u1	0.00
31) 4-Chloroaniline-d4	10.893	131	504326	17.769	ng/u1	0.00
46) Dimethylphthalate-d6	13.993	166	1910514	32.500	ng/u1	0.00
49) Acenaphthylene-d8	14.281	160	2078178	30.850	ng/u1	0.00
54) 4-Nitrophenol-d4	14.781	143	55500	4.606	ng/u1	0.00
60) Fluorene-d10	15.575	176	1624957	32.740	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	281701	26.537	ng/u1	0.00
73) Anthracene-d10	17.433	188	2773443	36.202	ng/u1	0.00
81) Pyrene-d10	19.727	212	3283361	35.583	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.816	264	3308202	36.419	ng/u1	-0.01
Target Compounds						
35) 4-Chloro-3-methylphenol	12.040	107	99101	4.503	ng/u1	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024895.D
Acq On : 14 Apr 2023 13:25
Operator : CG/JU
Sample : 02252-17
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMF3


Quant Time: Apr 14 22:47:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 14 22:34:56 2023
Response via : Initial Calibration

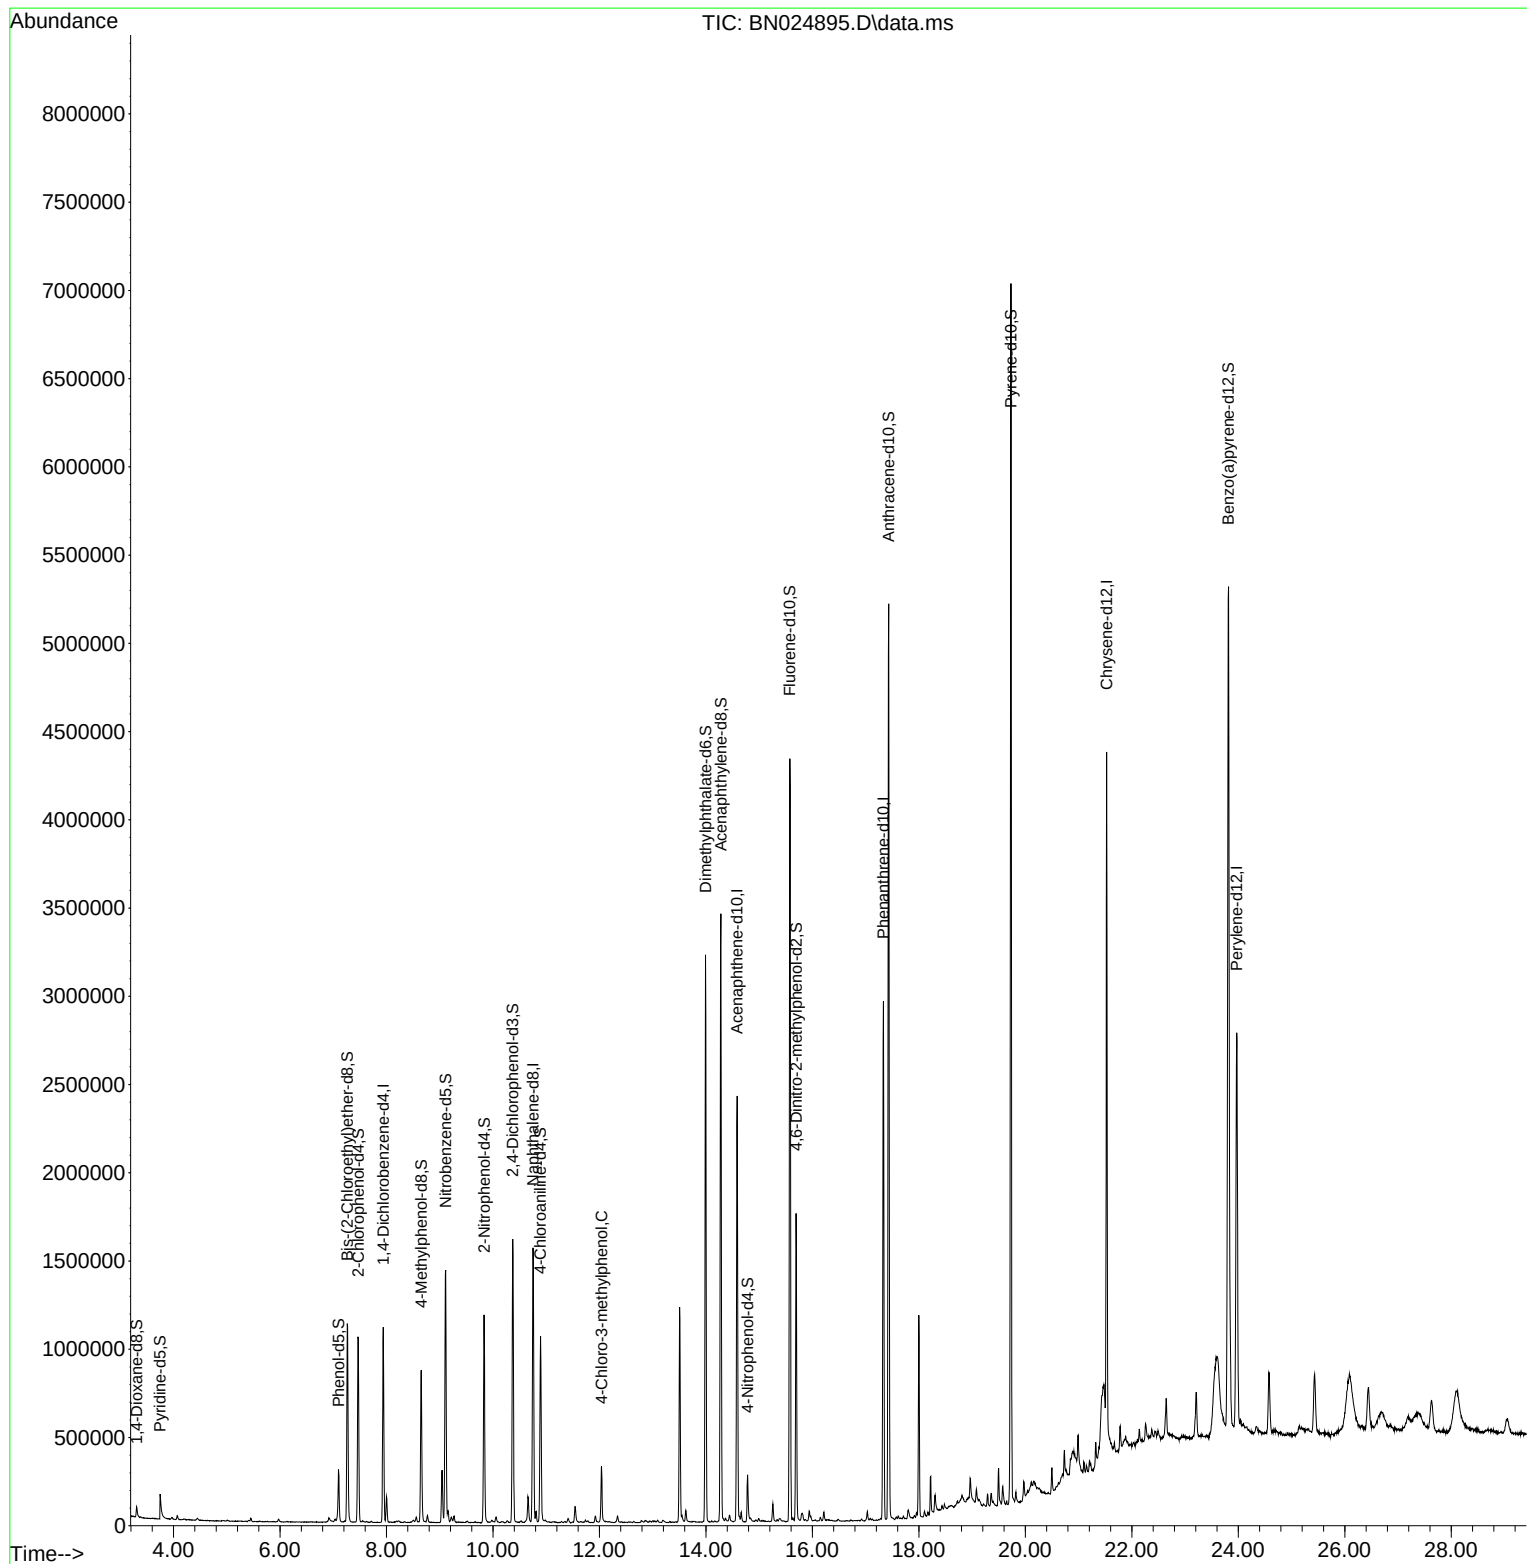

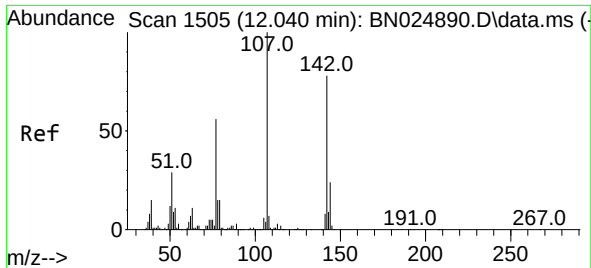

#35
 4-Chloro-3-methylphenol
 Concen: 4.503 ng/ul
 RT: 12.040 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BN024895.D
 Acq: 14 Apr 2023 13:25

Instrument :
 BNA_N
 ClientSampleId :
 COMF3

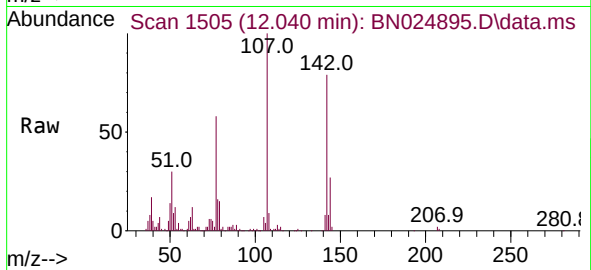

Tgt Ion:	107	Resp:	99101
Ion	Ratio	Lower	Upper
107	100		
144	26.7	19.6	29.4
142	78.9	60.7	91.1

