

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024933.D
 Acq On : 15 Apr 2023 14:03
 Operator : CG/JU
 Sample : 02254-17
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB6

Quant Time: Apr 17 03:02:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 17 02:58:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	285789	20.000	ng/u1	0.00
20) Naphthalene-d8	10.746	136	1262349	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	784960	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.328	188	1740150	20.000	ng/u1	0.00
79) Chrysene-d12	21.522	240	1797141	20.000	ng/u1	0.00
88) Perylene-d12	23.969	264	1994133	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	29689	3.954	ng/uL	0.00
4) Pyridine-d5	3.746	84	81253	3.614	ng/u1	0.01
7) Phenol-d5	7.093	99	170321	6.113	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.264	67	556503	29.862	ng/u1	0.00
11) 2-Chlorophenol-d4	7.464	132	483479	23.612	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	325488	14.715	ng/u1	0.00
21) Nitrobenzene-d5	9.105	128	319879	31.296	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	340669	30.771	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	544653	27.524	ng/u1	0.00
31) 4-Chloroaniline-d4	10.887	131	506915	16.880	ng/u1	0.00
46) Dimethylphthalate-d6	13.993	166	2019570	33.188	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	2282073	32.726	ng/u1	0.00
54) 4-Nitrophenol-d4	14.775	143	57246	4.589	ng/u1	0.00
60) Fluorene-d10	15.575	176	1790859	34.857	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	321572	28.395	ng/u1	0.00
73) Anthracene-d10	17.428	188	3000271	36.710	ng/u1	0.00
81) Pyrene-d10	19.722	212	3561314	34.126	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.816	264	3713616	35.617	ng/u1	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.340	88	46857	5.782	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024933.D
Acq On : 15 Apr 2023 14:03
Operator : CG/JU
Sample : 02254-17
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB6


Quant Time: Apr 17 03:02:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 17 02:58:51 2023
Response via : Initial Calibration

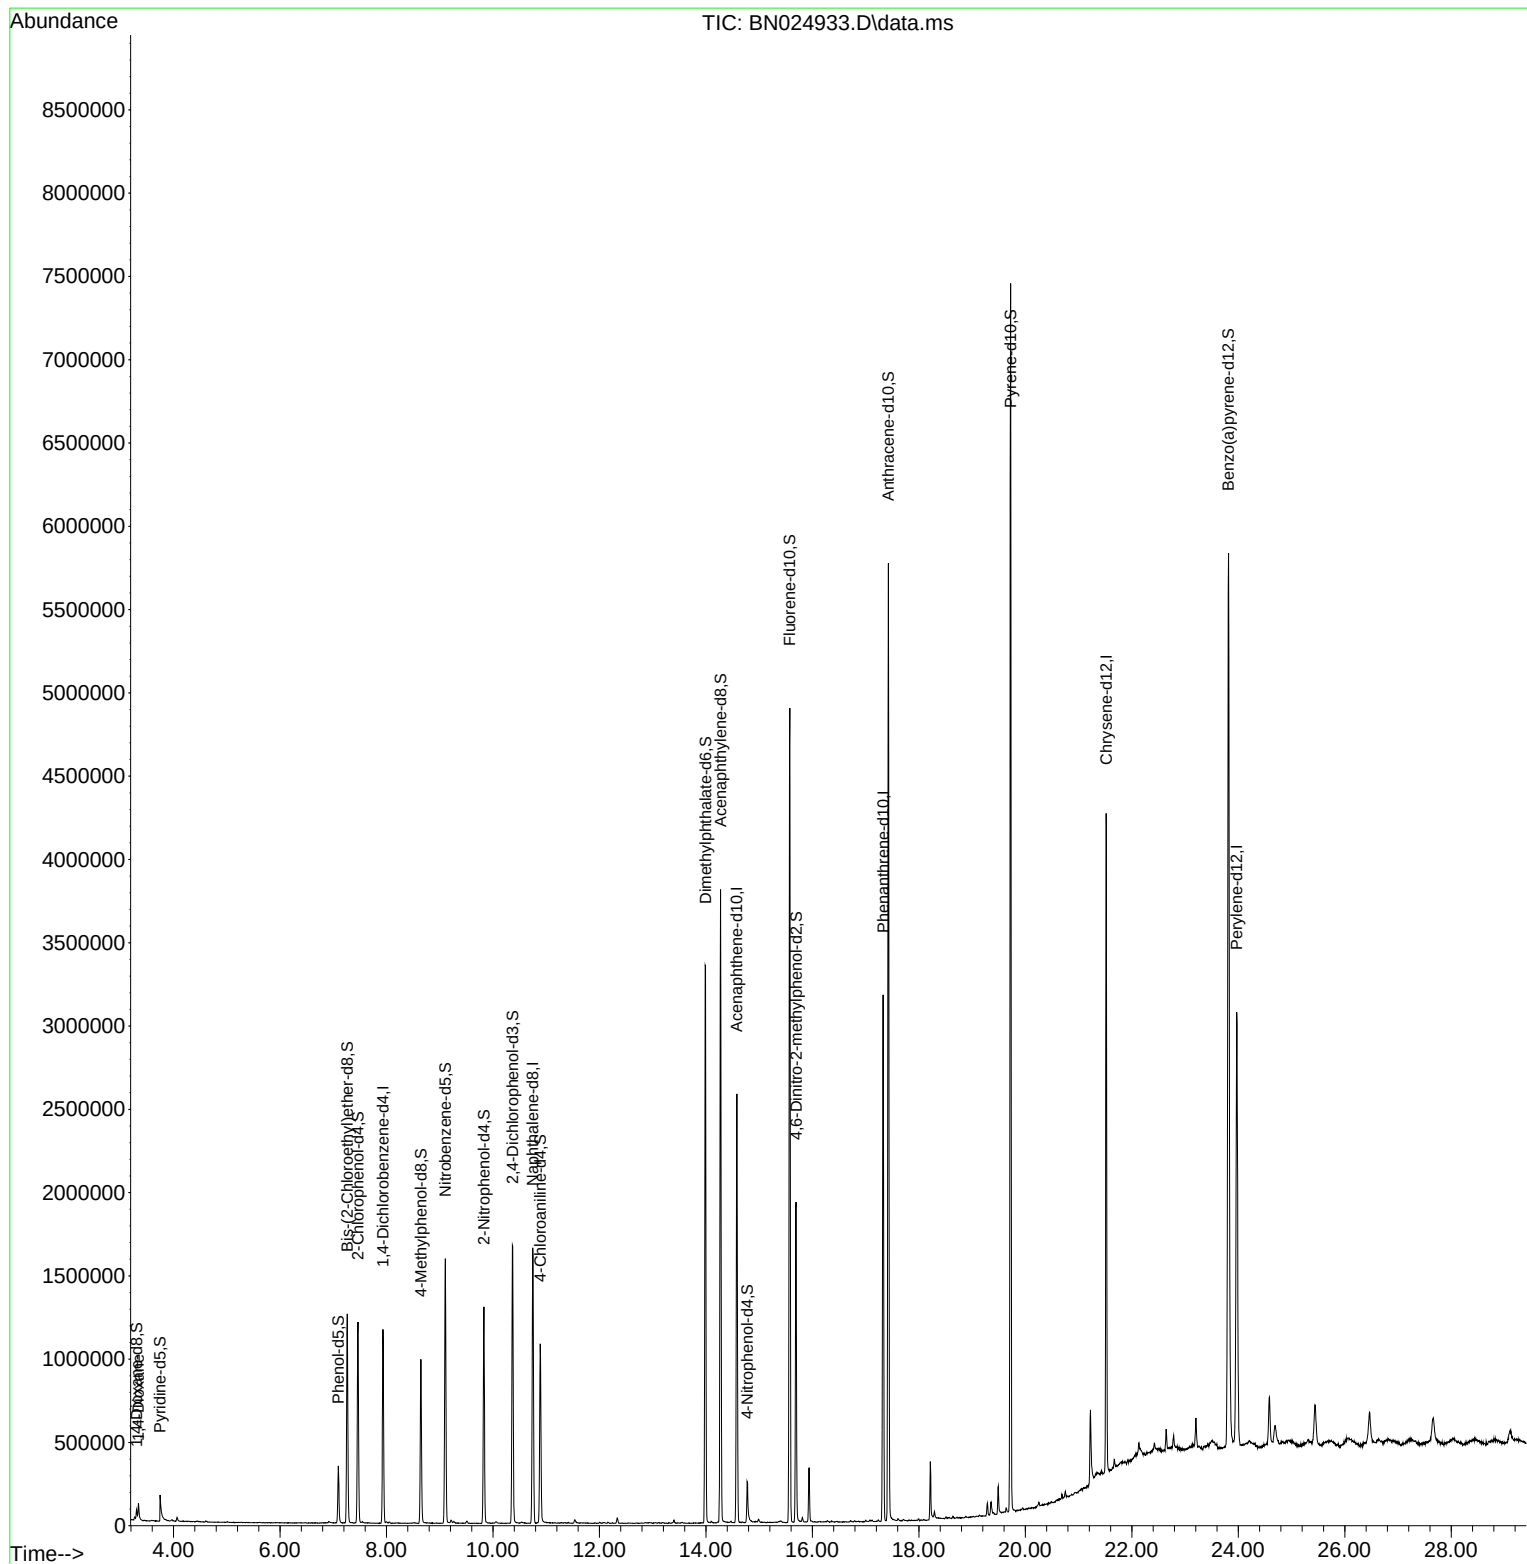

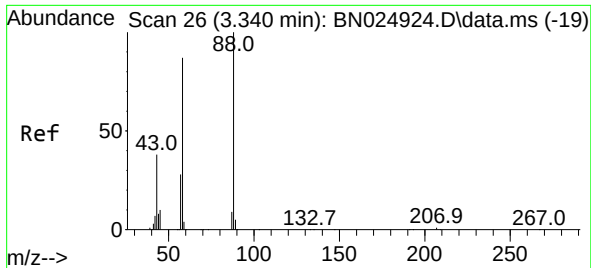

#2
 1,4-Dioxane
 Concen: 5.782 ng/uL
 RT: 3.340 min Scan# 20
 Delta R.T. 0.000 min
 Lab File: BN024933.D
 Acq: 15 Apr 2023 14:03

Instrument :
 BNA_N
 ClientSampleId :
 C0AB6

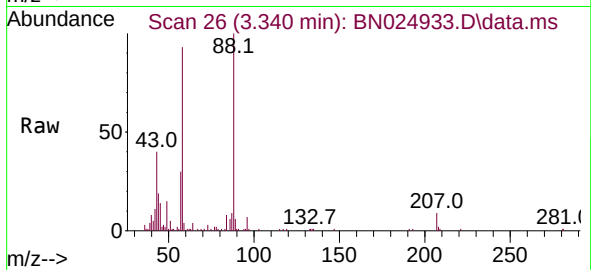

Tgt Ion:	88	Resp:	46857
Ion	Ratio	Lower	Upper
88	100		
43	39.8	33.0	49.4
58	93.1	72.3	108.5

