

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024934.D
 Acq On : 15 Apr 2023 14:39
 Operator : CG/JU
 Sample : 02254-18
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC0

Quant Time: Apr 17 03:02:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 17 02:58:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	306647	20.000	ng/u1	0.00
20) Naphthalene-d8	10.746	136	1335702	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	845014	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.328	188	1893462	20.000	ng/u1	0.00
79) Chrysene-d12	21.516	240	1861820	20.000	ng/u1	0.00
88) Perylene-d12	23.962	264	2069469	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	34711	4.308	ng/uL	0.00
4) Pyridine-d5	3.746	84	115915	4.805	ng/u1	0.01
7) Phenol-d5	7.093	99	188019	6.289	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	608924	30.452	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	538852	24.526	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	351117	14.794	ng/u1	0.00
21) Nitrobenzene-d5	9.104	128	348948	32.265	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	367334	31.358	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	588288	28.097	ng/u1	0.00
31) 4-Chloroaniline-d4	10.887	131	702130	22.097	ng/u1	0.00
46) Dimethylphthalate-d6	13.992	166	2103928	32.118	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	2405253	32.042	ng/u1	0.00
54) 4-Nitrophenol-d4	14.781	143	60075	4.474	ng/u1	0.00
60) Fluorene-d10	15.575	176	1891052	34.191	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	347490	28.200	ng/u1	0.00
73) Anthracene-d10	17.427	188	3118496	35.067	ng/u1	0.00
81) Pyrene-d10	19.721	212	3782141	34.983	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.810	264	3839948	35.487	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.340	88	450483	51.811	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024934.D
Acq On : 15 Apr 2023 14:39
Operator : CG/JU
Sample : 02254-18
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC0


Quant Time: Apr 17 03:02:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 17 02:58:51 2023
Response via : Initial Calibration

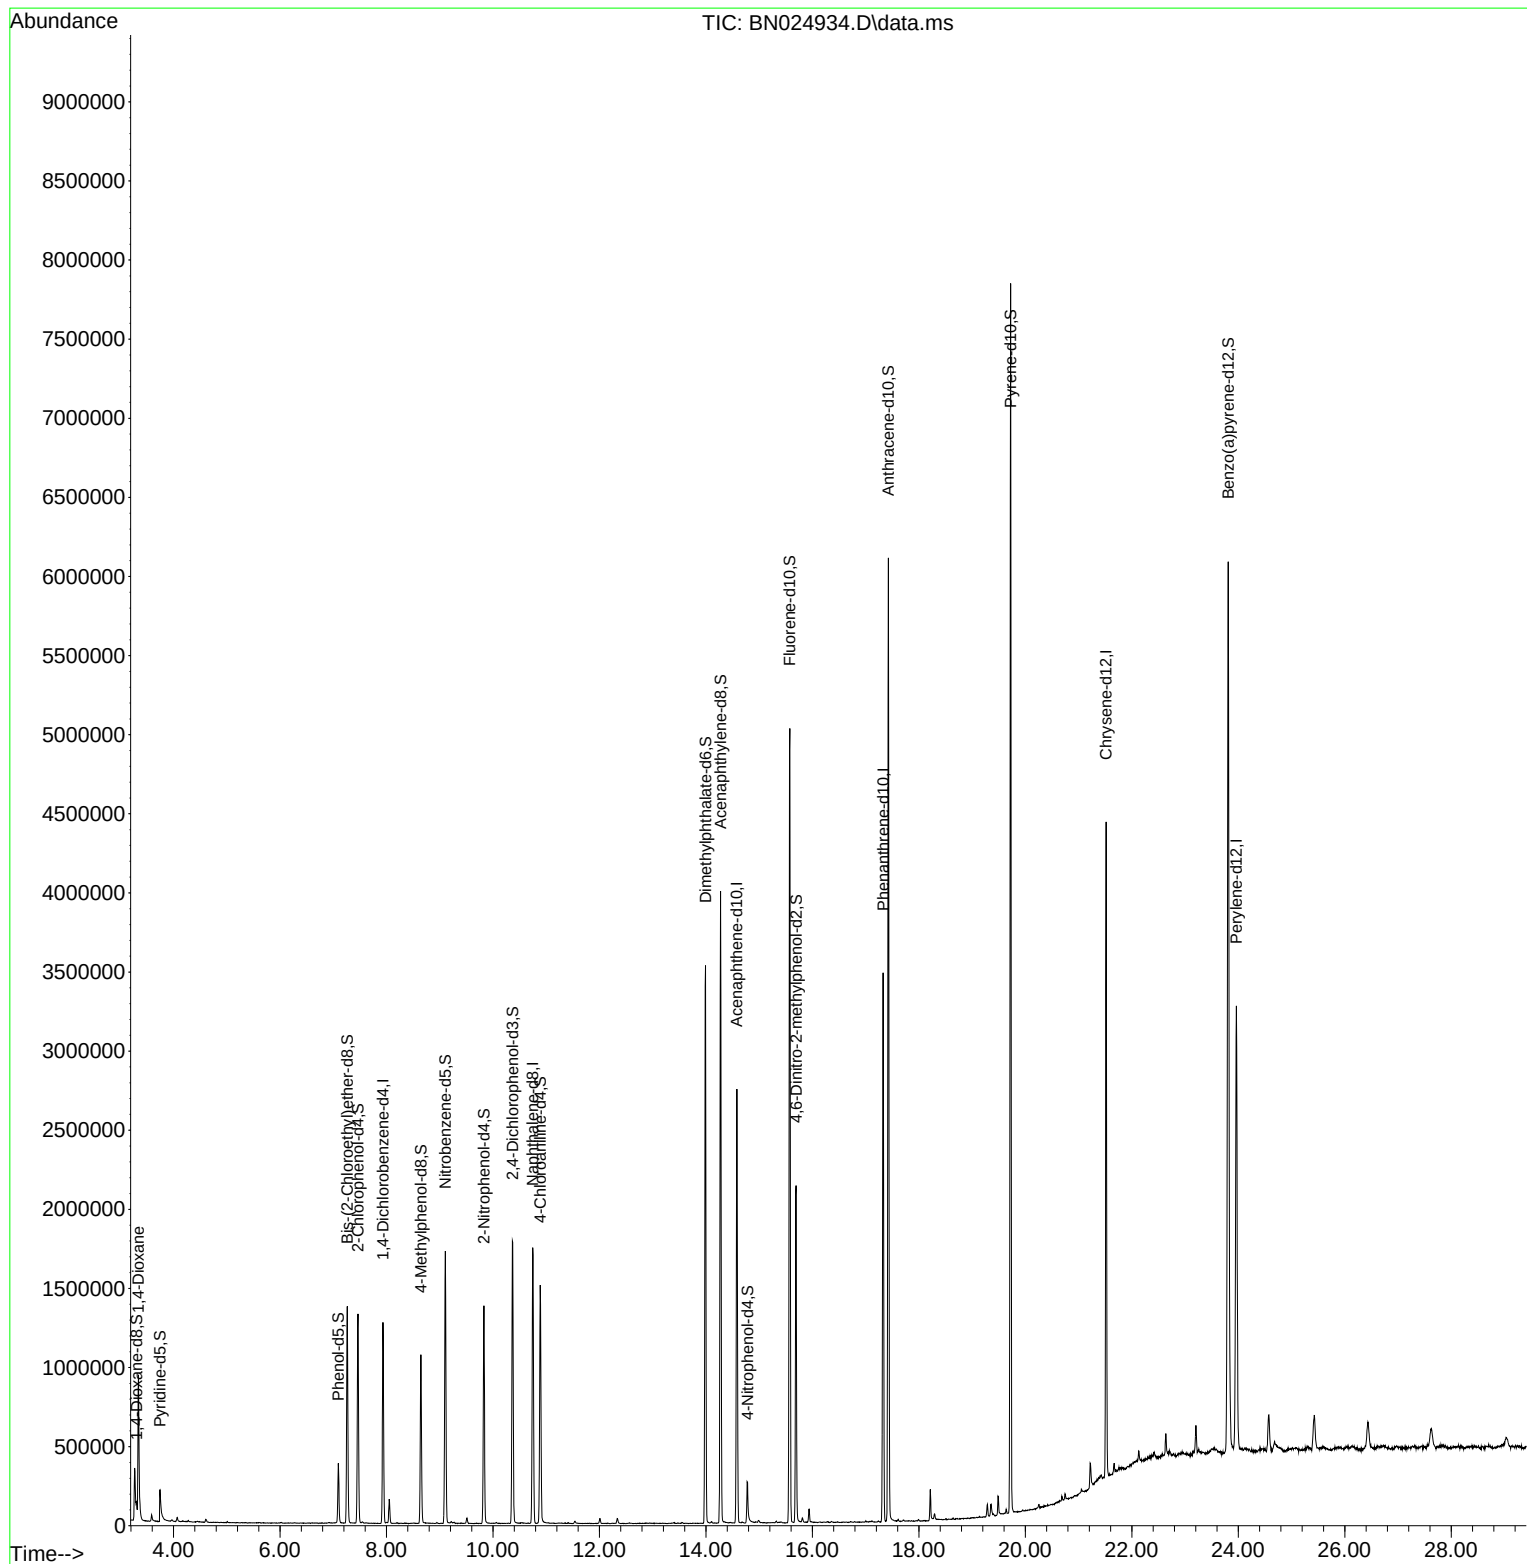

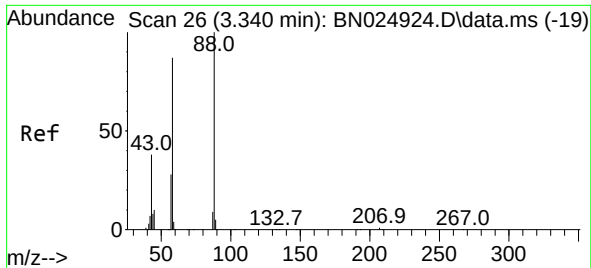

#2
 1,4-Dioxane
 Concen: 51.811 ng/uL
 RT: 3.340 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: BN024934.D
 Acq: 15 Apr 2023 14:39

Instrument :
 BNA_N
 ClientSampleId :
 C0AC0

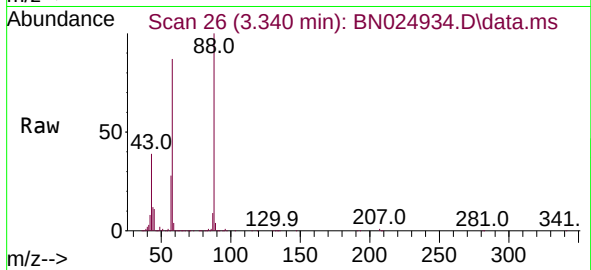

Tgt Ion: 88 Resp: 450483

Ion	Ratio	Lower	Upper
88	100		
43	39.4	33.0	49.4
58	86.6	72.3	108.5

