

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024937.D
 Acq On : 15 Apr 2023 16:29
 Operator : CG/JU
 Sample : 02275-14
 Misc :
 ALS Vial : 85 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ9

Quant Time: Apr 17 03:02:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 17 02:58:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	329937	20.000	ng/u1	0.00
20) Naphthalene-d8	10.746	136	1455874	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	897808	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.328	188	2002175	20.000	ng/u1	0.00
79) Chrysene-d12	21.522	240	2004392	20.000	ng/u1	0.00
88) Perylene-d12	23.969	264	2101256	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	53821	6.208	ng/uL	0.00
4) Pyridine-d5	3.734	84	240712	9.273	ng/u1	0.00
7) Phenol-d5	7.093	99	218496	6.793	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.264	67	706798	32.851	ng/u1	0.00
11) 2-Chlorophenol-d4	7.464	132	607442	25.696	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	396752	15.537	ng/u1	0.00
21) Nitrobenzene-d5	9.105	128	404319	34.299	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	417754	32.718	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	668020	29.271	ng/u1	0.00
31) 4-Chloroaniline-d4	10.887	131	922833	26.645	ng/u1	0.00
46) Dimethylphthalate-d6	13.993	166	2470470	35.495	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	2722872	34.140	ng/u1	0.00
54) 4-Nitrophenol-d4	14.781	143	80217	5.623	ng/u1	0.00
60) Fluorene-d10	15.575	176	2132766	36.294	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.693	200	387365	29.729	ng/u1	0.00
73) Anthracene-d10	17.428	188	3498635	37.206	ng/u1	0.00
81) Pyrene-d10	19.722	212	4173048	35.853	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.822	264	4137250	37.657	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.340	88	24467	2.615	ng/uL 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024937.D
Acq On : 15 Apr 2023 16:29
Operator : CG/JU
Sample : 02275-14
Misc :
ALS Vial : 85 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDZ9

Quant Time: Apr 17 03:02:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 17 02:58:51 2023
Response via : Initial Calibration

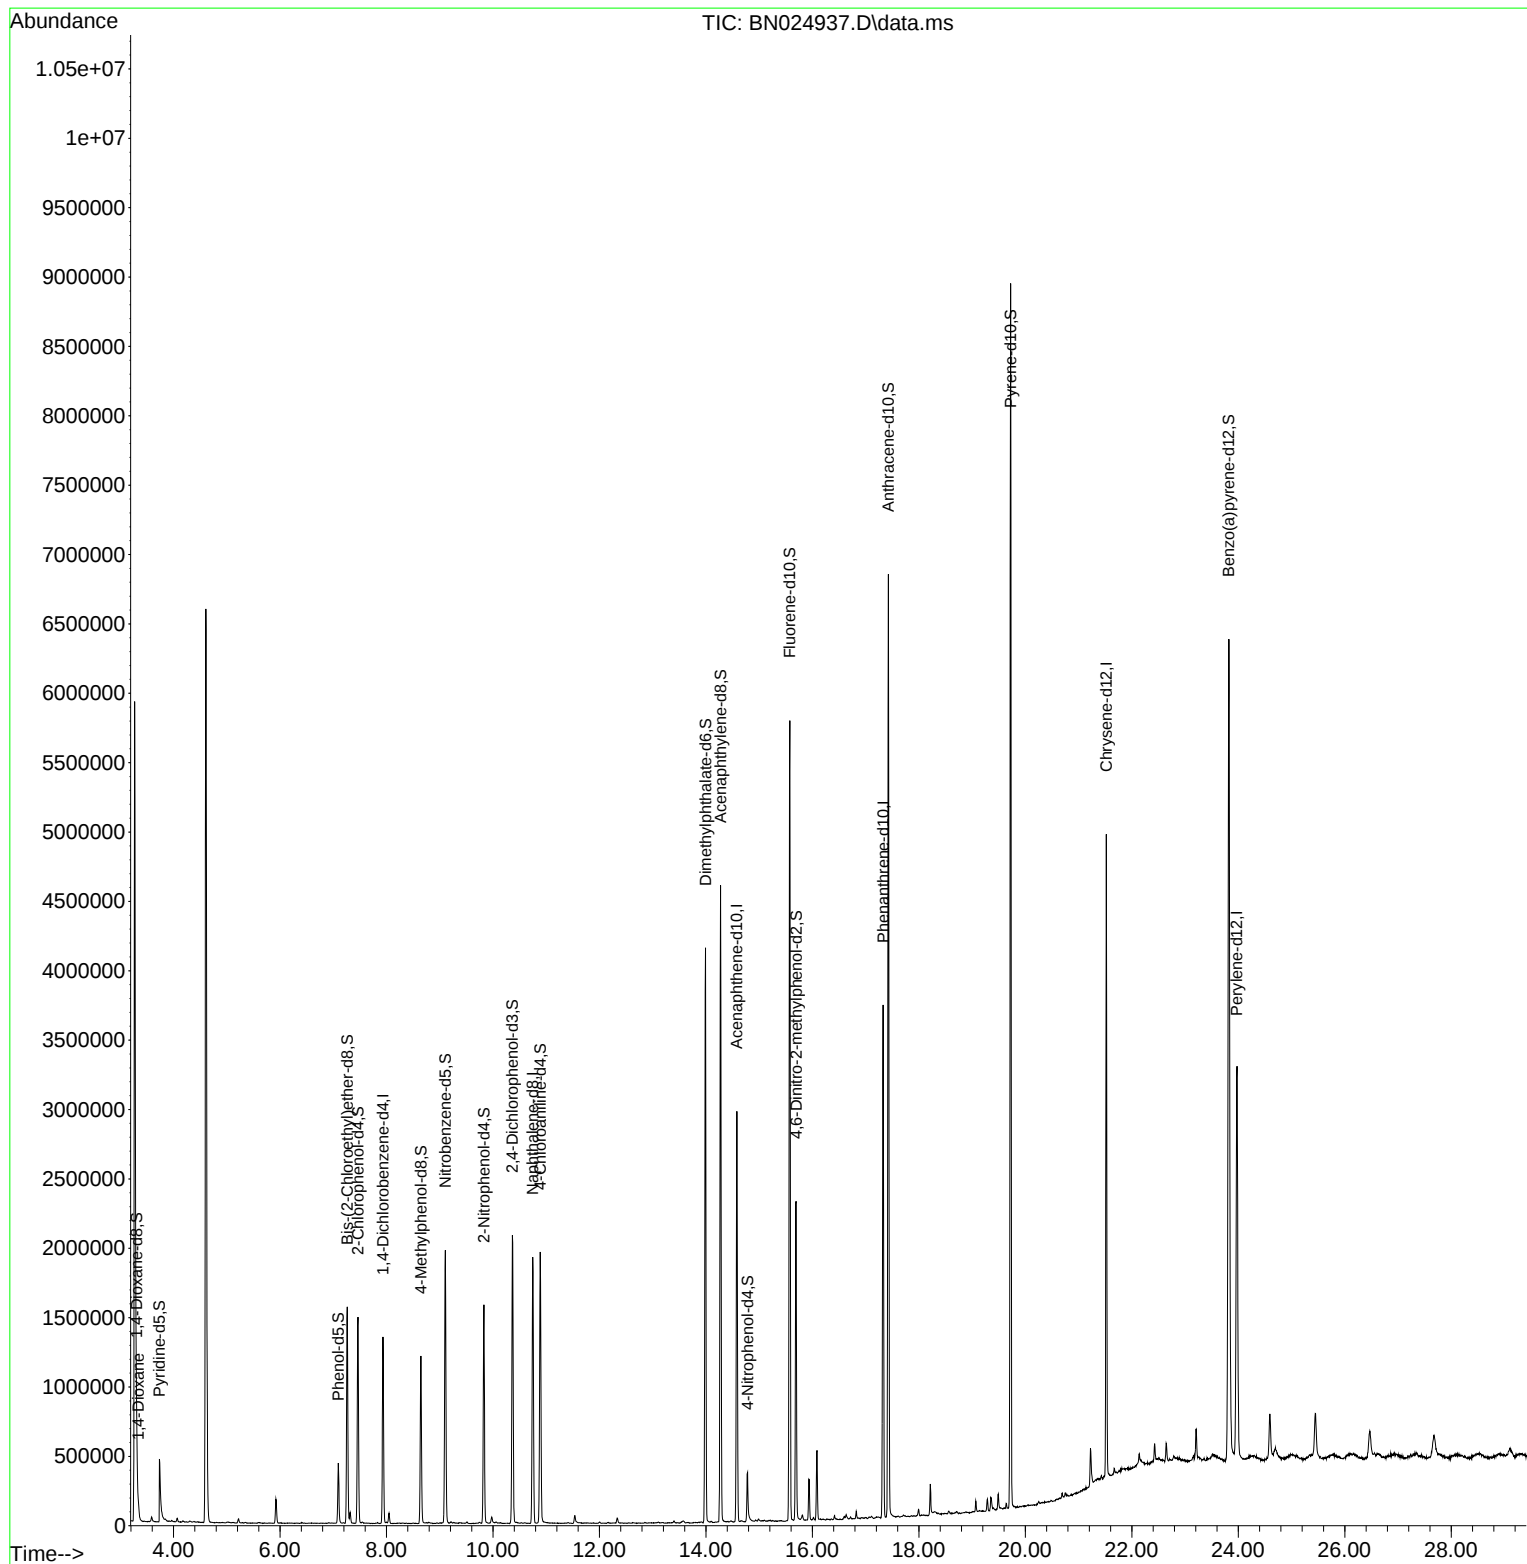

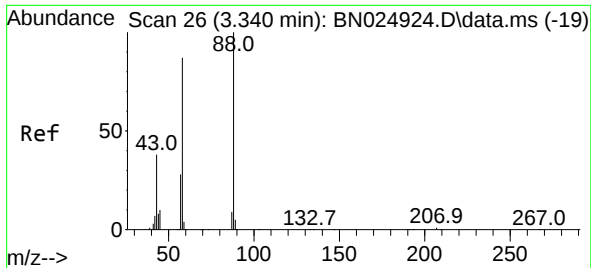

#2
 1,4-Dioxane
 Concen: 2.615 ng/uL
 RT: 3.340 min Scan# 20
 Delta R.T. 0.000 min
 Lab File: BN024937.D
 Acq: 15 Apr 2023 16:29

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ9

Tgt Ion: 88 Resp: 24467
 Ion Ratio Lower Upper
 88 100
 43 42.1 33.0 49.4
 58 85.4 72.3 108.5

