

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024876.D
 Acq On : 14 Apr 2023 01:52
 Operator : CG/JU
 Sample : PB152108BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	16	21	30	rBV	103111	168614	1.48%	0.156%
2	3.734	90	93	120	rBV	1526718	2670243	23.49%	2.464%
3	4.069	146	150	161	rVB	24377	40670	0.36%	0.038%
4	7.099	658	665	678	rBV	2040612	3132217	27.55%	2.891%
5	7.269	687	694	706	rVB	1569756	2419813	21.28%	2.233%
6	7.469	719	728	738	rBV	1806846	2943836	25.89%	2.717%
7	7.940	801	808	822	rVB	1169961	1827080	16.07%	1.686%
8	8.652	921	929	945	rBV	2217090	3507397	30.85%	3.237%
9	9.110	999	1007	1019	rBV	1895277	3062927	26.94%	2.827%
10	9.834	1121	1130	1144	rBV	1616646	2612768	22.98%	2.411%
11	10.369	1214	1221	1238	rBV	2177740	3622668	31.86%	3.343%
12	10.751	1278	1286	1295	rVB	1618770	2699944	23.75%	2.492%
13	10.893	1302	1310	1329	rBV	2589226	4399983	38.70%	4.061%
14	11.551	1417	1422	1428	rBV8	7208	15950	0.14%	0.015%
15	12.345	1551	1557	1563	rBV	33169	59356	0.52%	0.055%
16	13.998	1830	1838	1848	rBV	4096088	5718201	50.29%	5.277%
17	14.281	1879	1886	1896	rBV	4575593	6430374	56.56%	5.935%
18	14.587	1930	1938	1949	rBV	2458348	3520905	30.97%	3.249%
19	14.781	1963	1971	1991	rBV	2381835	3389454	29.81%	3.128%
20	15.575	2099	2106	2116	rBV	5651618	8078972	71.06%	7.456%
21	15.692	2120	2126	2140	rVV	2343518	3177609	27.95%	2.933%
22	15.816	2143	2147	2152	rVB2	27702	43339	0.38%	0.040%
23	16.363	2236	2240	2245	rBV5	7867	11619	0.10%	0.011%
24	17.333	2398	2405	2413	rBV	3039865	4200544	36.95%	3.877%
25	17.433	2415	2422	2436	rBV	6389932	9114961	80.17%	8.412%
26	19.292	2733	2738	2743	rBV3	69372	102373	0.90%	0.094%
27	19.363	2745	2750	2755	rBV	62952	93501	0.82%	0.086%
28	19.727	2805	2812	2824	rBV	7635324	10394199	91.42%	9.593%
29	21.521	3112	3117	3127	rBV	3513706	4629051	40.71%	4.272%
30	23.821	3500	3508	3523	rBV	6169234	11369540	100.00%	10.493%
31	23.980	3528	3535	3550	rVB2	2230549	4896980	43.07%	4.519%




Sum of corrected areas: 108355088

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024876.D
Acq On : 14 Apr 2023 01:52
Operator : CG/JU
Sample : PB152108BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK108

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

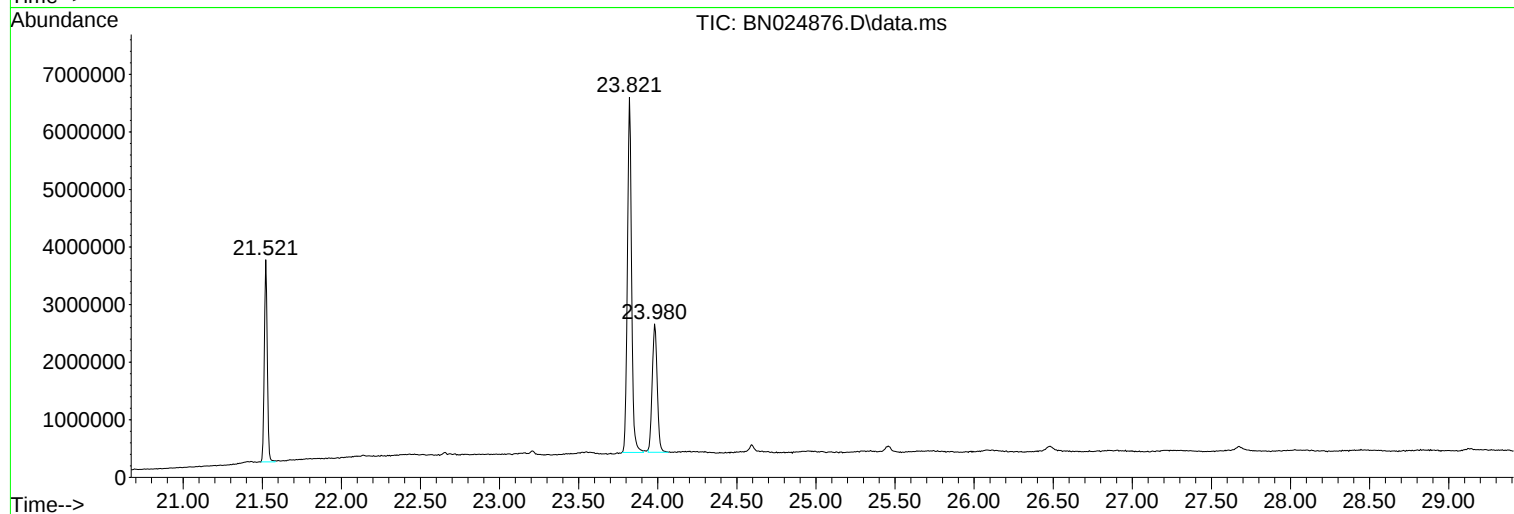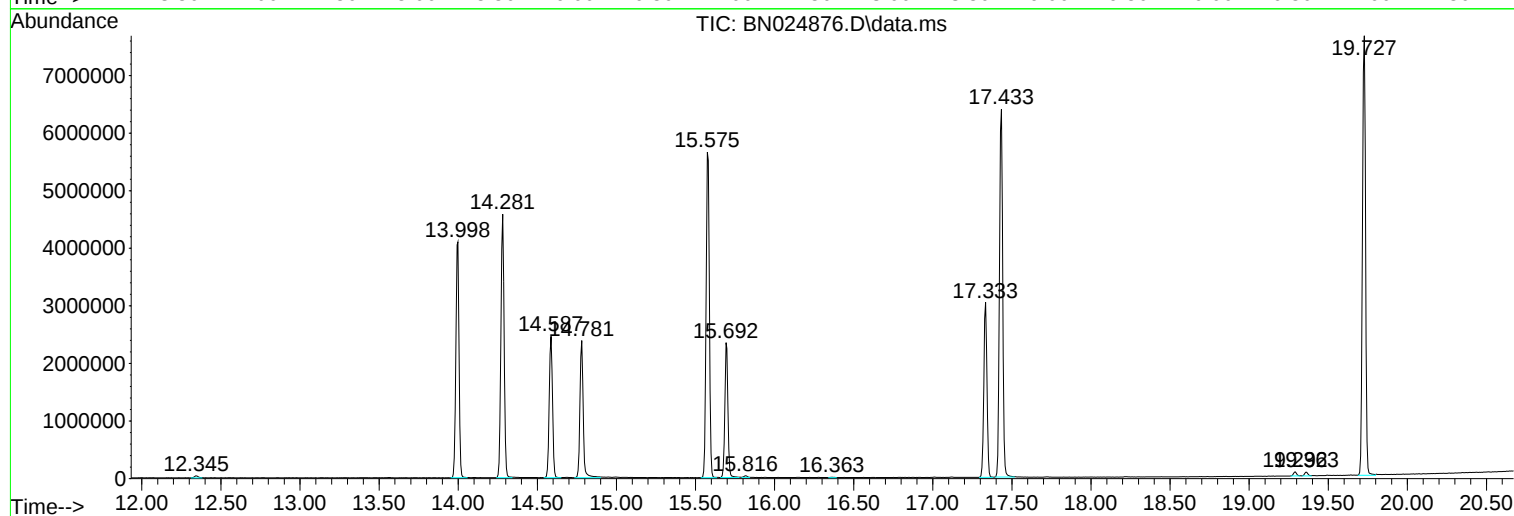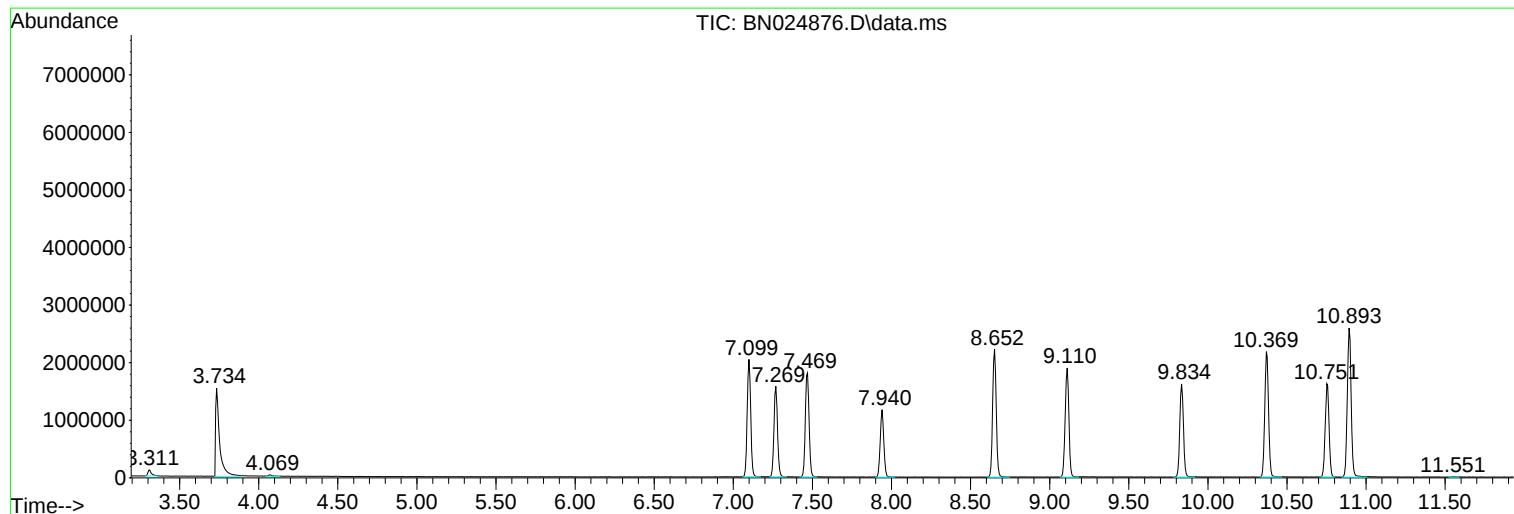

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024876.D
Acq On : 14 Apr 2023 01:52
Operator : CG/JU
Sample : PB152108BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK108

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024876.D
Acq On : 14 Apr 2023 01:52
Operator : CG/JU
Sample : PB152108BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK108

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc