

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024891.D
 Acq On : 14 Apr 2023 10:57
 Operator : CG/JU
 Sample : PB152118BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK118

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	17	21	29	rBV	85790	124159	1.44%	0.143%
2	3.734	91	93	116	rBV	1164111	1932278	22.38%	2.231%
3	4.069	146	150	157	rVB2	24078	36766	0.43%	0.042%
4	7.099	657	665	677	rBV	1473520	2299598	26.63%	2.655%
5	7.269	686	694	704	rVB	1102454	1769074	20.49%	2.043%
6	7.463	720	727	740	rBV	1397785	2234195	25.87%	2.580%
7	7.940	797	808	817	rBV	1139653	1869430	21.65%	2.159%
8	8.652	921	929	941	rBV	1712179	2748982	31.83%	3.174%
9	9.104	999	1006	1017	rBV	1363982	2275705	26.35%	2.628%
10	9.834	1121	1130	1143	rBV	1177541	1913662	22.16%	2.210%
11	10.369	1213	1221	1231	rBV	1642199	2669557	30.91%	3.083%
12	10.751	1277	1286	1296	rBV	1688623	2789040	32.30%	3.221%
13	10.893	1302	1310	1322	rBV	1788682	3071462	35.57%	3.547%
14	12.340	1552	1556	1563	rVB2	23834	37996	0.44%	0.044%
15	13.481	1743	1750	1755	rBV5	6745	12616	0.15%	0.015%
16	13.992	1831	1837	1845	rBV	2998287	4053692	46.94%	4.681%
17	14.281	1878	1886	1897	rBV	3159082	4736391	54.85%	5.469%
18	14.587	1931	1938	1947	rBV	2515602	3700168	42.85%	4.273%
19	14.775	1963	1970	1995	rBV	1580634	2354476	27.26%	2.719%
20	15.575	2097	2106	2114	rBV	4200877	5896994	68.29%	6.809%
21	15.692	2120	2126	2139	rBV	1689350	2220111	25.71%	2.564%
22	15.816	2143	2147	2152	rVB3	19019	28213	0.33%	0.033%
23	17.116	2363	2368	2376	rBV7	5428	9878	0.11%	0.011%
24	17.333	2398	2405	2411	rBV	3108562	4441820	51.43%	5.129%
25	17.428	2415	2421	2439	rVV2	4519350	6593453	76.35%	7.614%
26	17.716	2466	2470	2475	rVB7	5335	9040	0.10%	0.010%
27	19.286	2733	2737	2744	rVB3	55473	82743	0.96%	0.096%
28	19.363	2745	2750	2756	rVV	50408	75632	0.88%	0.087%
29	19.727	2806	2812	2823	rBV	5954997	7674124	88.86%	8.862%
30	21.527	3113	3118	3125	rBV	3891402	5051915	58.50%	5.834%
31	23.810	3498	3506	3519	rBV	3907855	8635802	100.00%	9.972%
32	23.968	3526	3533	3547	rVB2	2589348	5250560	60.80%	6.063%




Sum of corrected areas: 86599532

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024891.D
Acq On : 14 Apr 2023 10:57
Operator : CG/JU
Sample : PB152118BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

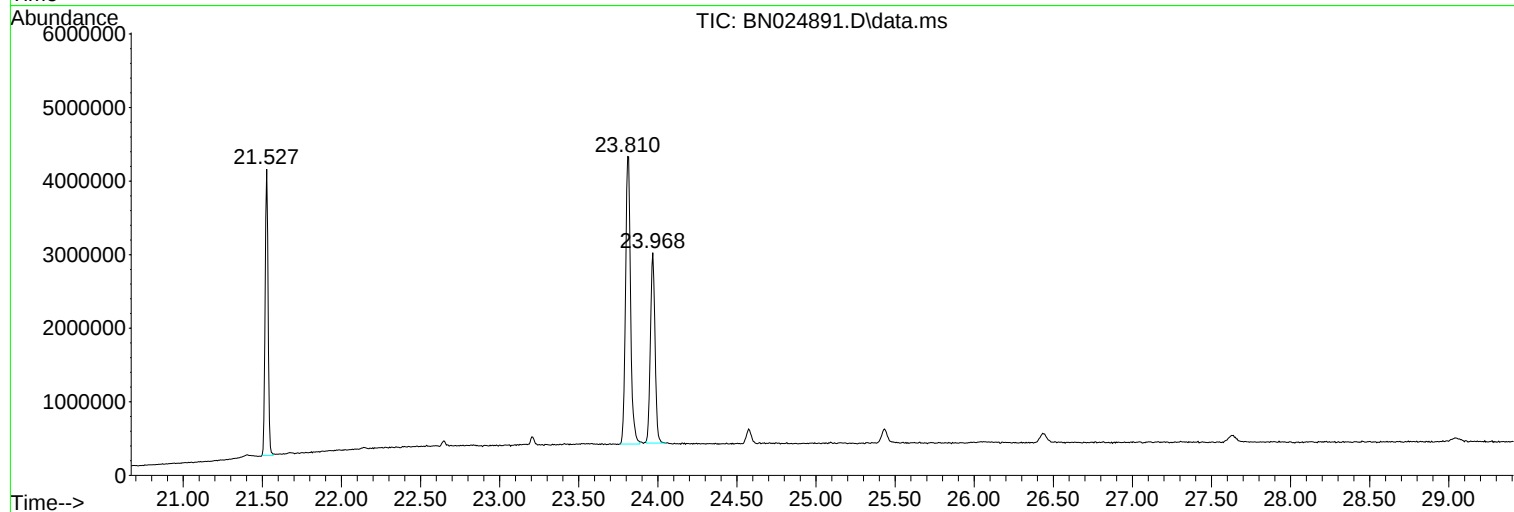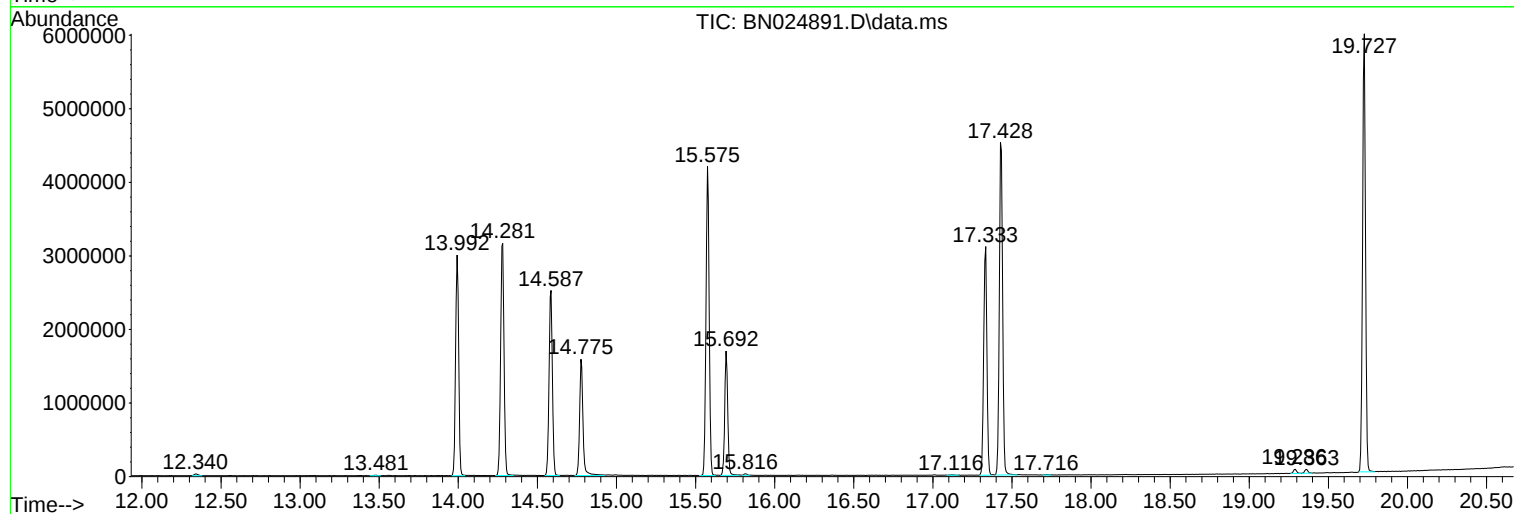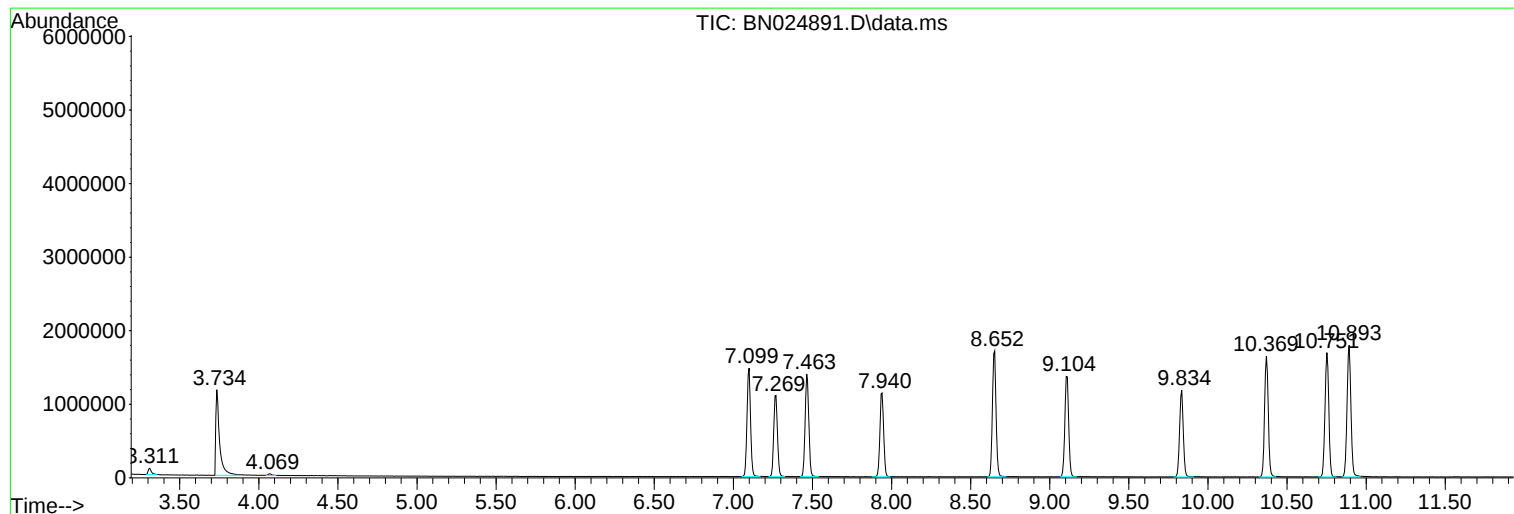

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024891.D
Acq On : 14 Apr 2023 10:57
Operator : CG/JU
Sample : PB152118BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024891.D
Acq On : 14 Apr 2023 10:57
Operator : CG/JU
Sample : PB152118BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc