

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024897.D
 Acq On : 14 Apr 2023 14:39
 Operator : CG/JU
 Sample : 02252-19
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	17	20	27	rBV	55212	80039	0.85%	0.099%
2	3.752	93	96	119	rBV	119597	249591	2.64%	0.310%
3	3.969	131	133	140	rVB6	8875	12911	0.14%	0.016%
4	4.069	146	150	158	rVB2	23090	39214	0.41%	0.049%
5	7.099	659	665	672	rBV	277454	436422	4.61%	0.541%
6	7.269	686	694	704	rBV	1128418	1815354	19.17%	2.252%
7	7.469	720	728	738	rBV	1078309	1729809	18.27%	2.146%
8	7.551	738	742	748	rVB7	7957	12928	0.14%	0.016%
9	7.940	799	808	817	rBV	1100899	1737677	18.35%	2.155%
10	8.651	922	929	941	rBV	827951	1303554	13.77%	1.617%
11	9.110	999	1007	1017	rBV	1456707	2368835	25.02%	2.938%
12	9.216	1021	1025	1030	rVV7	7810	16690	0.18%	0.021%
13	9.269	1030	1034	1041	rVB7	6551	11586	0.12%	0.014%
14	9.834	1122	1130	1141	rBV	1189755	1944734	20.54%	2.412%
15	10.369	1214	1221	1235	rBV	1561667	2577522	27.22%	3.197%
16	10.751	1278	1286	1297	rVB	1546194	2572875	27.17%	3.191%
17	10.892	1303	1310	1323	rBV	1032987	1720654	18.17%	2.134%
18	11.469	1403	1408	1415	rVB2	23427	40192	0.42%	0.050%
19	11.539	1415	1420	1427	rBV4	12876	23865	0.25%	0.030%
20	12.339	1550	1556	1563	rVB2	27655	49301	0.52%	0.061%
21	13.116	1682	1688	1693	rBV7	10563	17424	0.18%	0.022%
22	13.551	1756	1762	1768	rVB7	7721	16121	0.17%	0.020%
23	13.992	1831	1837	1845	rBV	3201425	4224917	44.62%	5.240%
24	14.280	1879	1886	1898	rBV	3419545	4916998	51.93%	6.099%
25	14.586	1931	1938	1949	rVB	2338290	3413968	36.06%	4.235%
26	14.780	1966	1971	1986	rBV	213861	397445	4.20%	0.493%
27	14.992	2003	2007	2013	rVB7	9907	14713	0.16%	0.018%
28	15.575	2098	2106	2114	rBV	4451809	6281042	66.34%	7.791%
29	15.692	2119	2126	2138	rVV	1817879	2407722	25.43%	2.986%
30	15.816	2141	2147	2154	rVB2	23904	48735	0.51%	0.060%
31	15.939	2163	2168	2174	rBV	65722	93043	0.98%	0.115%
32	16.280	2222	2226	2231	rBV6	9261	17046	0.18%	0.021%
33	17.010	2346	2350	2353	rBV5	6281	10555	0.11%	0.013%
34	17.074	2358	2361	2364	rBV4	9222	10830	0.11%	0.013%
35	17.122	2364	2369	2374	rVB4	7038	13106	0.14%	0.016%
36	17.333	2398	2405	2415	rBV	2889116	4119825	43.51%	5.110%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024897.D
 Acq On : 14 Apr 2023 14:39
 Operator : CG/JU
 Sample : 02252-19
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COMF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

37	17.433	2415	2422	2439	rVV	5224190	7544517	79.68%	9.358%
38	17.616	2447	2453	2456	rBV7	8028	15521	0.16%	0.019%
39	17.710	2466	2469	2474	rVB4	8962	12995	0.14%	0.016%
40	17.998	2514	2518	2523	rVB7	14132	23889	0.25%	0.030%
41	18.216	2550	2555	2562	rBV	129137	181162	1.91%	0.225%
42	18.298	2566	2569	2574	rVB	15152	24012	0.25%	0.030%
43	18.516	2603	2606	2610	rVB3	11382	14659	0.15%	0.018%
44	19.286	2733	2737	2743	rBV	68649	103375	1.09%	0.128%
45	19.363	2745	2750	2756	rBV	69512	114966	1.21%	0.143%
46	19.492	2769	2772	2777	rBV2	87661	108169	1.14%	0.134%
47	19.727	2806	2812	2820	rBV	6642068	8778028	92.71%	10.888%
48	21.221	3063	3066	3070	rBV3	91945	117176	1.24%	0.145%
49	21.521	3112	3117	3128	rBV	3605243	4651189	49.12%	5.769%
50	23.821	3500	3508	3525	rBV2	4725105	9468394	100.00%	11.744%
51	23.980	3528	3535	3548	rVB2	2142532	4716915	49.82%	5.851%




Sum of corrected areas: 80622210

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024897.D
Acq On : 14 Apr 2023 14:39
Operator : CG/JU
Sample : 02252-19
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

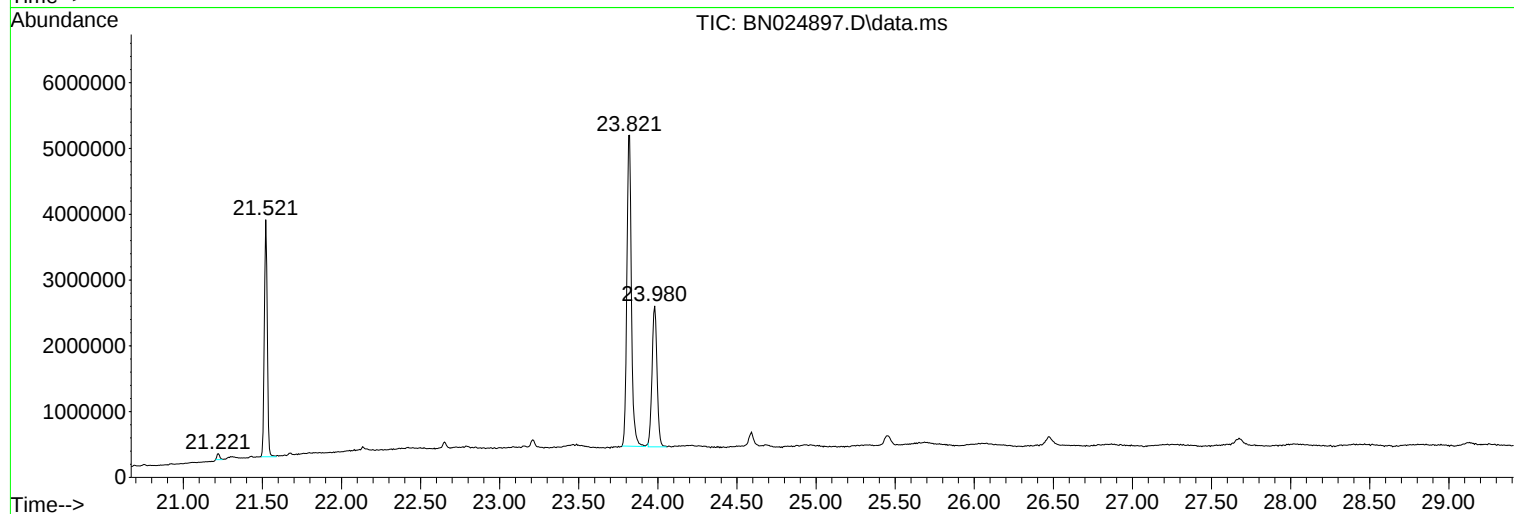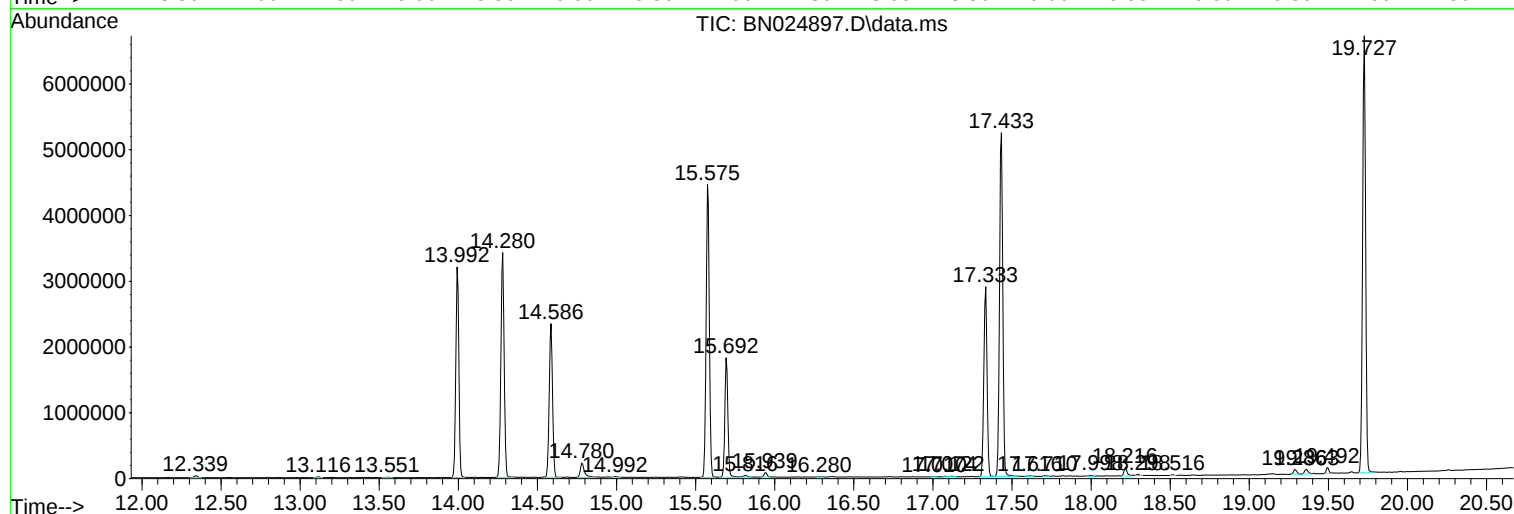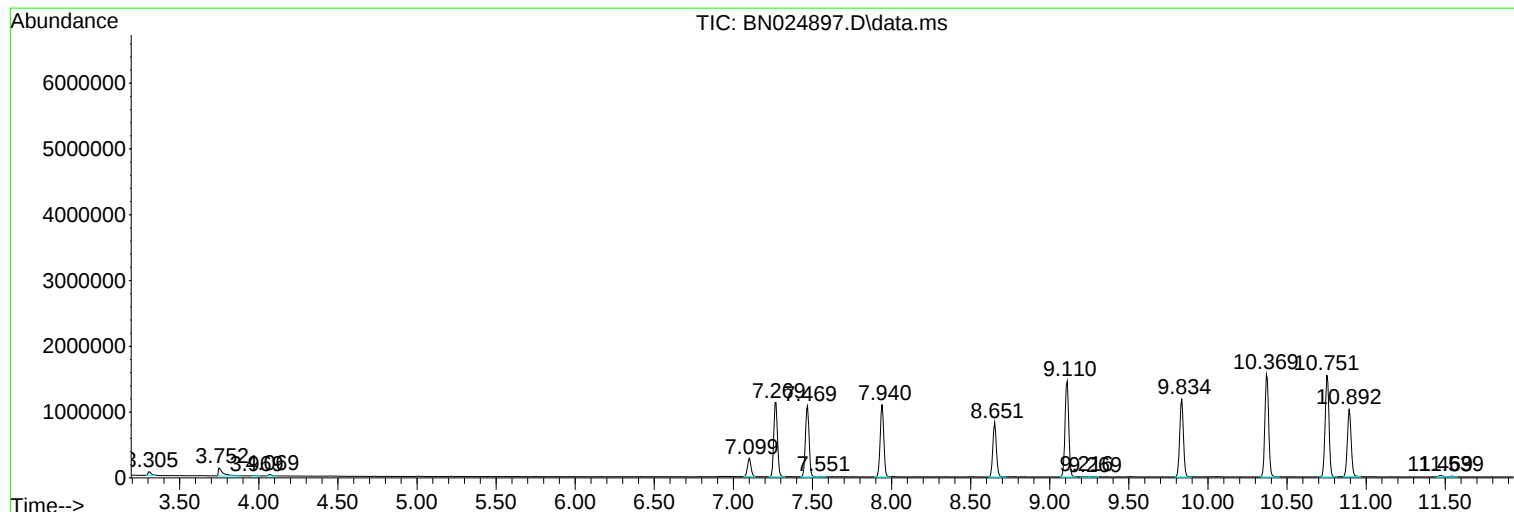

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024897.D
Acq On : 14 Apr 2023 14:39
Operator : CG/JU
Sample : 02252-19
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024897.D
Acq On : 14 Apr 2023 14:39
Operator : CG/JU
Sample : 02252-19
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COMF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc