

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024905.D
 Acq On : 14 Apr 2023 19:38
 Operator : CG/JU
 Sample : 02252-13
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COME9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024905.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	16	20	30	rBV	57175	94713	1.03%	0.121%
2	3.746	92	95	110	rBV	209705	391747	4.25%	0.501%
3	3.846	110	112	120	rVB5	19603	26449	0.29%	0.034%
4	4.070	145	150	159	rVB3	22237	36646	0.40%	0.047%
5	4.446	210	214	219	rVB8	6685	12026	0.13%	0.015%
6	7.099	659	665	675	rVB	262034	414149	4.49%	0.530%
7	7.264	687	693	704	rBV	1047124	1669669	18.12%	2.136%
8	7.464	718	727	739	rBV	971871	1570177	17.04%	2.008%
9	7.552	739	742	750	rVB7	5502	9418	0.10%	0.012%
10	7.822	785	788	794	rVB6	6462	12035	0.13%	0.015%
11	7.940	801	808	820	rBV	1122359	1941234	21.07%	2.483%
12	8.293	863	868	874	rBV3	24611	40610	0.44%	0.052%
13	8.652	922	929	939	rBV	690584	1096351	11.90%	1.402%
14	9.110	999	1007	1020	rBV	1311396	2192743	23.80%	2.805%
15	9.263	1030	1033	1039	rVB5	13129	19821	0.22%	0.025%
16	9.516	1071	1076	1080	rVB6	5182	10526	0.11%	0.013%
17	9.834	1122	1130	1139	rBV	1066735	1720546	18.67%	2.201%
18	10.369	1214	1221	1232	rBV	1388544	2266264	24.60%	2.899%
19	10.752	1278	1286	1294	rBV	1583021	2577176	27.97%	3.296%
20	10.893	1303	1310	1328	rVB	1047872	1804406	19.58%	2.308%
21	11.540	1414	1420	1428	rBV7	12484	27582	0.30%	0.035%
22	12.340	1551	1556	1562	rVB2	24273	40464	0.44%	0.052%
23	13.557	1757	1763	1767	rBV6	5477	9498	0.10%	0.012%
24	13.787	1797	1802	1811	rBV3	30839	44942	0.49%	0.057%
25	13.993	1829	1837	1846	rBV	2908553	3822224	41.48%	4.889%
26	14.281	1879	1886	1898	rBV	3045740	4382518	47.56%	5.606%
27	14.587	1929	1938	1948	rBV	2310772	3399148	36.89%	4.348%
28	14.781	1965	1971	1986	rBV	181469	331966	3.60%	0.425%
29	14.993	2003	2007	2013	rVB8	13240	22442	0.24%	0.029%
30	15.322	2058	2063	2068	rBV2	19808	28743	0.31%	0.037%
31	15.410	2073	2078	2079	rVV4	6382	10648	0.12%	0.014%
32	15.575	2099	2106	2113	rBV	4108238	5765010	62.57%	7.374%
33	15.692	2120	2126	2138	rBV	1626299	2100881	22.80%	2.687%
34	15.816	2142	2147	2153	rVB3	21674	35992	0.39%	0.046%
35	15.940	2162	2168	2181	rVB	451754	624273	6.78%	0.798%
36	16.287	2222	2227	2235	rVB6	12688	21146	0.23%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024905.D
 Acq On : 14 Apr 2023 19:38
 Operator : CG/JU
 Sample : 02252-13
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COME9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

37	16.363	2235	2240	2243	rBV7	5690	10640	0.12%	0.014%
38	16.504	2261	2264	2273	rVB7	13414	26193	0.28%	0.034%
39	16.798	2309	2314	2317	rBV7	6292	10208	0.11%	0.013%
40	16.869	2322	2326	2330	rVB3	14428	19626	0.21%	0.025%
41	17.010	2347	2350	2354	rVB5	7924	9332	0.10%	0.012%
42	17.081	2358	2362	2365	rBV4	11256	15753	0.17%	0.020%
43	17.334	2398	2405	2411	rBV	2913807	4090410	44.39%	5.232%
44	17.434	2415	2422	2437	rVV	4774369	6750887	73.27%	8.635%
45	17.710	2466	2469	2475	rVB6	11810	18709	0.20%	0.024%
46	17.816	2484	2487	2492	rBV7	10139	15165	0.16%	0.019%
47	17.998	2513	2518	2523	rVB2	116535	147899	1.61%	0.189%
48	18.216	2551	2555	2562	rBV	164691	231265	2.51%	0.296%
49	18.292	2566	2568	2572	rVB	11820	15283	0.17%	0.020%
50	18.563	2611	2614	2620	rBV8	6880	12210	0.13%	0.016%
51	19.139	2707	2712	2715	rBV3	79982	113896	1.24%	0.146%
52	19.169	2715	2717	2721	rVB2	62720	64421	0.70%	0.082%
53	19.292	2733	2738	2743	rBV3	84959	143226	1.55%	0.183%
54	19.357	2745	2749	2753	rBV	72506	116200	1.26%	0.149%
55	19.492	2768	2772	2778	rBV3	102296	131894	1.43%	0.169%
56	19.722	2805	2811	2825	rBV	6244026	8457348	91.79%	10.818%
57	21.216	3061	3065	3070	rBV2	104031	173911	1.89%	0.222%
58	21.516	3111	3116	3124	rBV	3795549	4753149	51.59%	6.080%
59	23.816	3499	3507	3519	rBV2	4207409	9213823	100.00%	11.785%
60	23.969	3526	3533	3544	rVB2	2658036	5066061	54.98%	6.480%




Sum of corrected areas: 78181692

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024905.D
Acq On : 14 Apr 2023 19:38
Operator : CG/JU
Sample : 02252-13
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COME9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

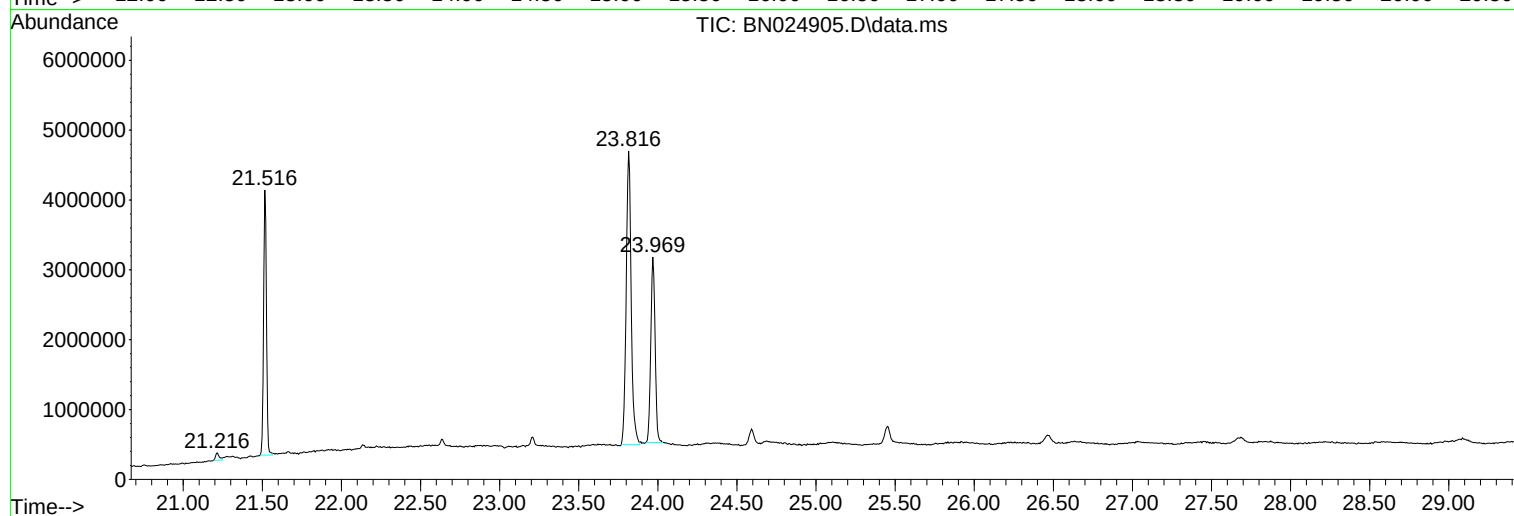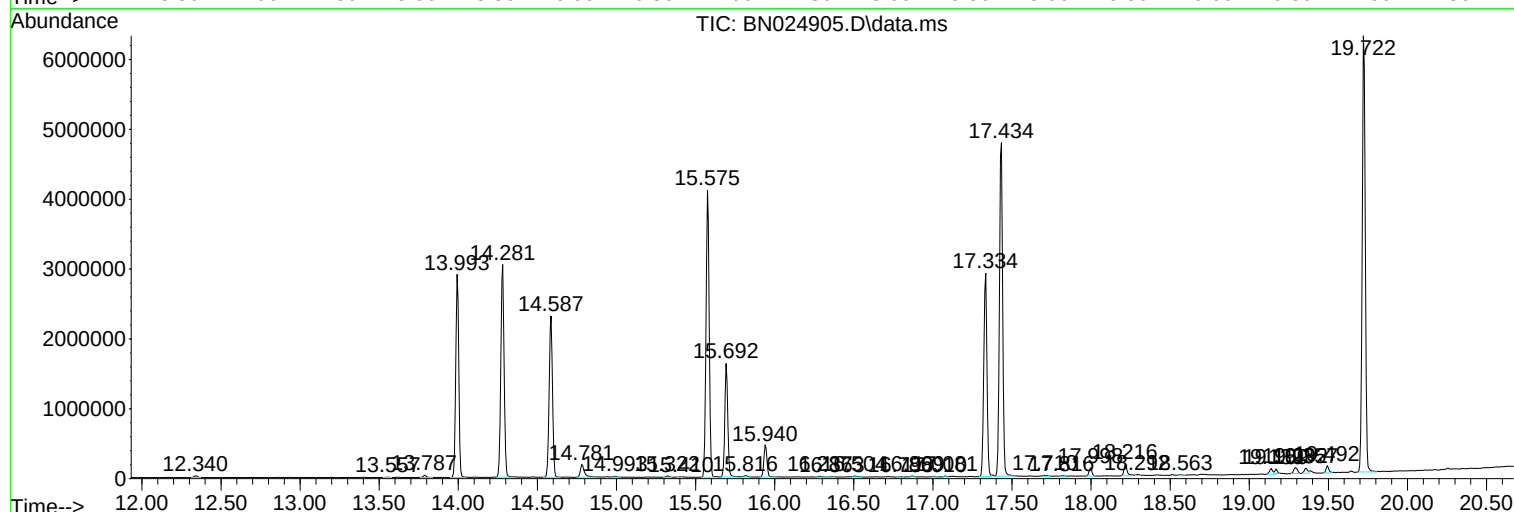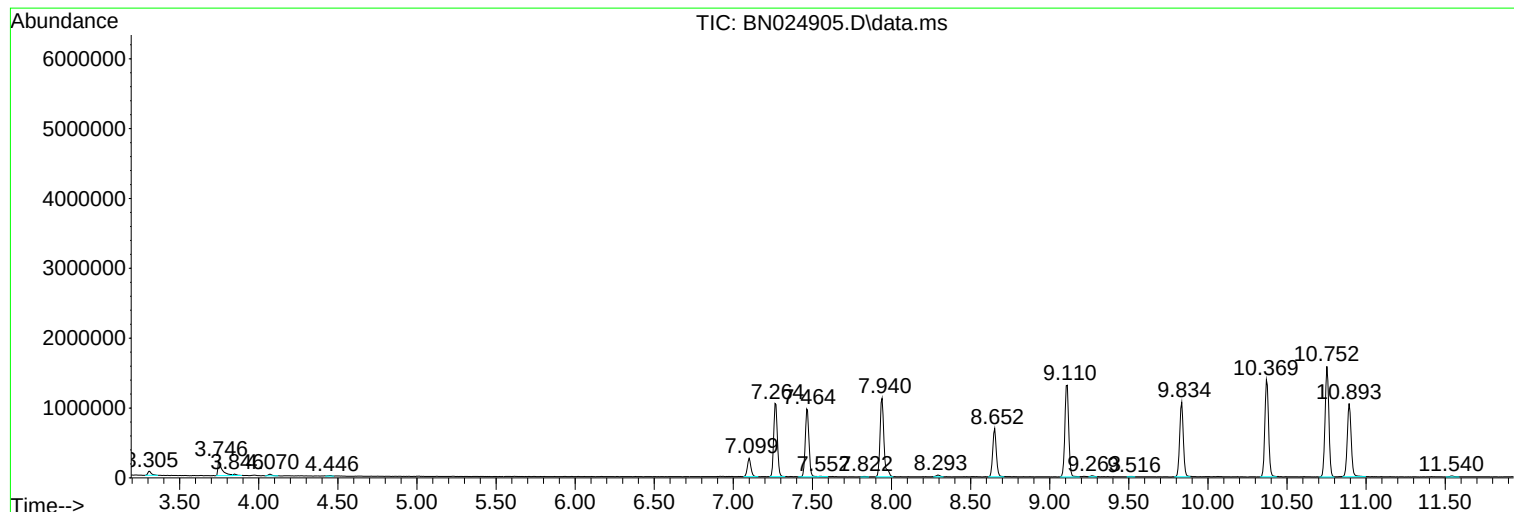

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024905.D
Acq On : 14 Apr 2023 19:38
Operator : CG/JU
Sample : 02252-13
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COME9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.940	3.67 ng/ul	624273	Acenaphthene-d10	14.587

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	97
3			Benzophenone	182	C13H10O	000119-61-9	97
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	91

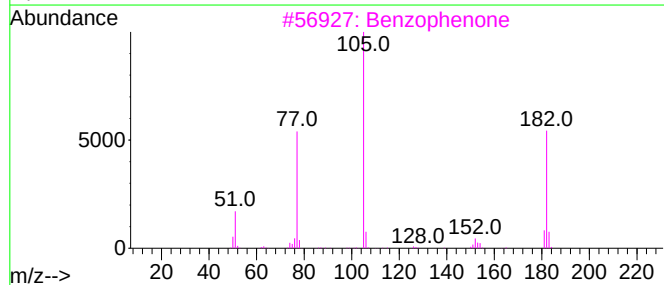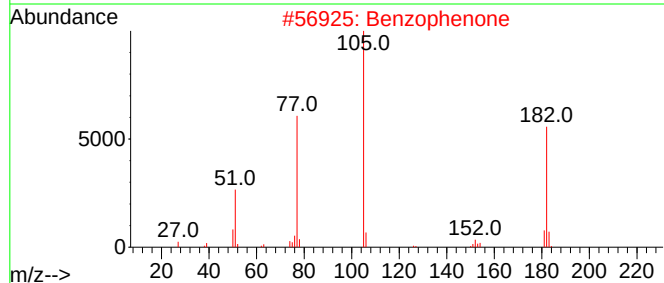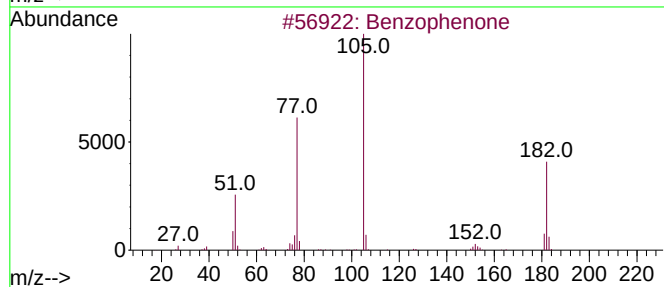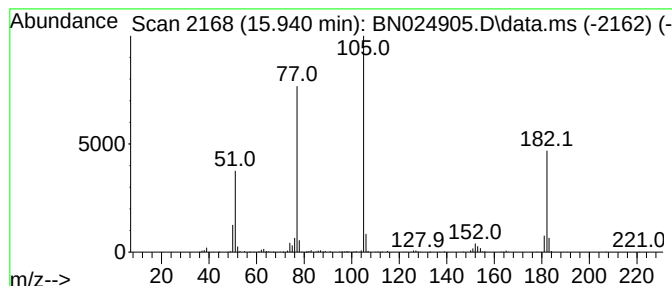

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024905.D
Acq On : 14 Apr 2023 19:38
Operator : CG/JU
Sample : 02252-13
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0ME9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.940	3.7	ng/u1	624273	3	14.587	3399150	20.0