

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024909.D
 Acq On : 14 Apr 2023 22:44
 Operator : CG/JU
 Sample : PB152090BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK090

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	16	20	32	rVB	93617	146659	1.68%	0.159%
2	3.734	90	93	119	rBV	1287379	2167694	24.81%	2.345%
3	4.070	146	150	158	rVB	23604	35219	0.40%	0.038%
4	5.222	342	346	353	rBV7	7990	14099	0.16%	0.015%
5	7.099	658	665	679	rVB	1668278	2561660	29.32%	2.771%
6	7.264	686	693	703	rBV	1264810	1958788	22.42%	2.119%
7	7.464	719	727	741	rBV	1556373	2477564	28.35%	2.680%
8	7.940	800	808	818	rBV	1133585	1857215	21.25%	2.009%
9	8.652	919	929	947	rBV	1934820	3090657	35.37%	3.343%
10	9.105	995	1006	1018	rBV	1571852	2604380	29.81%	2.817%
11	9.834	1121	1130	1142	rBV	1318596	2195368	25.12%	2.375%
12	10.369	1213	1221	1236	rBV	1881932	3036682	34.75%	3.285%
13	10.752	1276	1286	1294	rBV	1707949	2832283	32.41%	3.064%
14	10.893	1302	1310	1329	rBV	2035530	3418261	39.12%	3.697%
15	11.546	1416	1421	1427	rBV7	6997	14728	0.17%	0.016%
16	12.340	1551	1556	1565	rBV2	32076	54983	0.63%	0.059%
17	13.481	1745	1750	1755	rVB3	11526	15780	0.18%	0.017%
18	13.993	1830	1837	1848	rBV	3285964	4482894	51.30%	4.849%
19	14.275	1878	1885	1896	rBV	3590874	5266028	60.27%	5.696%
20	14.587	1931	1938	1946	rBV	2511543	3679484	42.11%	3.980%
21	14.781	1964	1971	1995	rBV	1759659	2580901	29.54%	2.792%
22	14.993	2004	2007	2013	rVB7	7164	11694	0.13%	0.013%
23	15.575	2095	2106	2114	rBV	4895155	6839972	78.28%	7.399%
24	15.692	2120	2126	2137	rBV	1831920	2345599	26.84%	2.537%
25	15.816	2143	2147	2151	rVB3	22732	32474	0.37%	0.035%
26	17.122	2364	2369	2372	rBV2	7788	9558	0.11%	0.010%
27	17.334	2398	2405	2414	rBV	3022382	4412565	50.50%	4.773%
28	17.428	2414	2421	2433	rBV2	5004590	7141568	81.73%	7.725%
29	17.710	2467	2469	2477	rVB3	5528	10291	0.12%	0.011%
30	19.286	2733	2737	2744	rBV3	60244	84453	0.97%	0.091%
31	19.357	2745	2749	2754	rVV	62190	77629	0.89%	0.084%
32	19.722	2805	2811	2822	rBV	6723355	8737822	100.00%	9.452%
33	21.516	3111	3116	3123	rBV	3944931	4833037	55.31%	5.228%
34	23.816	3499	3507	3520	rBV2	4323101	8454597	96.76%	9.145%
35	23.963	3526	3532	3544	rVB	2570370	4965959	56.83%	5.372%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024909.D
Acq On : 14 Apr 2023 22:44
Operator : CG/JU
Sample : PB152090BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK090

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Title : SVOA CALIBRATION




Sum of corrected areas: 92448545

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024909.D
Acq On : 14 Apr 2023 22:44
Operator : CG/JU
Sample : PB152090BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

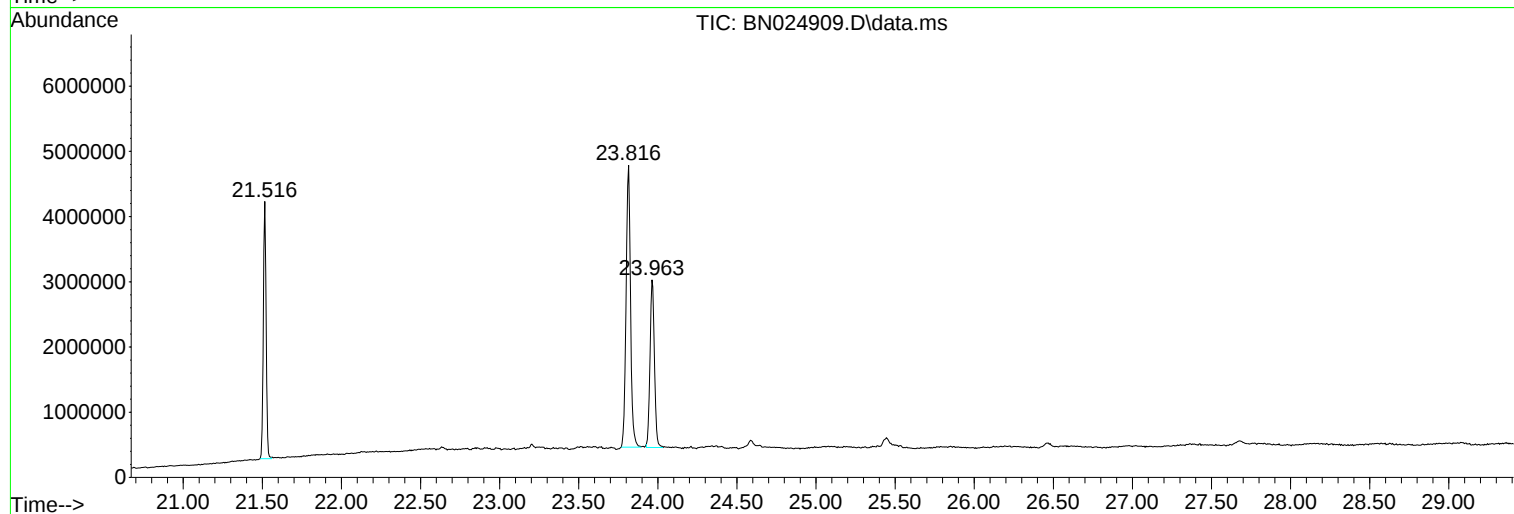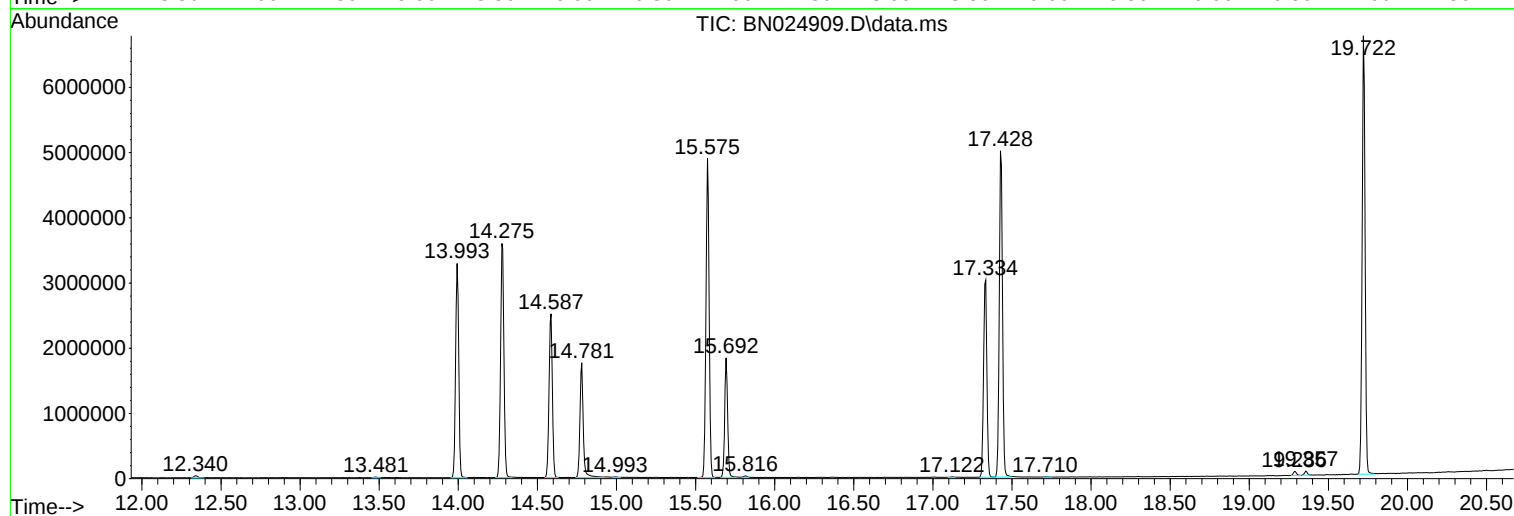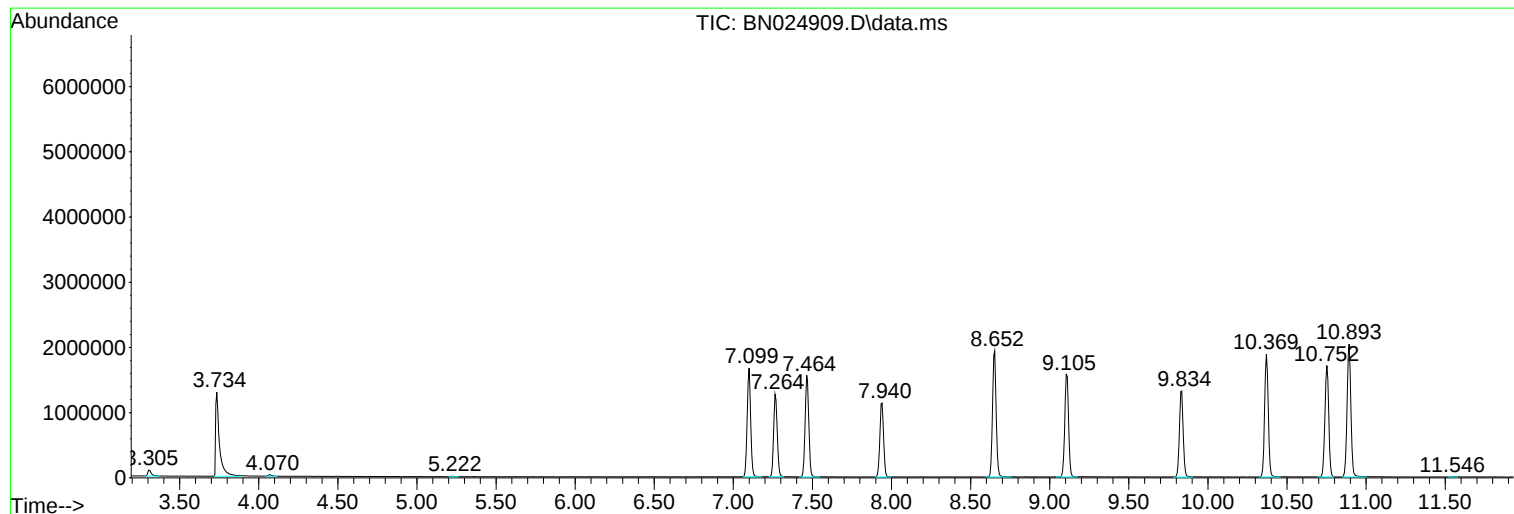

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024909.D
Acq On : 14 Apr 2023 22:44
Operator : CG/JU
Sample : PB152090BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024909.D
Acq On : 14 Apr 2023 22:44
Operator : CG/JU
Sample : PB152090BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc