

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024921.D
 Acq On : 15 Apr 2023 06:08
 Operator : CG/JU
 Sample : PB152117BL
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK117

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	16	20	35	rVB	104267	171568	1.92%	0.192%
2	3.752	93	96	114	rBV	151989	333573	3.74%	0.374%
3	4.069	145	150	155	rBV2	21243	34332	0.38%	0.039%
4	5.187	336	340	346	rBV6	7619	15515	0.17%	0.017%
5	7.099	658	665	676	rBV	1720208	2747903	30.81%	3.083%
6	7.263	684	693	705	rBV	1429370	2203944	24.71%	2.473%
7	7.463	720	727	745	rBV	1771353	2768357	31.04%	3.106%
8	7.934	799	807	818	rBV	1216068	1953942	21.91%	2.192%
9	8.646	919	928	942	rBV	2103911	3401647	38.14%	3.816%
10	9.104	997	1006	1019	rBV	1766967	2829270	31.72%	3.174%
11	9.828	1122	1129	1141	rBV	1449627	2341369	26.25%	2.627%
12	10.369	1213	1221	1237	rBV	1951376	3331790	37.36%	3.738%
13	10.751	1278	1286	1294	rBV	1717853	2895476	32.47%	3.248%
14	10.898	1306	1311	1319	rBV3	22475	48164	0.54%	0.054%
15	12.287	1542	1547	1551	rBV4	8853	14272	0.16%	0.016%
16	12.340	1551	1556	1564	rVB	32018	57136	0.64%	0.064%
17	12.563	1588	1594	1597	rBV7	5067	10260	0.12%	0.012%
18	13.992	1830	1837	1848	rBV	3476620	4755795	53.33%	5.335%
19	14.275	1878	1885	1898	rBV2	3248421	4725296	52.98%	5.301%
20	14.581	1930	1937	1946	rBV	2445460	3553168	39.84%	3.986%
21	14.781	1964	1971	1993	rBV	1740764	2686155	30.12%	3.014%
22	14.939	1996	1998	2003	rVV6	7765	13248	0.15%	0.015%
23	14.986	2003	2006	2011	rVB7	7274	10577	0.12%	0.012%
24	15.575	2099	2106	2113	rBV	4778264	6588621	73.88%	7.392%
25	15.692	2120	2126	2138	rBV	1920253	2518187	28.24%	2.825%
26	15.810	2142	2146	2152	rVB2	22367	33730	0.38%	0.038%
27	16.081	2188	2192	2197	rBV4	17588	24797	0.28%	0.028%
28	16.351	2235	2238	2244	rBV7	6147	10357	0.12%	0.012%
29	17.327	2397	2404	2413	rBV	3090025	4296522	48.18%	4.820%
30	17.427	2414	2421	2436	rVV	5240105	7202410	80.76%	8.080%
31	17.998	2514	2518	2522	rVB6	10421	13767	0.15%	0.015%
32	19.286	2732	2737	2742	rBV3	69673	100202	1.12%	0.112%
33	19.357	2744	2749	2754	rBV	60549	86543	0.97%	0.097%
34	19.721	2805	2811	2820	rBV	6596264	8622830	96.69%	9.674%
35	21.515	3111	3116	3125	rBV	3816269	4947907	55.48%	5.551%
36	23.804	3497	3505	3520	rVB	3975257	8918203	100.00%	10.005%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024921.D
Acq On : 15 Apr 2023 06:08
Operator : CG/JU
Sample : PB152117BL
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK117

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Title : SVOA CALIBRATION

37	23.968	3527	3533	3543	rVB	2509339	4868261	54.59%	5.462%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 89135094

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024921.D
Acq On : 15 Apr 2023 06:08
Operator : CG/JU
Sample : PB152117BL
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK117

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

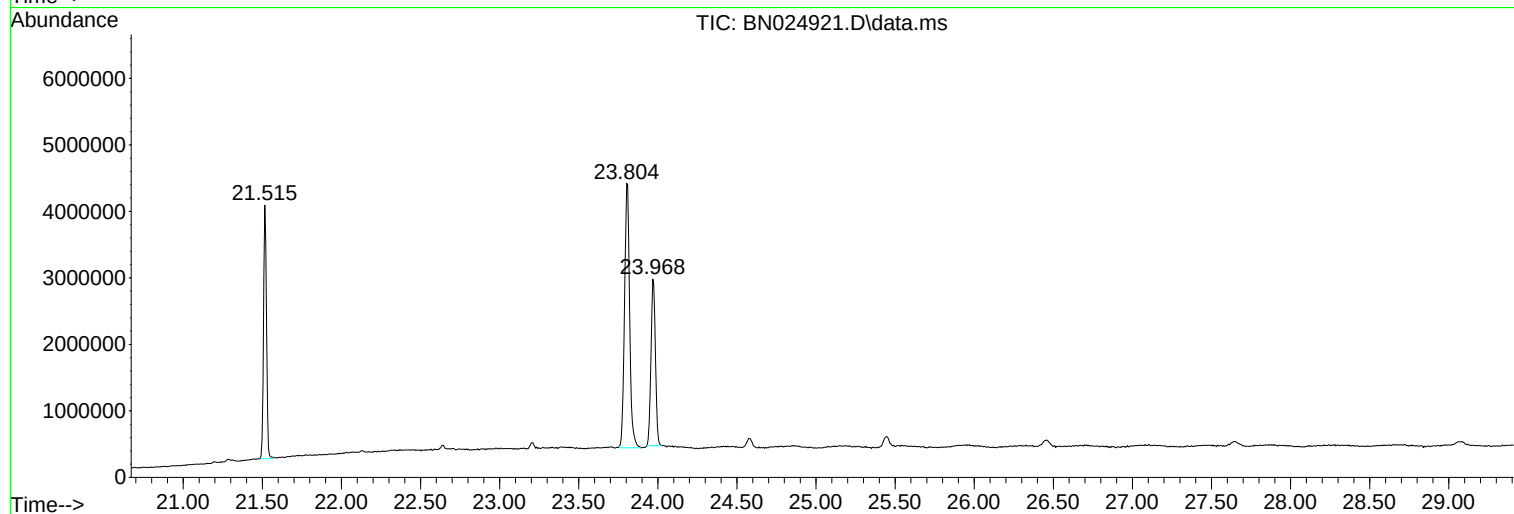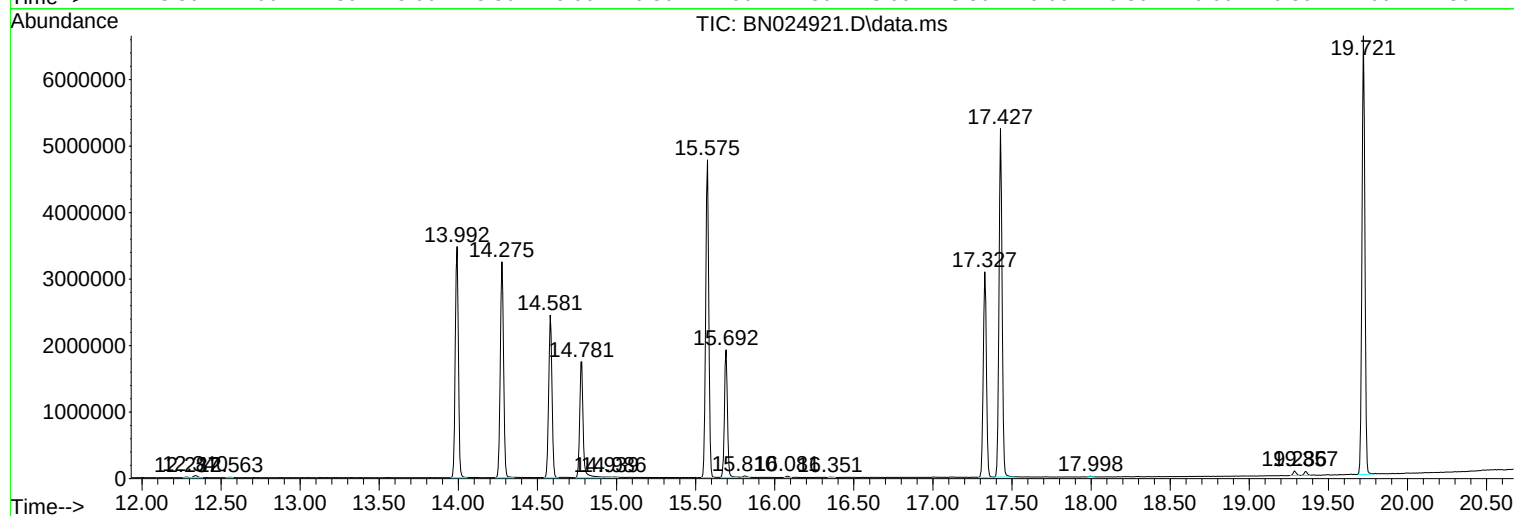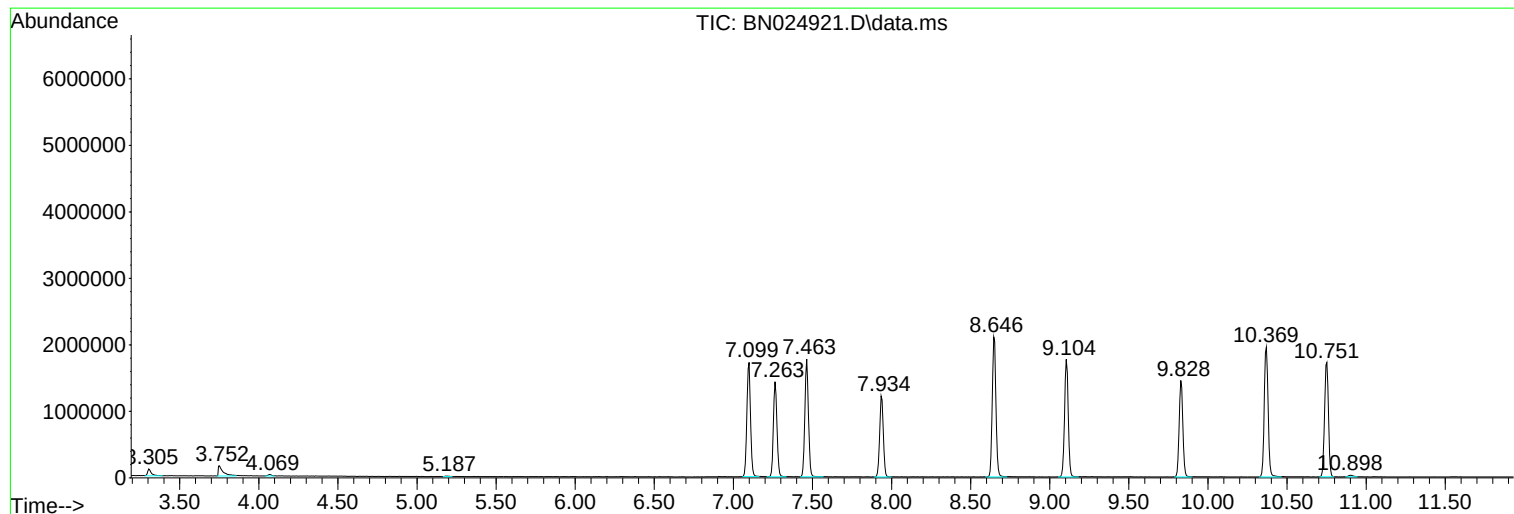

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024921.D
Acq On : 15 Apr 2023 06:08
Operator : CG/JU
Sample : PB152117BL
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK117

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024921.D
Acq On : 15 Apr 2023 06:08
Operator : CG/JU
Sample : PB152117BL
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK117

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------