

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024923.D
 Acq On : 15 Apr 2023 07:21
 Operator : CG/JU
 Sample : PB152131BL
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK131

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	17	20	33	rVB	94807	151470	1.76%	0.165%
2	3.758	96	97	118	rBV	69673	167194	1.94%	0.182%
3	4.070	144	150	159	rBV	25265	43365	0.50%	0.047%
4	4.528	224	228	234	rVB3	16418	25264	0.29%	0.028%
5	5.193	336	341	346	rVB5	11662	20067	0.23%	0.022%
6	7.099	657	665	678	rBV	1587634	2590821	30.12%	2.828%
7	7.263	685	693	704	rBV	1302464	1989793	23.13%	2.172%
8	7.463	718	727	743	rBV	1612509	2531390	29.43%	2.763%
9	7.934	798	807	816	rBV	1388287	2223724	25.85%	2.427%
10	8.646	921	928	943	rBV	1964763	3121882	36.30%	3.407%
11	9.105	998	1006	1017	rBV	1603624	2553467	29.69%	2.787%
12	9.828	1122	1129	1141	rBV	1337169	2155269	25.06%	2.352%
13	10.369	1213	1221	1237	rBV	1822948	3080216	35.81%	3.362%
14	10.752	1278	1286	1294	rBV	1941519	3305869	38.44%	3.608%
15	10.899	1302	1311	1323	rBV3	37030	112802	1.31%	0.123%
16	11.052	1332	1337	1342	rBV7	5966	10353	0.12%	0.011%
17	12.281	1541	1546	1549	rBV5	5593	9674	0.11%	0.011%
18	12.334	1549	1555	1562	rVB2	29588	51883	0.60%	0.057%
19	13.993	1828	1837	1849	rBV	3322337	4639913	53.95%	5.064%
20	14.275	1878	1885	1896	rBV	3227969	4612881	53.63%	5.035%
21	14.581	1927	1937	1945	rBV	3090268	4451833	51.76%	4.859%
22	14.775	1962	1970	1990	rBV	1826142	2706720	31.47%	2.954%
23	14.992	2003	2007	2011	rVB5	9111	11024	0.13%	0.012%
24	15.575	2098	2106	2115	rBV	4690798	6657361	77.40%	7.266%
25	15.692	2119	2126	2137	rVV	1912658	2567583	29.85%	2.802%
26	15.810	2140	2146	2155	rVB2	24181	48713	0.57%	0.053%
27	16.081	2188	2192	2196	rVV2	13904	17329	0.20%	0.019%
28	17.116	2363	2368	2375	rVB5	6878	11768	0.14%	0.013%
29	17.328	2397	2404	2414	rBV	3933525	5422868	63.05%	5.919%
30	17.428	2414	2421	2435	rVV	5312847	7356998	85.54%	8.030%
31	17.998	2513	2518	2521	rBV4	14675	20354	0.24%	0.022%
32	19.286	2732	2737	2744	rBV2	68590	104819	1.22%	0.114%
33	19.357	2744	2749	2754	rBV	63526	93224	1.08%	0.102%
34	19.722	2805	2811	2823	rBV	6580129	8601135	100.00%	9.388%
35	21.522	3112	3117	3129	rBV2	4743173	6016293	69.95%	6.567%
36	23.821	3500	3508	3521	rBV	3956155	8249190	95.91%	9.004%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024923.D
Acq On : 15 Apr 2023 07:21
Operator : CG/JU
Sample : PB152131BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK131

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Title : SVOA CALIBRATION

37 23.968 3526 3533 3547 rVB2 2980761 5885804 68.43% 6.424%




Sum of corrected areas: 91620313

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024923.D
Acq On : 15 Apr 2023 07:21
Operator : CG/JU
Sample : PB152131BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK131

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

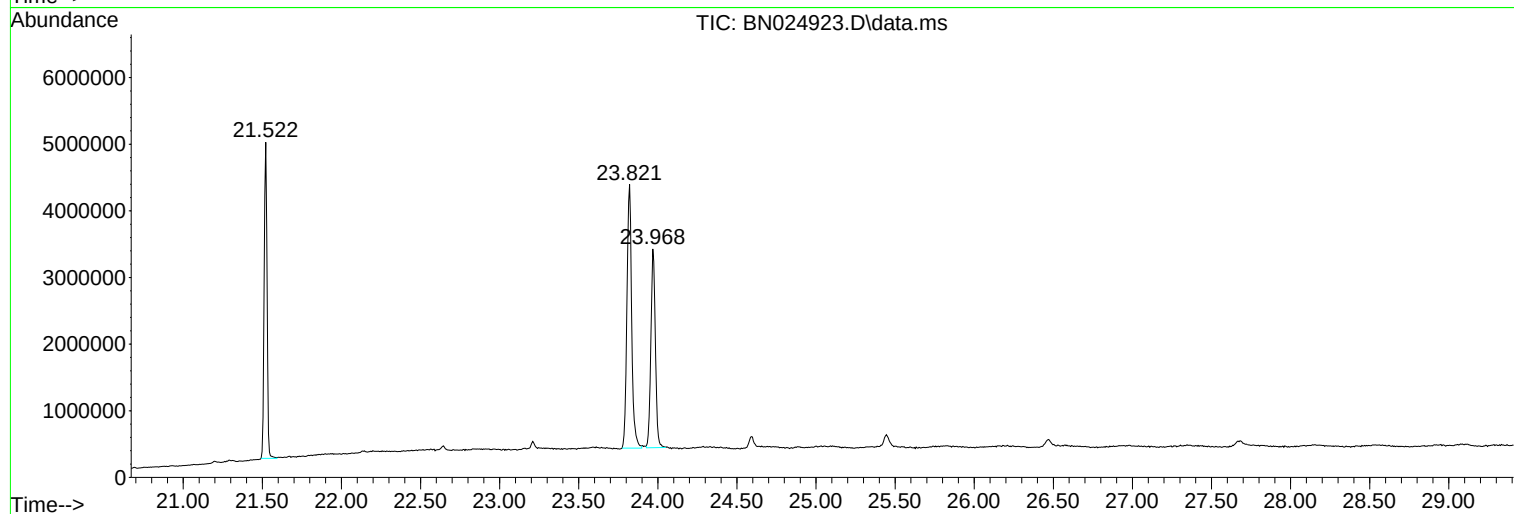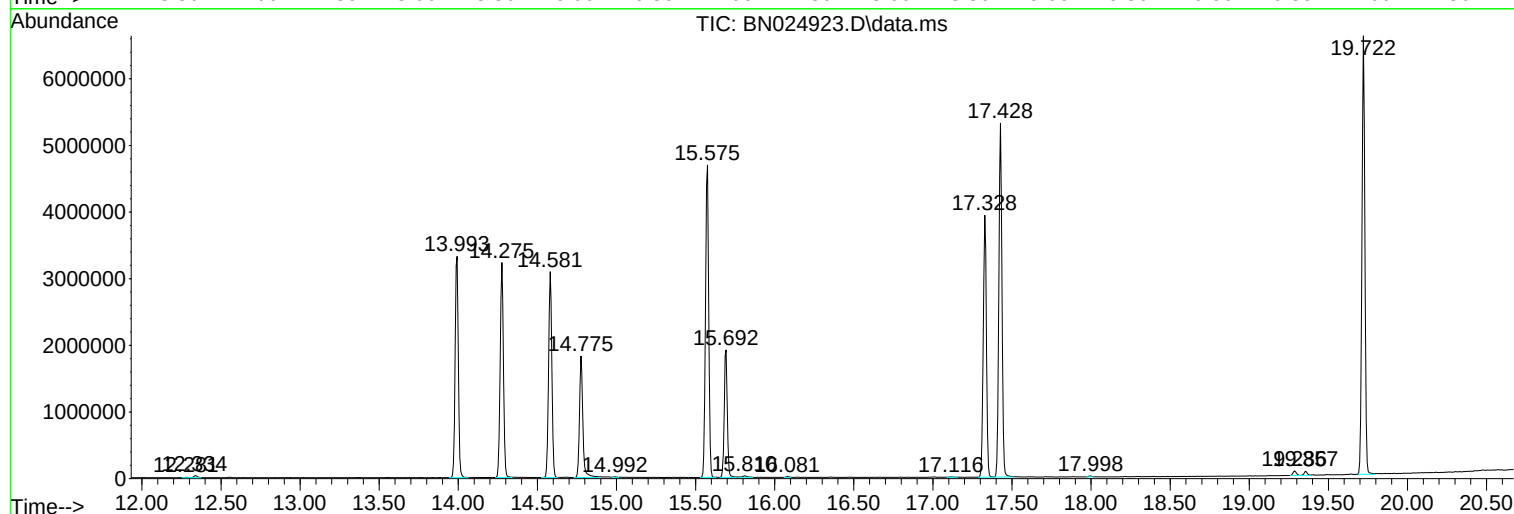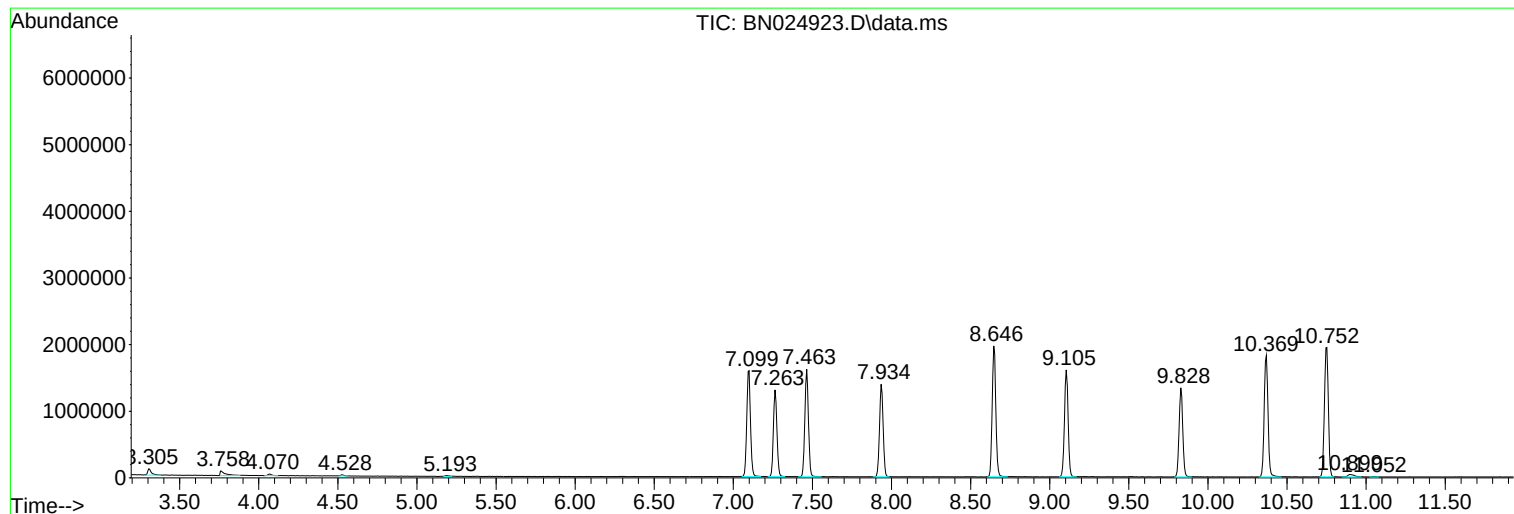

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024923.D
Acq On : 15 Apr 2023 07:21
Operator : CG/JU
Sample : PB152131BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK131

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024923.D
Acq On : 15 Apr 2023 07:21
Operator : CG/JU
Sample : PB152131BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK131

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------