

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024925.D
 Acq On : 15 Apr 2023 09:11
 Operator : CG/JU
 Sample : PB152119BL
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK119

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	16	20	32	rVB	95586	139077	1.55%	0.142%
2	3.734	89	93	113	rBV	1213028	2119751	23.70%	2.168%
3	4.069	145	150	159	rVB	26235	44468	0.50%	0.045%
4	7.093	657	664	677	rBV	1658051	2634143	29.45%	2.694%
5	7.263	686	693	703	rBV	1303410	1994495	22.30%	2.040%
6	7.463	720	727	740	rBV	1628288	2553482	28.55%	2.612%
7	7.934	799	807	815	rBV	1339769	2138788	23.91%	2.188%
8	8.646	921	928	939	rBV	2005203	3132113	35.01%	3.204%
9	9.104	996	1006	1017	rBV	1633197	2616390	29.25%	2.676%
10	9.828	1120	1129	1140	rBV	1392404	2199061	24.58%	2.249%
11	10.369	1213	1221	1236	rBV	1833169	3092770	34.57%	3.163%
12	10.746	1277	1285	1295	rVB	1888303	3211101	35.90%	3.284%
13	10.887	1302	1309	1328	rBV	2006230	3494825	39.07%	3.575%
14	12.340	1549	1556	1566	rVB2	29599	52048	0.58%	0.053%
15	13.469	1744	1748	1753	rBV4	8247	12214	0.14%	0.012%
16	13.992	1830	1837	1850	rBV	3355694	4732674	52.91%	4.841%
17	14.275	1878	1885	1902	rBV2	3786521	5491453	61.39%	5.617%
18	14.581	1930	1937	1947	rBV	3027107	4311101	48.19%	4.409%
19	14.687	1949	1955	1960	rVB9	4230	10030	0.11%	0.010%
20	14.775	1963	1970	1992	rBV	1833970	2719135	30.40%	2.781%
21	14.986	2003	2006	2012	rVB8	6595	12339	0.14%	0.013%
22	15.575	2098	2106	2113	rBV	4844599	6847867	76.55%	7.004%
23	15.692	2120	2126	2137	rBV	2007889	2641797	29.53%	2.702%
24	15.810	2143	2146	2153	rVB2	23964	32386	0.36%	0.033%
25	17.122	2363	2369	2372	rBV4	7874	14276	0.16%	0.015%
26	17.328	2397	2404	2414	rBV	3858650	5242332	58.60%	5.362%
27	17.428	2414	2421	2433	rVV	5609633	7623022	85.22%	7.797%
28	19.286	2732	2737	2744	rBV2	63556	96124	1.07%	0.098%
29	19.357	2744	2749	2754	rBV	62165	87733	0.98%	0.090%
30	19.722	2805	2811	2822	rBV	6774477	8945249	100.00%	9.149%
31	21.516	3111	3116	3125	rBV	4565248	5682917	63.53%	5.813%
32	23.792	3496	3503	3521	rVB2	4157212	8489181	94.90%	8.683%
33	23.951	3523	3530	3543	rVB2	2603455	5355573	59.87%	5.478%




Sum of corrected areas: 97769915

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024925.D
Acq On : 15 Apr 2023 09:11
Operator : CG/JU
Sample : PB152119BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK119

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

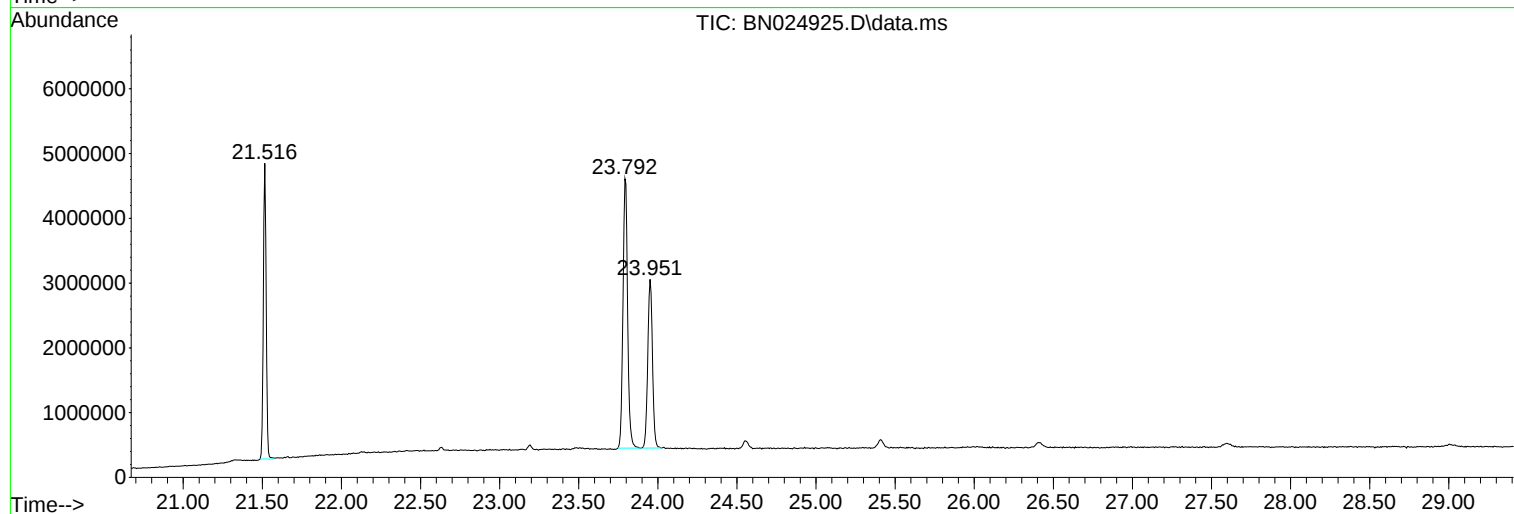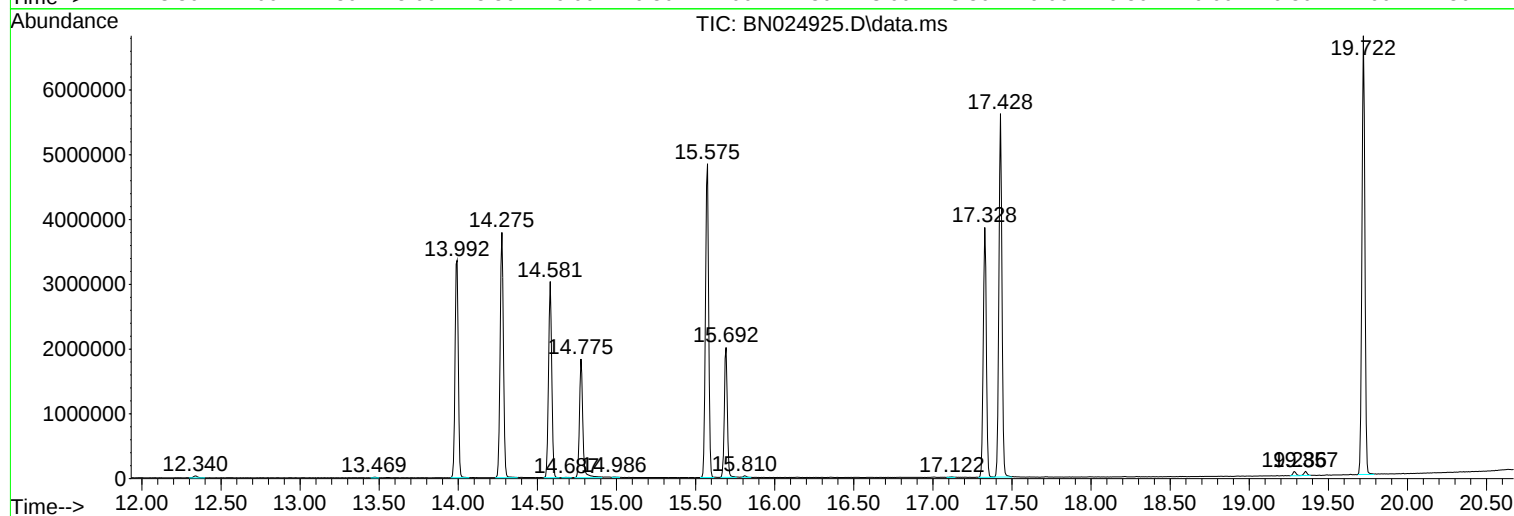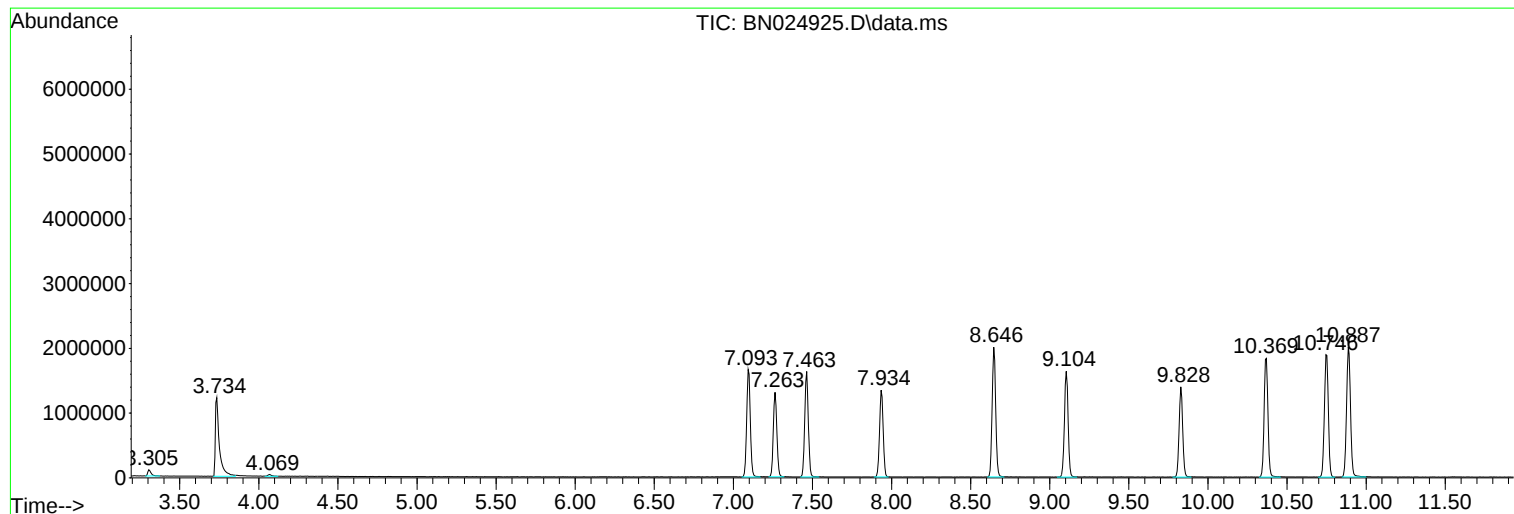

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024925.D
Acq On : 15 Apr 2023 09:11
Operator : CG/JU
Sample : PB152119BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK119

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024925.D
Acq On : 15 Apr 2023 09:11
Operator : CG/JU
Sample : PB152119BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK119

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------