

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024926.D
 Acq On : 15 Apr 2023 09:47
 Operator : CG/JU
 Sample : PB152052TB 10X
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024926.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	16	20	31	rVB	96647	142850	1.55%	0.157%
2	3.758	94	97	105	rBV	76784	152287	1.65%	0.167%
3	4.069	146	150	154	rBV2	20017	30202	0.33%	0.033%
4	4.528	226	228	232	rVB4	8424	10414	0.11%	0.011%
5	5.187	336	340	344	rBV3	6920	9936	0.11%	0.011%
6	7.093	657	664	678	rBV	1717261	2773557	30.08%	3.040%
7	7.263	686	693	702	rBV	1398065	2133334	23.13%	2.339%
8	7.463	720	727	736	rBV	1749214	2697626	29.25%	2.957%
9	7.934	800	807	819	rVB	1180617	1861529	20.19%	2.041%
10	8.646	921	928	938	rBV	2099559	3318640	35.99%	3.638%
11	9.104	998	1006	1015	rBV	1741926	2763409	29.96%	3.029%
12	9.828	1121	1129	1144	rBV	1443644	2316681	25.12%	2.540%
13	10.369	1212	1221	1234	rBV	1926405	3275796	35.52%	3.591%
14	10.746	1278	1285	1298	rVB	1660267	2765260	29.99%	3.031%
15	11.051	1328	1337	1340	rBV5	9055	14885	0.16%	0.016%
16	12.334	1550	1555	1565	rVB2	29832	55438	0.60%	0.061%
17	12.551	1587	1592	1598	rBV8	5853	12106	0.13%	0.013%
18	13.992	1830	1837	1852	rBV	3474788	4853421	52.63%	5.320%
19	14.275	1878	1885	1899	rBV	3512043	5038555	54.64%	5.523%
20	14.581	1928	1937	1945	rBV	2533294	3677444	39.88%	4.031%
21	14.775	1962	1970	1985	rBV	1925632	2829799	30.68%	3.102%
22	14.987	2004	2006	2016	rVB9	7860	12691	0.14%	0.014%
23	15.575	2098	2106	2117	rBV	4954086	7079551	76.77%	7.760%
24	15.692	2119	2126	2137	rBV	2045421	2724434	29.54%	2.986%
25	15.810	2142	2146	2156	rVB3	24770	43204	0.47%	0.047%
26	16.081	2189	2192	2197	rVB3	17579	22515	0.24%	0.025%
27	17.004	2346	2349	2354	rVB7	8586	13886	0.15%	0.015%
28	17.328	2398	2404	2411	rBV	3136486	4430586	48.04%	4.857%
29	17.428	2414	2421	2442	rVV	5496230	7728163	83.80%	8.471%
30	17.992	2514	2517	2521	rBV3	10314	12163	0.13%	0.013%
31	19.286	2732	2737	2742	rBV2	68883	105783	1.15%	0.116%
32	19.357	2744	2749	2754	rVV	65449	86300	0.94%	0.095%
33	19.722	2805	2811	2820	rBV	7131515	9056449	98.20%	9.928%
34	21.521	3111	3117	3129	rBV	3760944	5035580	54.60%	5.520%
35	23.815	3499	3507	3524	rBV	4678334	9222129	100.00%	10.109%
36	23.974	3526	3534	3543	rVB	2253153	4918975	53.34%	5.392%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024926.D
Acq On : 15 Apr 2023 09:47
Operator : CG/JU
Sample : PB152052TB 10X
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB052

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Title : SVOA CALIBRATION




Sum of corrected areas: 91225578

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024926.D
Acq On : 15 Apr 2023 09:47
Operator : CG/JU
Sample : PB152052TB 10X
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB052

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

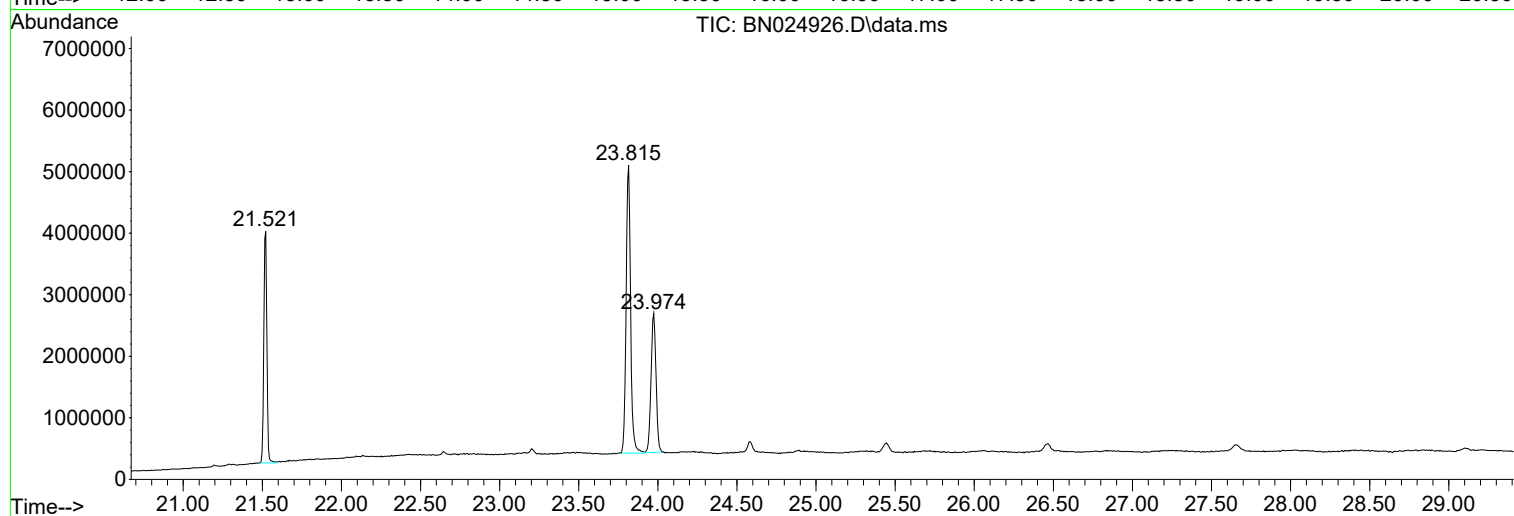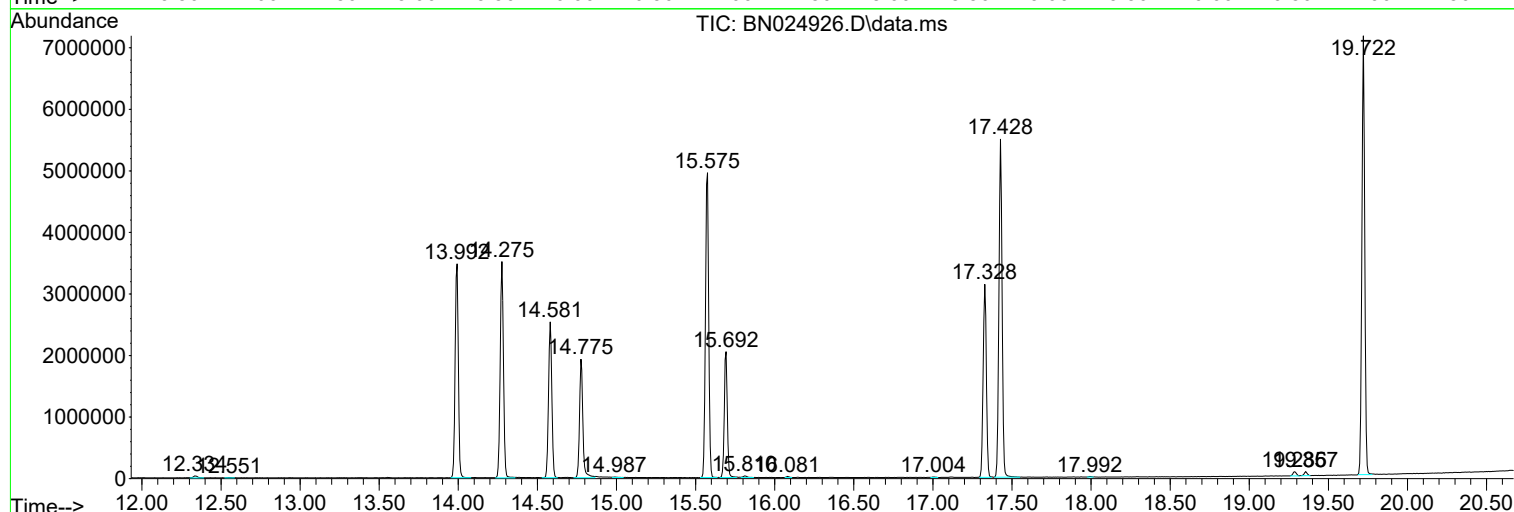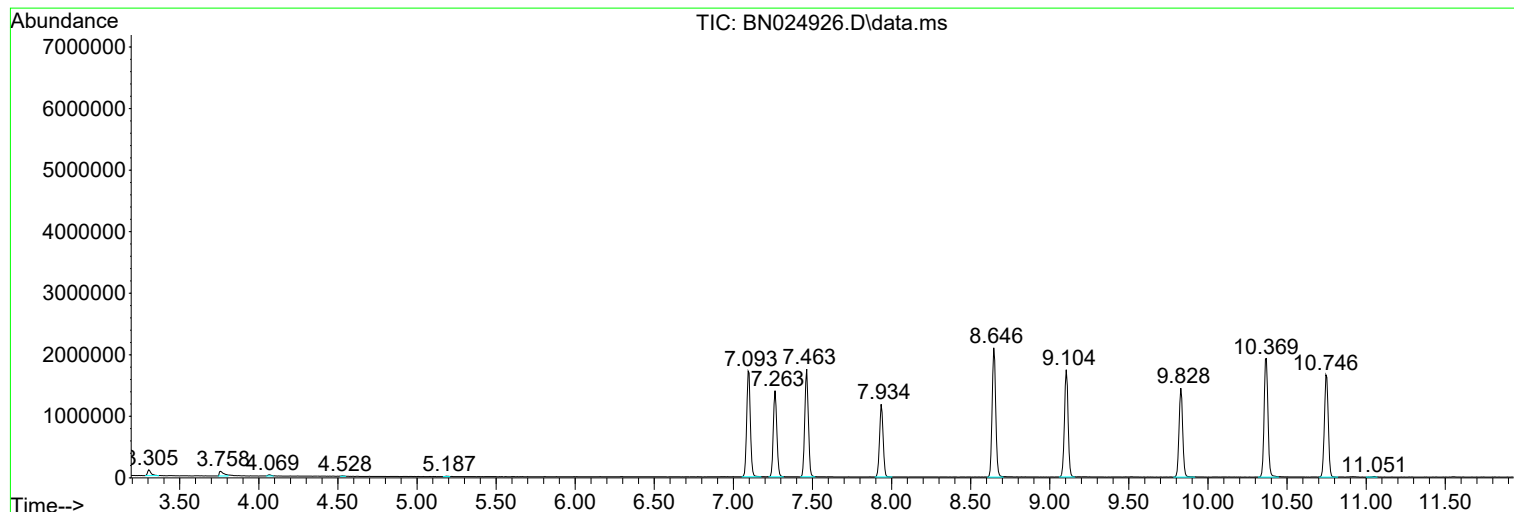

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024926.D
Acq On : 15 Apr 2023 09:47
Operator : CG/JU
Sample : PB152052TB 10X
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB052

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024926.D
Acq On : 15 Apr 2023 09:47
Operator : CG/JU
Sample : PB152052TB 10X
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB052

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------