

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024930.D
 Acq On : 15 Apr 2023 12:13
 Operator : CG/JU
 Sample : 02252-05DL 5X
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COME1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024930.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.234	338	348	367	rBV3	48863870	110790958	100.00%	45.026%
2	7.122	666	669	678	rVB	93390	146227	0.13%	0.059%
3	7.258	684	692	714	rBV	4018630	6525316	5.89%	2.652%
4	7.463	719	727	737	rVV	235537	427828	0.39%	0.174%
5	7.822	780	788	795	rBV	1283997	2032015	1.83%	0.826%
6	7.981	798	815	826	rBV	28305692	51278768	46.28%	20.840%
7	8.293	858	868	880	rBV	17441598	29826381	26.92%	12.122%
8	8.646	922	928	938	rBV	168339	278061	0.25%	0.113%
9	9.104	999	1006	1008	rBV	301048	472620	0.43%	0.192%
10	9.146	1008	1013	1023	rVB	1731895	2811905	2.54%	1.143%
11	9.775	1112	1120	1125	rBV	301346	516230	0.47%	0.210%
12	9.828	1125	1129	1139	rVB	224673	379756	0.34%	0.154%
13	10.369	1214	1221	1227	rBV	331366	543678	0.49%	0.221%
14	10.610	1255	1262	1278	rVB	1465288	2420824	2.19%	0.984%
15	10.746	1278	1285	1297	rVB	1864238	3152252	2.85%	1.281%
16	10.863	1297	1305	1320	rBV2	1065449	2367437	2.14%	0.962%
17	11.134	1344	1351	1358	rVB2	78322	131834	0.12%	0.054%
18	13.987	1829	1836	1846	rBV	677344	938417	0.85%	0.381%
19	14.275	1878	1885	1895	rBV2	665791	987808	0.89%	0.401%
20	14.581	1924	1937	1947	rBV	2867411	4149991	3.75%	1.687%
21	15.569	2099	2105	2112	rBV	944945	1398414	1.26%	0.568%
22	15.692	2119	2126	2134	rBV	237166	363894	0.33%	0.148%
23	15.939	2162	2168	2174	rBV	168910	230365	0.21%	0.094%
24	17.328	2396	2404	2414	rBV	3645254	4998486	4.51%	2.031%
25	17.428	2414	2421	2430	rVV	1084605	1554632	1.40%	0.632%
26	19.722	2805	2811	2825	rBV	1509917	2021889	1.82%	0.822%
27	21.222	3063	3066	3071	rBV4	76709	121863	0.11%	0.050%
28	21.516	3111	3116	3126	rBV	4485904	5692720	5.14%	2.314%
29	23.810	3500	3506	3520	rVB3	986264	2369858	2.14%	0.963%
30	23.968	3525	3533	3549	rVB	2781588	5965031	5.38%	2.424%
31	24.580	3633	3637	3647	rVB	293752	566789	0.51%	0.230%
32	25.439	3779	3783	3793	rVB	257849	599423	0.54%	0.244%




Sum of corrected areas: 246061670

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024930.D
Acq On : 15 Apr 2023 12:13
Operator : CG/JU
Sample : 02252-05DL 5X
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COME1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

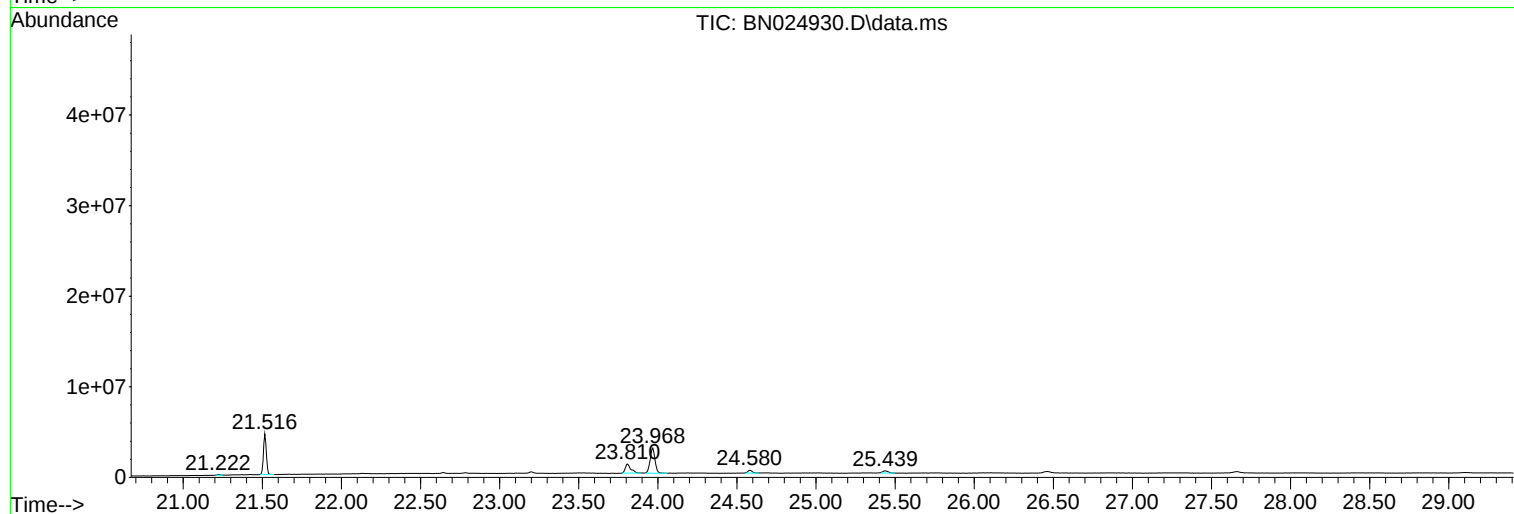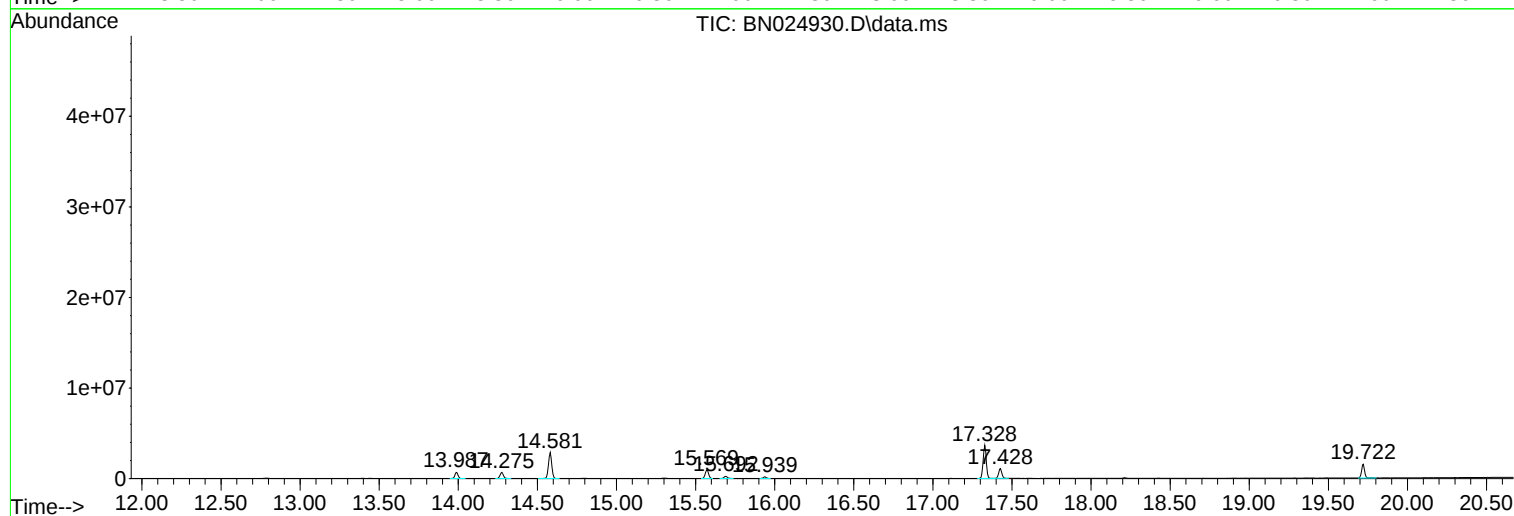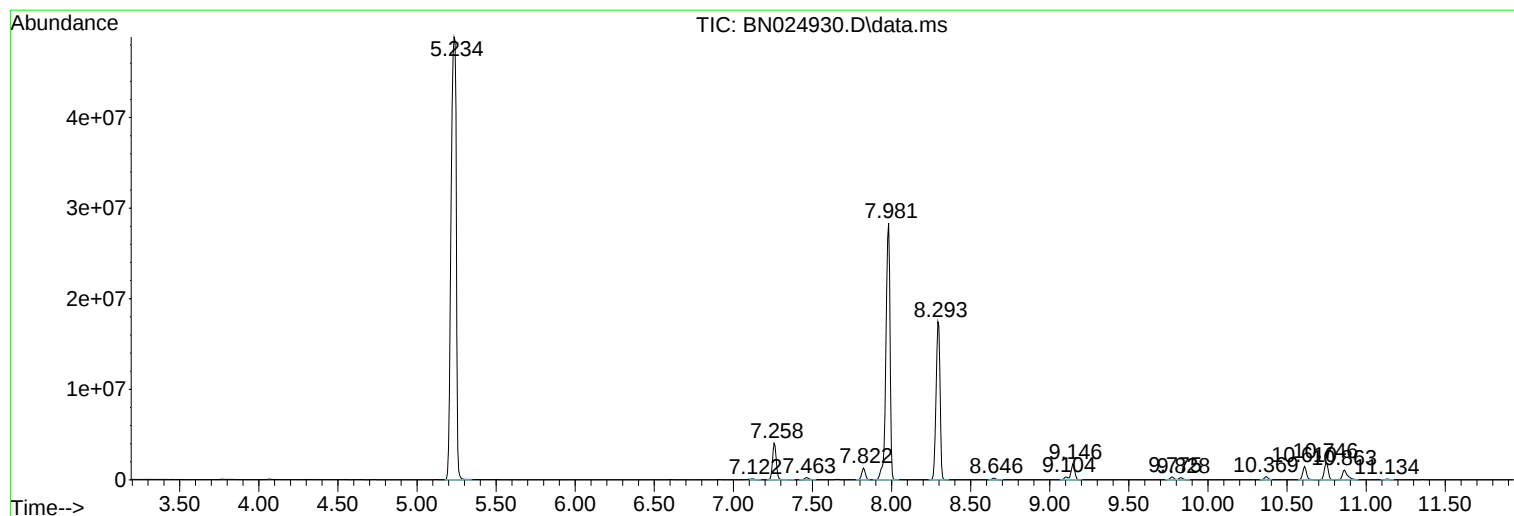

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024930.D
Acq On : 15 Apr 2023 12:13
Operator : CG/JU
Sample : 02252-05DL 5X
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COME1DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 o-Chloroaniline Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.775	3.28 ng/ul	516230	Naphthalene-d8	10.746

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			o-Chloroaniline	127	C6H6ClN	000095-51-2	97
2			m-Chloroaniline	127	C6H6ClN	000108-42-9	97
3			o-Chloroaniline	127	C6H6ClN	000095-51-2	96
4			m-Chloroaniline	127	C6H6ClN	000108-42-9	95
5			o-Chloroaniline	127	C6H6ClN	000095-51-2	94

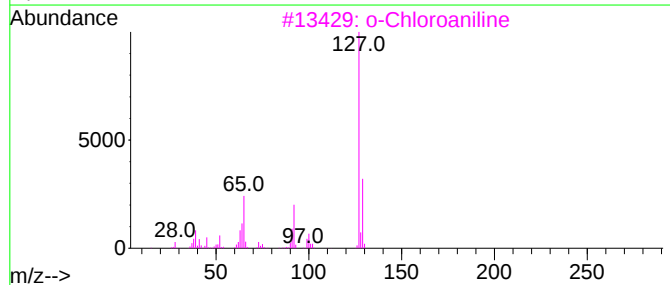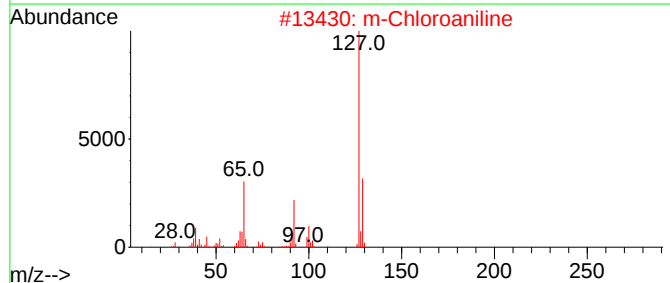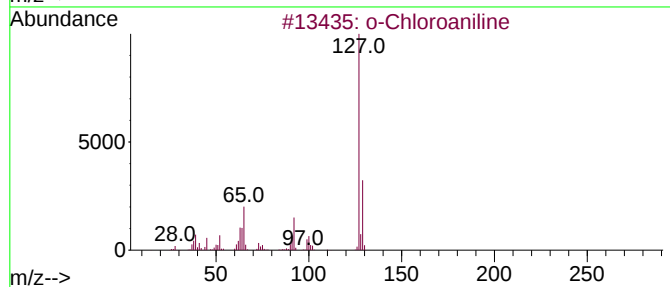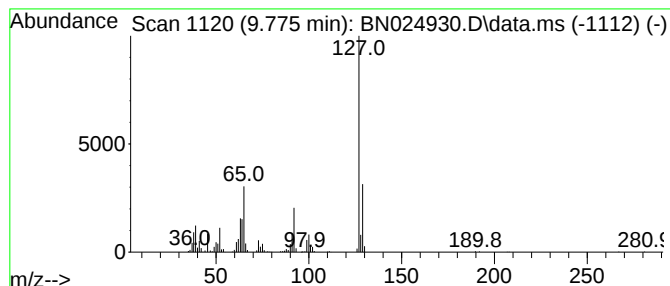

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024930.D
Acq On : 15 Apr 2023 12:13
Operator : CG/JU
Sample : 02252-05DL 5X
Misc :
ALS Vial : 78 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
COME1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 (DEL) Alkane: Straight-Chai... Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.	
25.439	2.01 ng/ul	599423	Perylene-d12	23.968	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hexacosane	366	C26H54	000630-01-3	90
2	4-Methylheneicosane	310	C22H46	025117-29-7	87
3	Behenyl chloride	344	C22H45Cl	042217-03-8	86
4	Nonadecane	268	C19H40	000629-92-5	83
5	Heptacosane	380	C27H56	000593-49-7	83

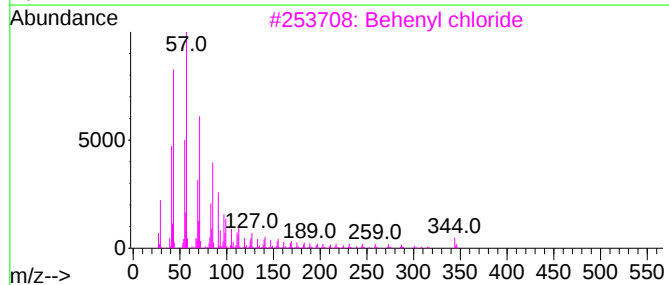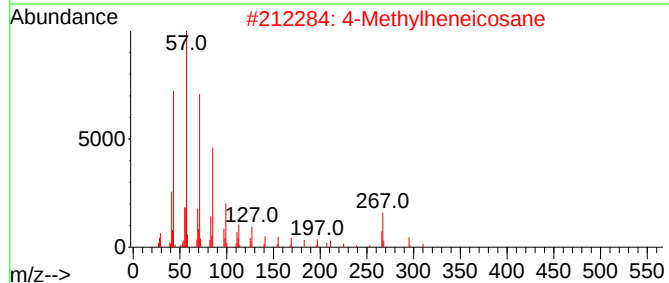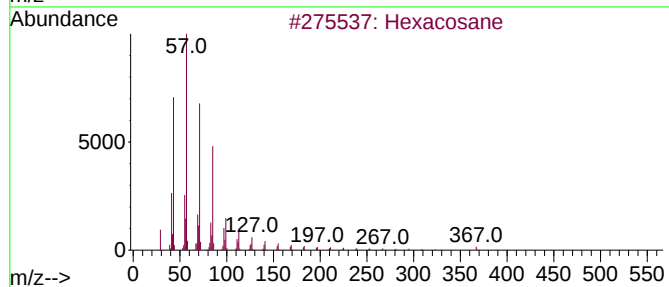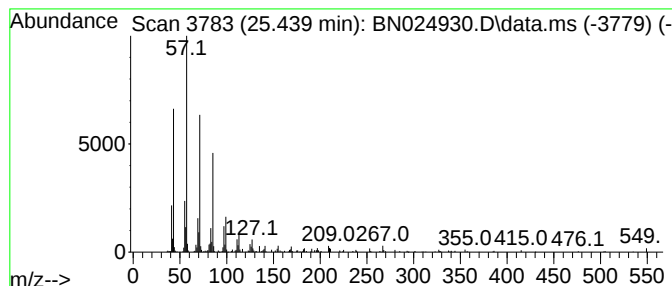

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024930.D
Acq On : 15 Apr 2023 12:13
Operator : CG/JU
Sample : 02252-05DL 5X
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0ME1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
o-Chloroaniline	9.775	3.3	ng/u1	516230	2	10.746	3152250	20.0
(DEL) Alkane: S...	25.439	2.0	ng/u1	599423	6	23.968	5965030	20.0