

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024934.D
 Acq On : 15 Apr 2023 14:39
 Operator : CG/JU
 Sample : 02254-18
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024934.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	9	14	18	rBV	330771	510003	4.56%	0.519%
2	3.340	22	26	43	rVB	921393	1441025	12.88%	1.465%
3	3.587	64	68	78	rVB	39579	56414	0.50%	0.057%
4	3.746	93	95	109	rBV	200105	393222	3.51%	0.400%
5	3.969	129	133	143	rVB4	11004	21364	0.19%	0.022%
6	4.069	145	150	156	rBV	26043	42547	0.38%	0.043%
7	4.605	237	241	249	rBV4	18963	32122	0.29%	0.033%
8	5.011	306	310	316	rBV5	7306	11547	0.10%	0.012%
9	7.093	654	664	674	rBV	377236	603408	5.39%	0.614%
10	7.263	686	693	703	rBV	1369873	2111012	18.87%	2.146%
11	7.463	718	727	737	rBV	1323030	2118559	18.94%	2.154%
12	7.552	737	742	749	rVB7	8529	15175	0.14%	0.015%
13	7.934	799	807	815	rBV	1271323	1992070	17.81%	2.025%
14	8.052	821	827	834	rVB	152055	238946	2.14%	0.243%
15	8.646	921	928	938	rBV	1064570	1655569	14.80%	1.683%
16	9.104	999	1006	1021	rBV	1722626	2784962	24.89%	2.832%
17	9.216	1021	1025	1030	rVV4	11916	23301	0.21%	0.024%
18	9.269	1030	1034	1038	rVB7	8095	13286	0.12%	0.014%
19	9.510	1069	1075	1080	rVB	34505	52179	0.47%	0.053%
20	9.828	1121	1129	1143	rBV	1376447	2247861	20.09%	2.286%
21	10.363	1212	1220	1238	rBV	1785358	3017779	26.98%	3.068%
22	10.746	1276	1285	1294	rBV	1742637	2952645	26.39%	3.002%
23	10.887	1300	1309	1321	rBV	1505248	2533348	22.65%	2.576%
24	11.540	1414	1420	1428	rBV5	14466	29534	0.26%	0.030%
25	12.004	1492	1499	1505	rVB	31243	50095	0.45%	0.051%
26	12.334	1550	1555	1565	rVB	31784	55994	0.50%	0.057%
27	13.992	1830	1837	1845	rBV	3525332	4879510	43.62%	4.961%
28	14.110	1850	1857	1861	rVB8	10118	16722	0.15%	0.017%
29	14.275	1877	1885	1895	rBV2	3994326	5792772	51.78%	5.890%
30	14.581	1929	1937	1948	rBV	2742646	3908598	34.94%	3.974%
31	14.675	1951	1953	1963	rVB9	6319	12961	0.12%	0.013%
32	14.775	1964	1970	1983	rBV	260443	483347	4.32%	0.491%
33	14.986	2002	2006	2012	rVB7	14691	26020	0.23%	0.026%
34	15.322	2058	2063	2066	rBV2	11060	14963	0.13%	0.015%
35	15.575	2098	2106	2119	rBV	5020746	7368768	65.87%	7.492%
36	15.692	2119	2126	2137	rBV	2129736	2820460	25.21%	2.868%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
 Data File : BN024934.D
 Acq On : 15 Apr 2023 14:39
 Operator : CG/JU
 Sample : 02254-18
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

37	15.810	2142	2146	2154	rVB3	27944	47086	0.42%	0.048%
38	15.939	2162	2168	2173	rBV	83373	117120	1.05%	0.119%
39	16.357	2235	2239	2246	rBV8	7146	14269	0.13%	0.015%
40	17.116	2365	2368	2374	rVB4	8142	12934	0.12%	0.013%
41	17.328	2397	2404	2411	rBV	3471807	4799914	42.91%	4.880%
42	17.428	2414	2421	2433	rBV	6088013	8430463	75.36%	8.572%
43	17.610	2448	2452	2456	rVB4	13055	15518	0.14%	0.016%
44	17.716	2466	2470	2474	rVB6	8094	12251	0.11%	0.012%
45	17.992	2514	2517	2522	rVB4	10307	12777	0.11%	0.013%
46	18.216	2549	2555	2562	rBV	198696	288946	2.58%	0.294%
47	18.292	2564	2568	2574	rVB	35720	57560	0.51%	0.059%
48	18.504	2602	2604	2608	rVB4	8876	12123	0.11%	0.012%
49	18.645	2624	2628	2631	rBV6	10106	12660	0.11%	0.013%
50	19.286	2732	2737	2742	rBV2	78854	115018	1.03%	0.117%
51	19.357	2744	2749	2755	rBV	74432	131123	1.17%	0.133%
52	19.486	2768	2771	2775	rBV	118661	150119	1.34%	0.153%
53	19.639	2795	2797	2800	rVB3	25593	24315	0.22%	0.025%
54	19.722	2805	2811	2821	rVV	7768738	10096258	90.25%	10.266%
55	20.745	2983	2985	2988	rBV2	31863	31790	0.28%	0.032%
56	21.216	3062	3065	3074	rBV2	156910	295379	2.64%	0.300%
57	21.516	3111	3116	3124	rVB	4130525	5472207	48.92%	5.564%
58	22.639	3304	3307	3313	rVB3	125066	167001	1.49%	0.170%
59	23.204	3400	3403	3407	rVB2	171148	237728	2.13%	0.242%
60	23.810	3498	3506	3516	rBV	5608640	11187157	100.00%	11.375%
61	23.962	3525	3532	3542	rVB	2800623	5791432	51.77%	5.889%
62	24.574	3631	3636	3643	rVB2	227475	489679	4.38%	0.498%




Sum of corrected areas: 98350915

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024934.D
Acq On : 15 Apr 2023 14:39
Operator : CG/JU
Sample : 02254-18
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

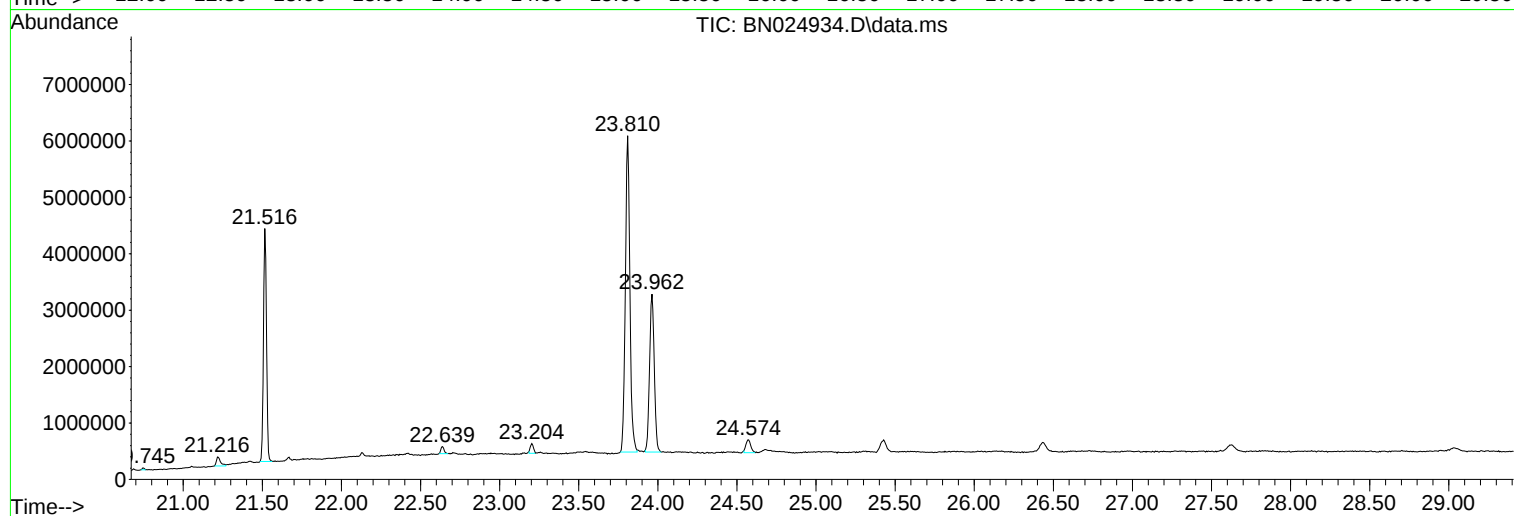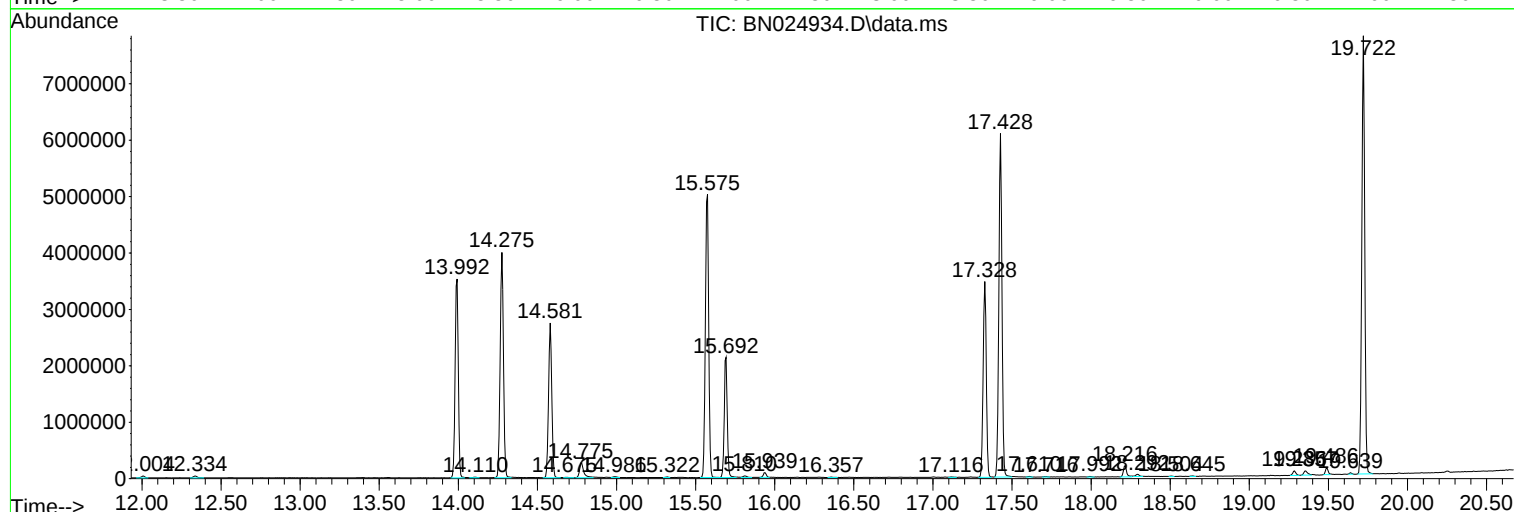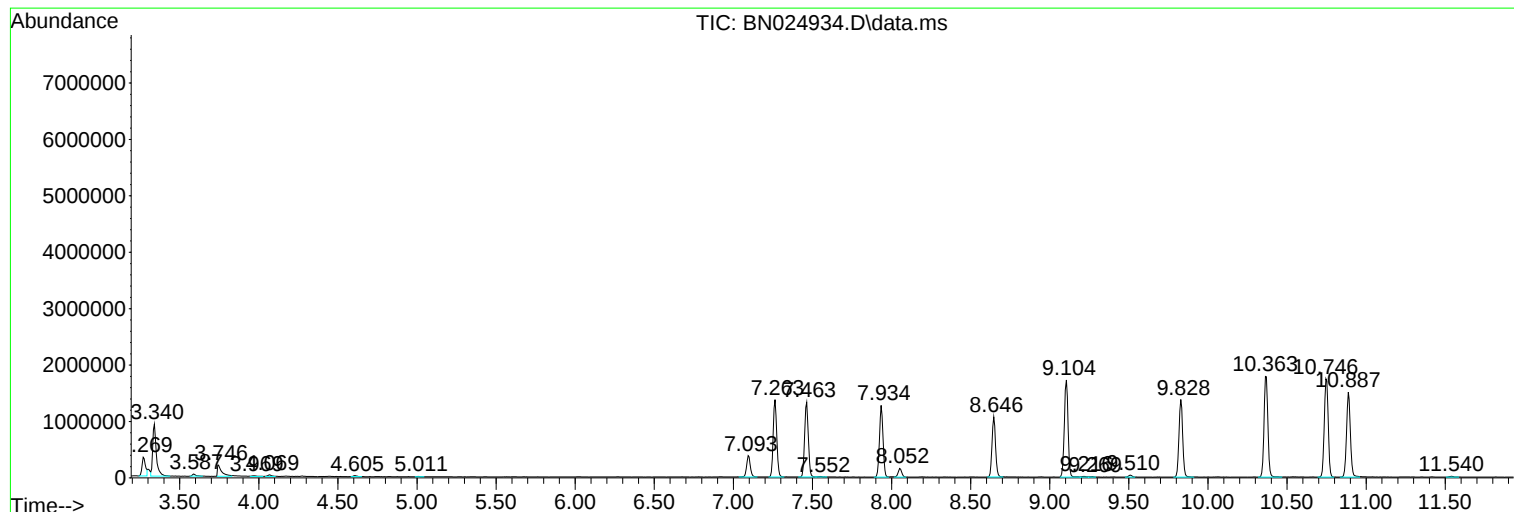

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041423\
Data File : BN024934.D
Acq On : 15 Apr 2023 14:39
Operator : CG/JU
Sample : 02254-18
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	8.052	2.4	ng/u1	238946	1	7.934	1992070	20.0