


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041520\
 Data File : BN010502.D
 Acq On : 15 Apr 2020 09:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 13 18:04:22 2020

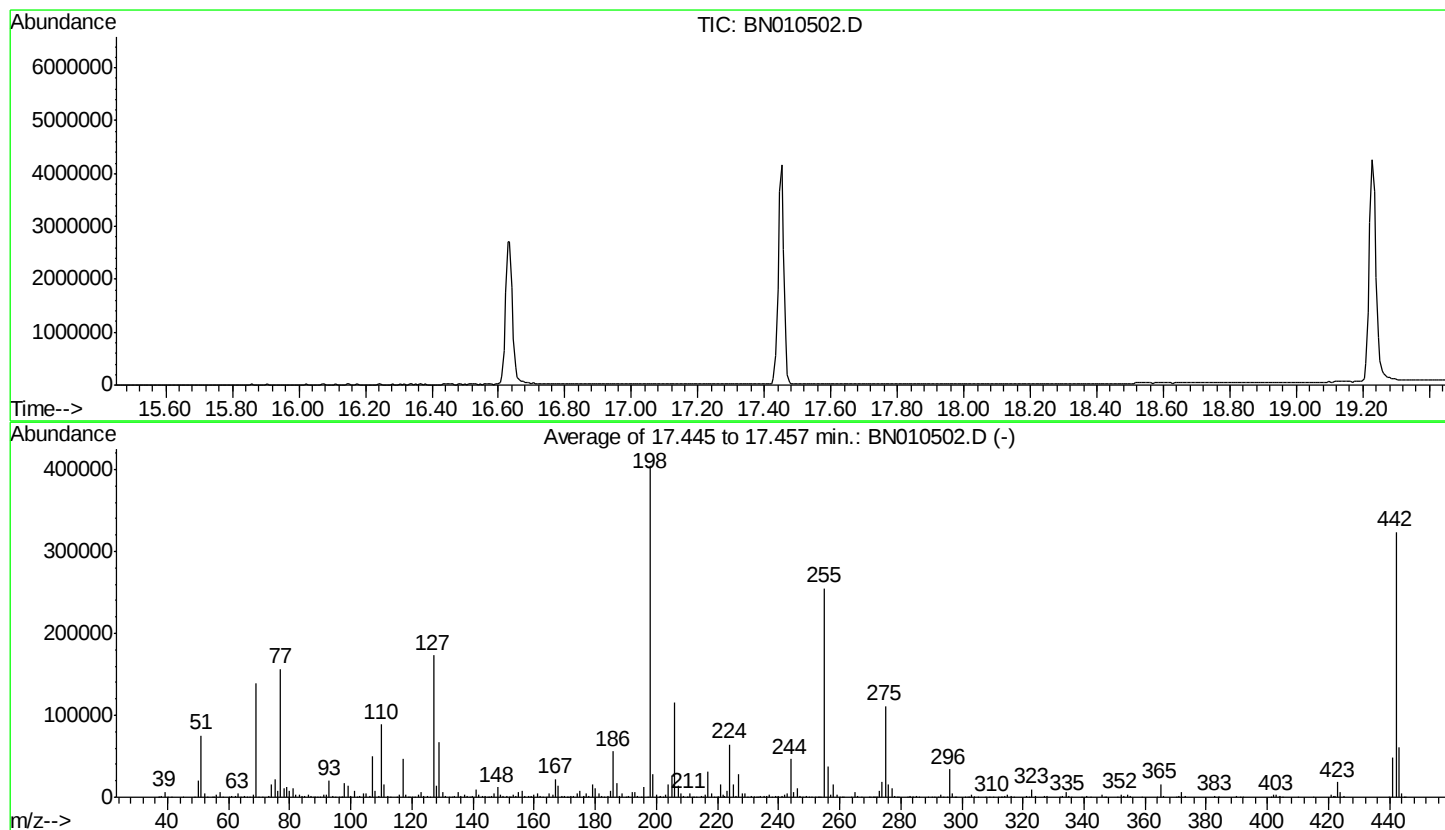

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.7	75760	PASS
68	69	0.00	2	1.8	2451	PASS
69	198	0.00	100	34.2	138304	PASS
70	69	0.00	2	0.5	630	PASS
127	198	10	80	42.7	172704	PASS
197	198	0.00	2	0.2	775	PASS
198	198	100	100	100.0	404650	PASS
199	198	5	9	6.9	27917	PASS
275	198	10	60	27.5	111200	PASS
365	198	1	100	4.0	16011	PASS
441	198	0.01	100	12.1	48994	PASS
442	198	50	100	80.0	323669	PASS
443	442	15	24	18.8	60722	PASS