

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041525\
 Data File : BN036918.D
 Acq On : 15 Apr 2025 16:12
 Operator : RC/JU
 Sample : PB166495BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK495

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041525.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN036918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	34	38	44	rBV	38185	49473	1.96%	0.167%
2	3.522	104	108	131	rBV	544158	848144	33.66%	2.863%
3	3.840	158	162	166	rBV2	9207	12717	0.50%	0.043%
4	6.805	660	666	674	rBV	735326	1089894	43.25%	3.678%
5	6.969	687	694	703	rVB	471879	709155	28.14%	2.393%
6	7.163	720	727	736	rBV	672912	1010124	40.08%	3.409%
7	7.628	799	806	814	rBV	394311	603557	23.95%	2.037%
8	8.340	920	927	942	rBV	815236	1235738	49.04%	4.171%
9	8.781	994	1002	1010	rBV	631316	989226	39.25%	3.339%
10	8.910	1020	1024	1029	rVB6	8076	12623	0.50%	0.043%
11	9.499	1117	1124	1136	rVB	540957	845673	33.56%	2.854%
12	10.034	1209	1215	1229	rBV	749712	1214551	48.20%	4.099%
13	10.410	1272	1279	1288	rVB	508491	823095	32.66%	2.778%
14	10.551	1296	1303	1318	rBV	743638	1197241	47.51%	4.041%
15	12.010	1545	1551	1557	rVB	8784	14235	0.56%	0.048%
16	13.698	1831	1838	1847	rBV	1251852	1683887	66.82%	5.683%
17	13.969	1877	1884	1892	rBV	1273991	1882964	74.72%	6.355%
18	14.281	1929	1937	1944	rBV	773585	1086642	43.12%	3.667%
19	14.487	1965	1972	1989	rBV	675114	992945	39.40%	3.351%
20	15.116	2074	2079	2082	rVB4	2990	4220	0.17%	0.014%
21	15.275	2100	2106	2117	rBV	1601379	2256623	89.55%	7.616%
22	15.398	2121	2127	2138	rBV	706809	896898	35.59%	3.027%
23	15.522	2143	2148	2153	rVB6	5441	9038	0.36%	0.031%
24	16.816	2365	2368	2372	rVB3	2643	3057	0.12%	0.010%
25	17.028	2396	2404	2410	rBV	895863	1225029	48.61%	4.135%
26	17.128	2414	2421	2434	rBV	1799607	2405048	95.44%	8.117%
27	17.616	2500	2504	2509	rVB6	2175	4304	0.17%	0.015%
28	17.710	2517	2520	2525	rVB5	2808	4373	0.17%	0.015%
29	17.763	2525	2529	2531	rBV4	2085	3399	0.13%	0.011%
30	17.933	2554	2558	2562	rVV6	6697	9678	0.38%	0.033%
31	18.680	2676	2685	2689	rBV9	4305	12480	0.50%	0.042%
32	18.933	2723	2728	2731	rBV7	3592	6953	0.28%	0.023%
33	18.992	2733	2738	2741	rVV2	17076	23082	0.92%	0.078%
34	19.063	2746	2750	2756	rVB	16423	22926	0.91%	0.077%
35	19.227	2775	2778	2779	rBV3	4581	3266	0.13%	0.011%
36	19.280	2784	2787	2788	rBV3	7405	6120	0.24%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041525\
Data File : BN036918.D
Acq On : 15 Apr 2025 16:12
Operator : RC/JU
Sample : PB166495BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041525.MA.M
Title : SVOA CALIBRATION

37	19.427	2806	2812	2818	rBV	1993643	2520021	100.00%	8.505%
38	21.257	3118	3123	3135	rBV	779839	1113399	44.18%	3.758%
39	23.957	3574	3582	3593	rBV	796098	1789164	71.00%	6.038%
40	24.157	3608	3616	3630	rVB2	400070	1008462	40.02%	3.404%




Sum of corrected areas: 29629424

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041525\
Data File : BN036918.D
Acq On : 15 Apr 2025 16:12
Operator : RC/JU
Sample : PB166495BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041525.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

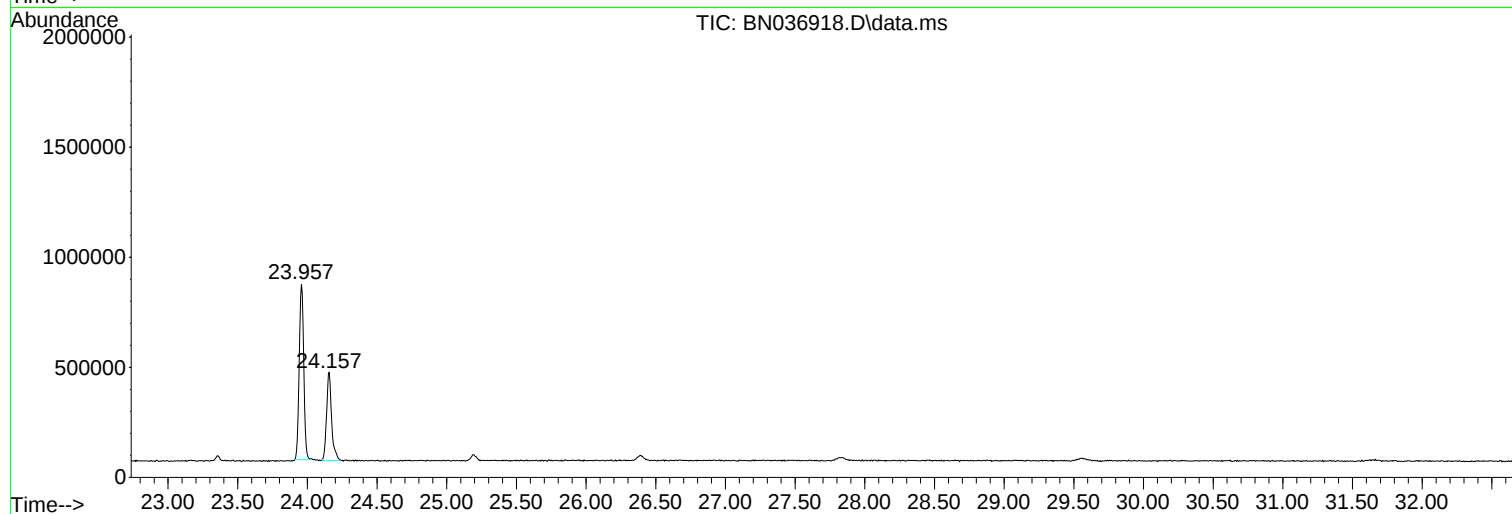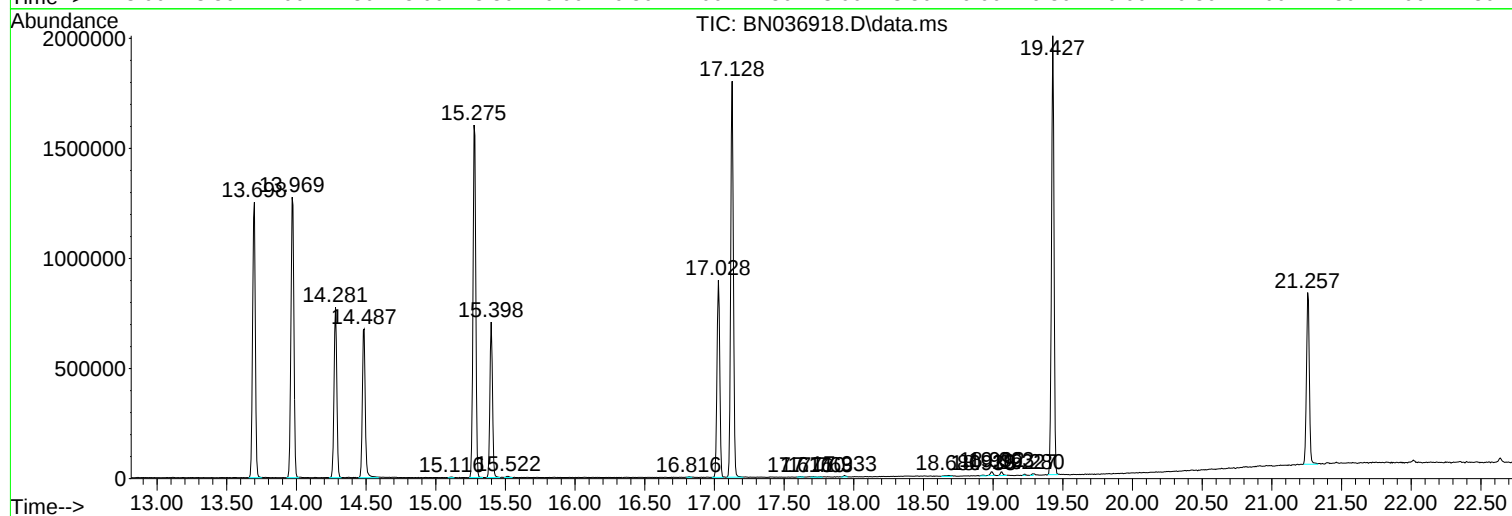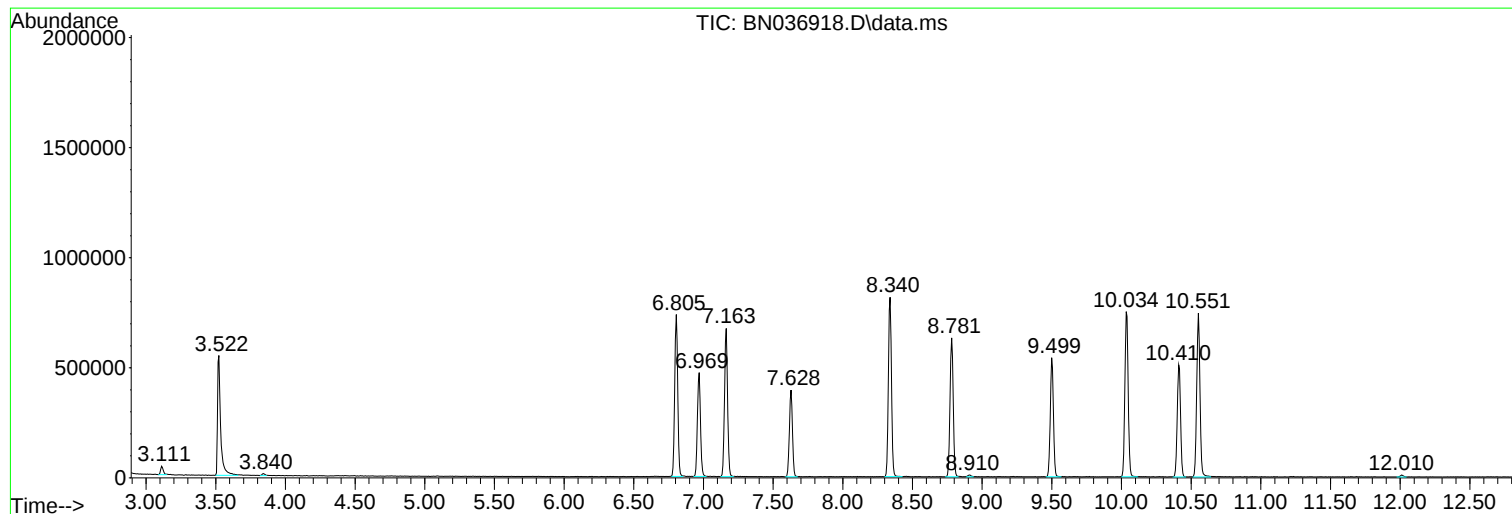

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041525\
Data File : BN036918.D
Acq On : 15 Apr 2025 16:12
Operator : RC/JU
Sample : PB166495BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041525.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041525\
Data File : BN036918.D
Acq On : 15 Apr 2025 16:12
Operator : RC/JU
Sample : PB166495BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041525.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc