

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041620\
 Data File : BN010522.D
 Acq On : 16 Apr 2020 18:34
 Operator : CG/JU
 Sample : L2191-17
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB7B7

Quant Time: Apr 17 01:06:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 16 10:21:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	467959	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	2078346	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	1381150	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	3068628	20.00	ng/ul	0.00
78) Chrysene-d12	21.17	240	2875466	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2511818	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	38181	4.27	ng/uL	0.00
5) Phenol-d5	6.79	99	1225552	33.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	650443	34.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	1030589	32.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	1051503	33.75	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	530744	33.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	594965	33.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	1118896	31.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1524220	37.99	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	3431574	33.49	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	4306851	34.20	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	552170	27.67	ng/ul	0.00
58) Fluorene-d10	15.22	176	2992983	32.55	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	438368	27.35	ng/ul	0.00
71) Anthracene-d10	17.07	188	4791672	33.71	ng/ul	0.00
79) Pyrene-d10	19.37	212	5445057	33.55	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	4280350	32.85	ng/ul	0.00

Target Compounds


				Ovalue		
15) N-Nitroso-di-n-propylamine	8.30	70	26168	1.160	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
Data File : BN010522.D
Acq On : 16 Apr 2020 18:34
Operator : CG/JU
Sample : L2191-17
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB7B7

Quant Time: Apr 17 01:06:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 10:21:51 2020
Response via : Initial Calibration

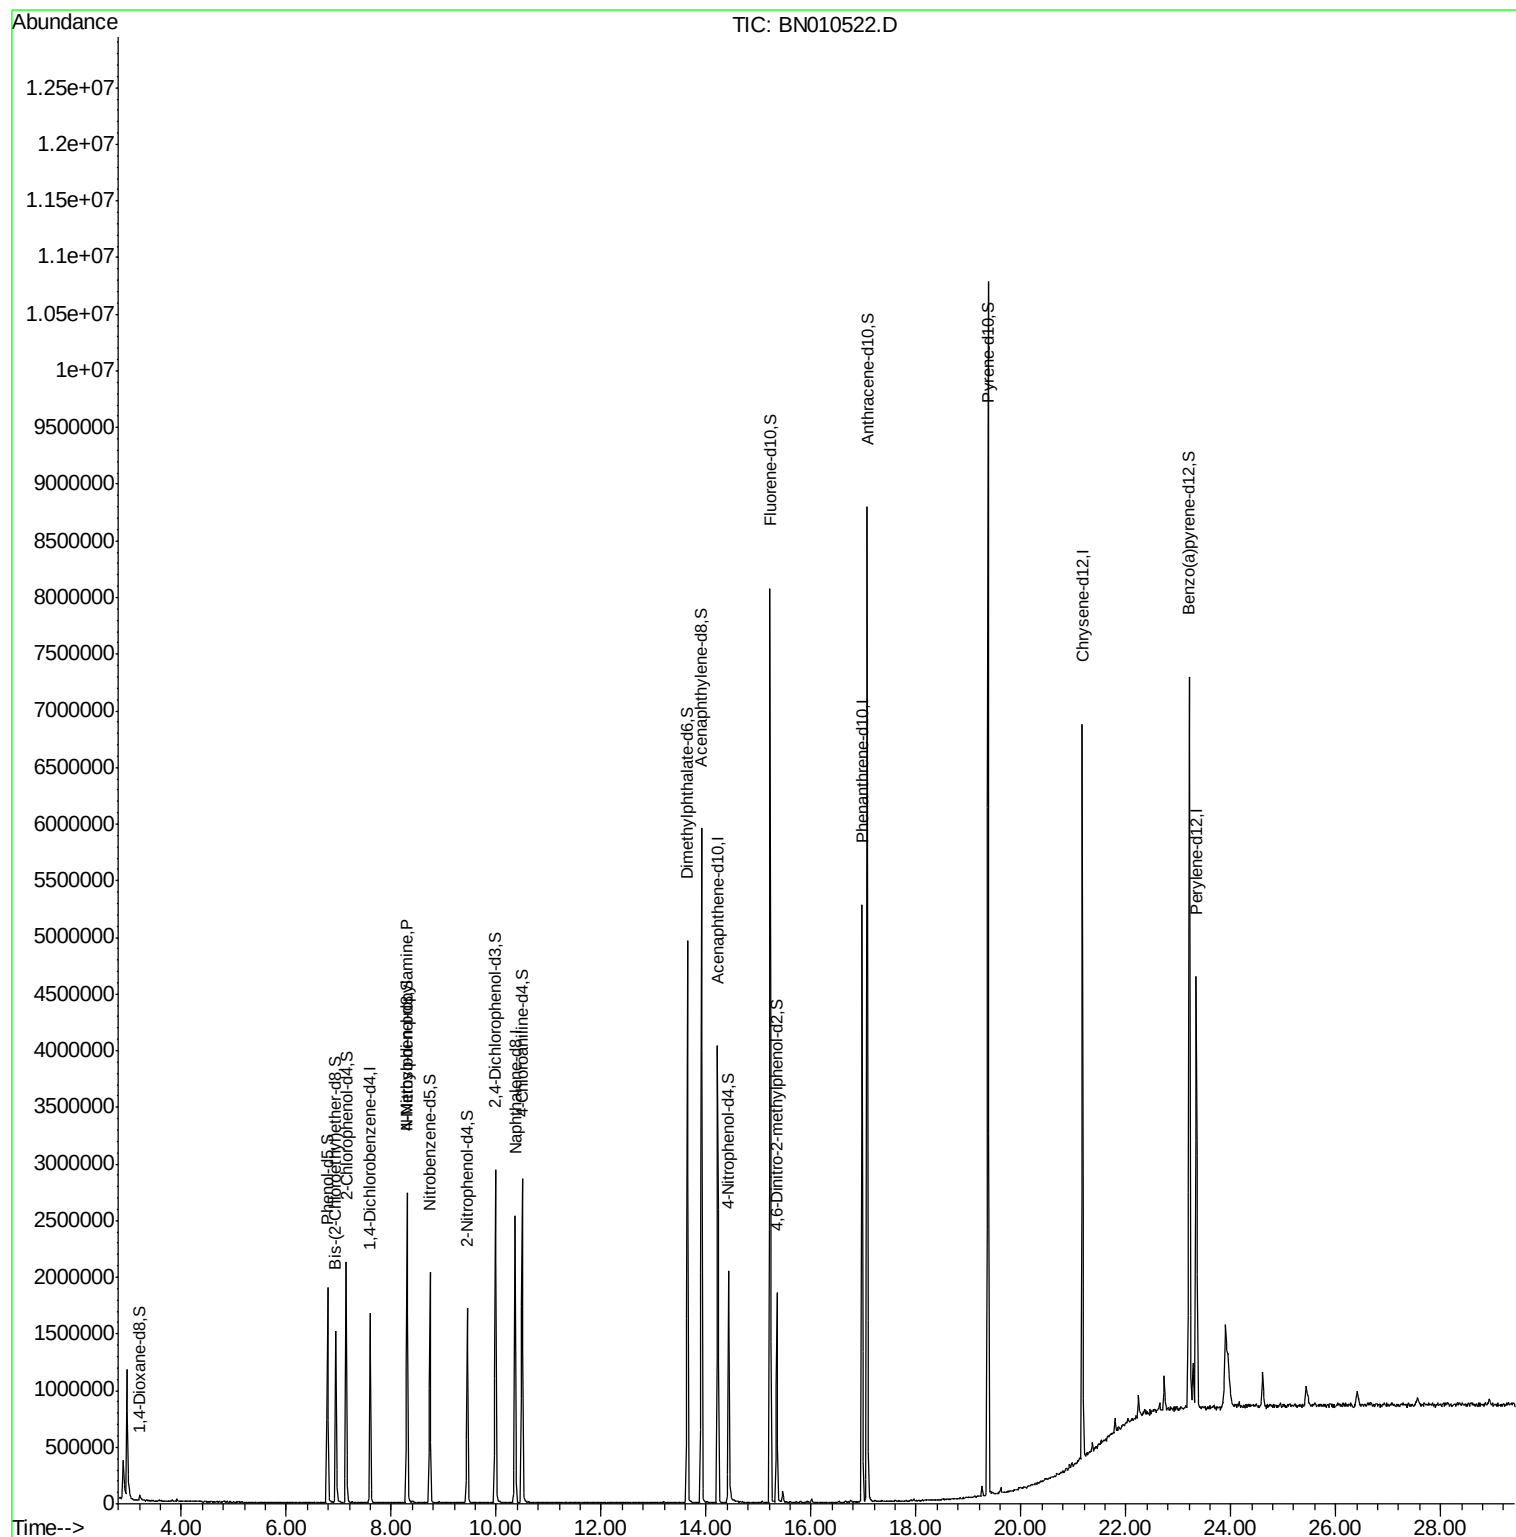

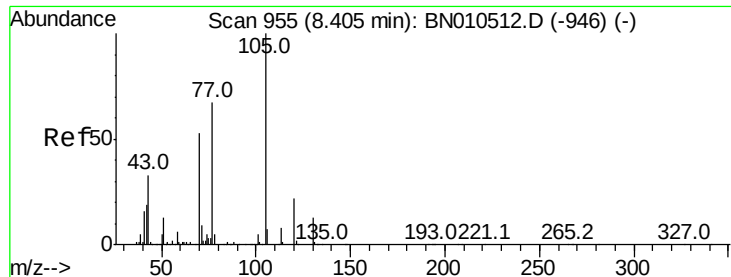

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.160 ng/ul
 RT: 8.30 min Scan# 938
 Delta R.T. -0.10 min
 Lab File: BN010522.D
 Acq: 16 Apr 2020 18:34

Instrument :
 BNA_N
 ClientSampleId :
 CB7B7

Tot Ion: 70 Resp: 26168
 Ion Ratio Lower Upper
 70 100
 42 217.4 26.6 39.8#
 101 0.0 8.4 12.6#
 130 0.0 19.7 29.5#

