

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041620\
 Data File : BN010523.D
 Acq On : 16 Apr 2020 19:10
 Operator : CG/JU
 Sample : L2191-19
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB7B9

Quant Time: Apr 17 01:07:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 16 10:21:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	426458	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1898366	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	1252077	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	2831452	20.00	ng/ul	0.00
78) Chrysene-d12	21.17	240	2903067	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2560785	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	31704	3.89	ng/uL	0.00
5) Phenol-d5	6.78	99	1057527	31.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	567247	33.31	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	896596	31.23	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	899788	31.69	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	452457	30.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	502016	30.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	969802	30.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1318909	35.99	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	2956047	31.82	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	3722923	32.62	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	494510	27.34	ng/ul	0.00
58) Fluorene-d10	15.22	176	2631859	31.57	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	367154	24.82	ng/ul	0.00
71) Anthracene-d10	17.07	188	4236585	32.30	ng/ul	0.00
79) Pyrene-d10	19.37	212	4883175	29.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	4036275	30.39	ng/ul	0.00


Target Compounds				Ovalue	
15) N-Nitroso-di-n-propylamine	8.30	70	23051	1.121	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
Data File : BN010523.D
Acq On : 16 Apr 2020 19:10
Operator : CG/JU
Sample : L2191-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB7B9

Quant Time: Apr 17 01:07:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 10:21:51 2020
Response via : Initial Calibration

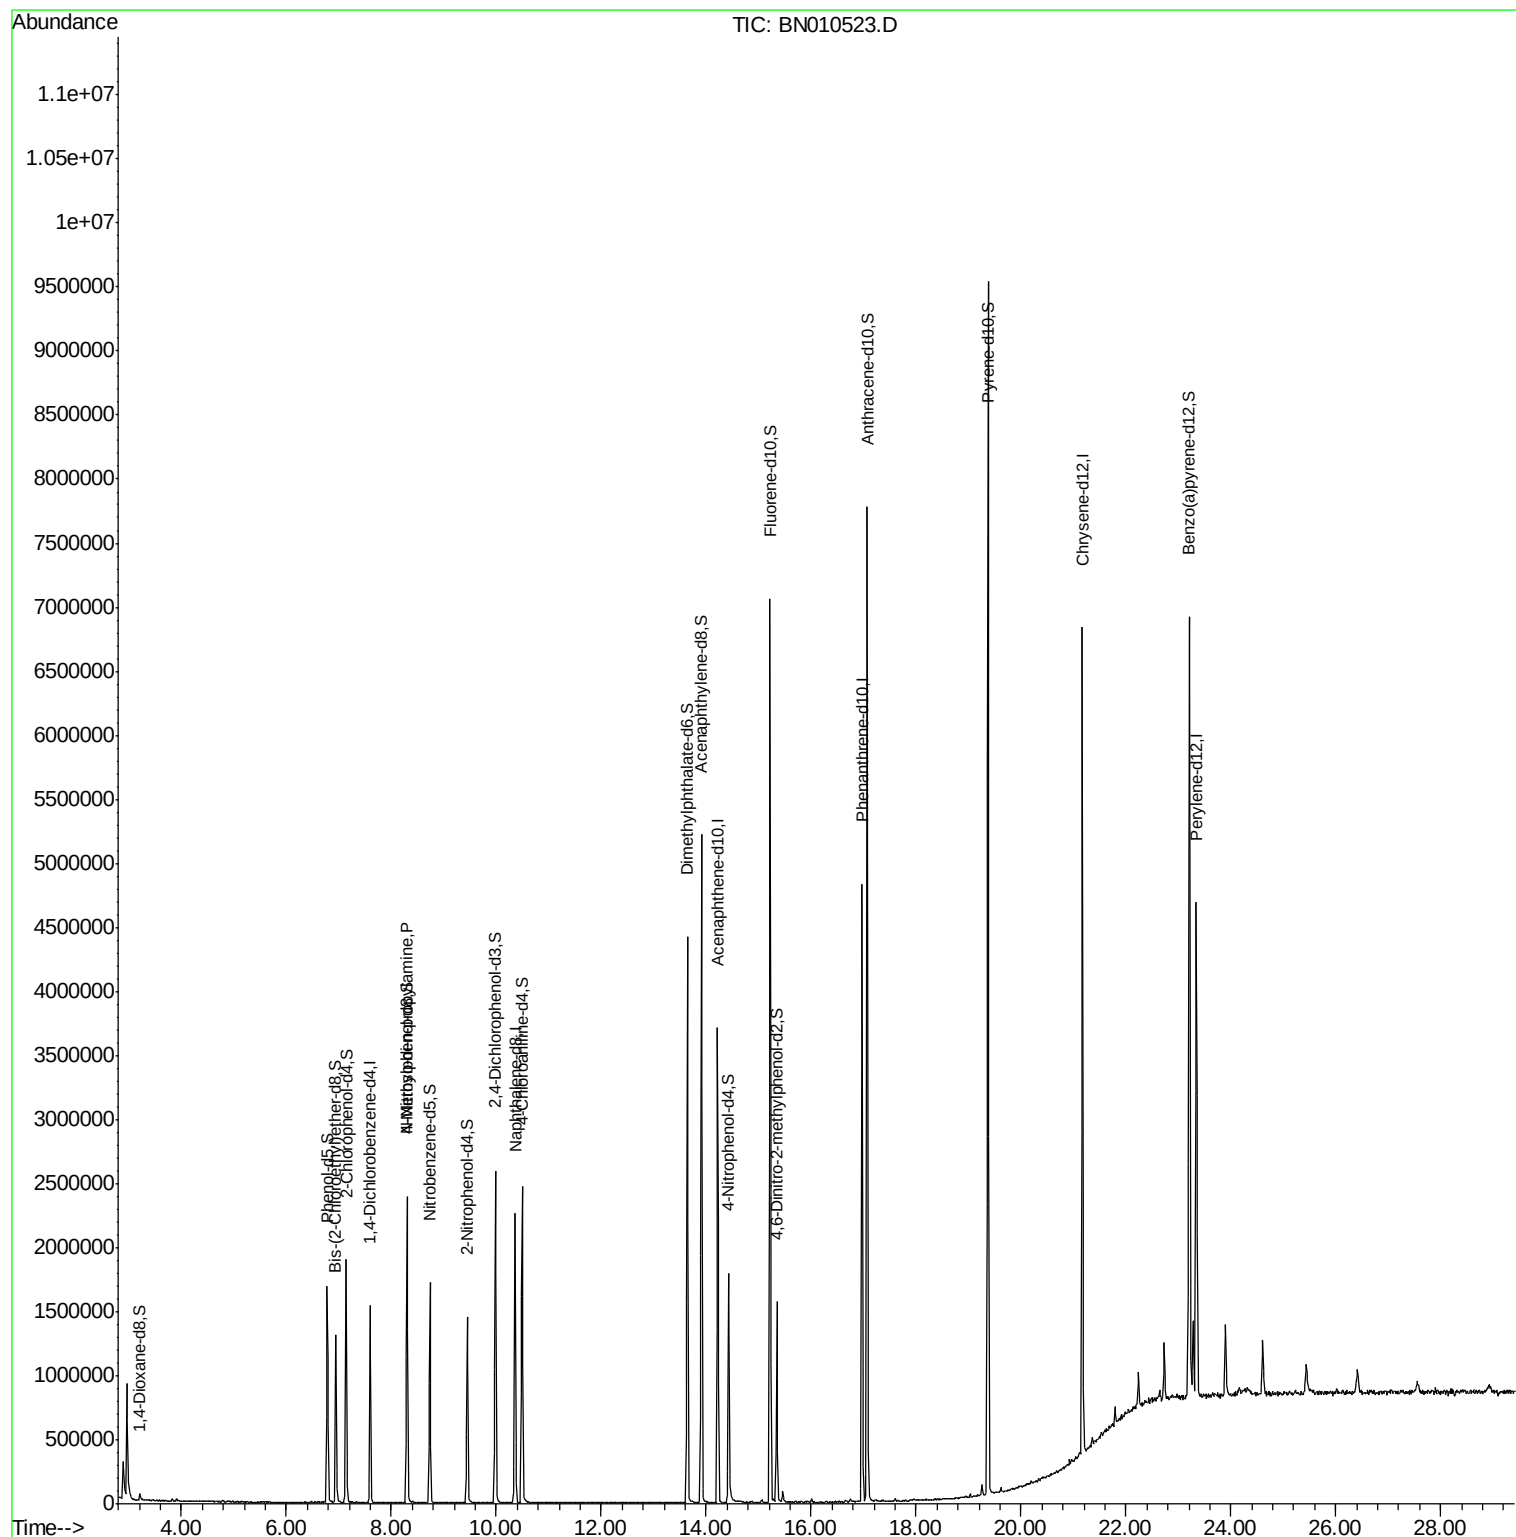

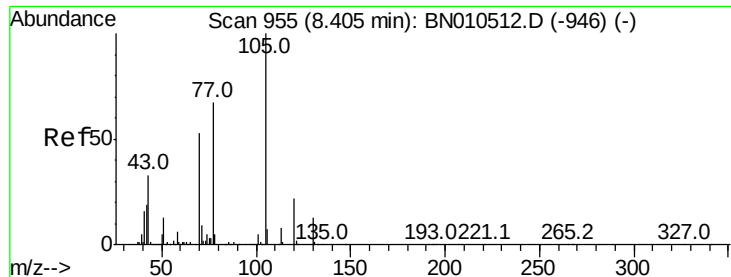

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.121 ng/ul
 RT: 8.30 min Scan# 938
 Delta R.T. -0.10 min
 Lab File: BN010523.D
 Acq: 16 Apr 2020 19:10

Instrument :
 BNA_N
 ClientSampleId :
 CB7B9

Tot Ion: 70 Resp: 23051
 Ion Ratio Lower Upper
 70 100
 42 211.7 26.6 39.8#
 101 0.0 8.4 12.6#
 130 0.0 19.7 29.5#

