

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041620\
 Data File : BN010527.D
 Acq On : 16 Apr 2020 21:34
 Operator : CG/JU
 Sample : L2191-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB7A0

Quant Time: Apr 17 01:07:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 16 10:21:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	454141	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	2031461	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	1322593	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	2974059	20.00	ng/ul	0.00
78) Chrysene-d12	21.17	240	2971209	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2647622	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	64896	7.48	ng/uL	0.00
5) Phenol-d5	6.79	99	1442767	40.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	767775	42.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	1241614	40.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	1259476	41.66	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	644167	41.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	708915	40.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	1329773	38.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1360045	34.68	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	4126540	42.05	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	5052439	41.90	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	714620	37.40	ng/ul	0.00
58) Fluorene-d10	15.22	176	3703637	42.06	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	579632	37.31	ng/ul	0.00
71) Anthracene-d10	17.07	188	5786645	42.01	ng/ul	0.00
79) Pyrene-d10	19.37	212	6689064	39.88	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	6054917	44.09	ng/ul	0.00

Target Compounds


					Ovalue	
45) Dimethylphthalate	13.69	163	511810	5.024	ng/ul	99
70) Phenanthrene	17.01	178	916498	5.549	ng/ul	98
72) Anthracene	17.10	178	176813	1.056	ng/ul	98
77) Fluoranthene	19.03	202	1590736	8.865	ng/ul	97
80) Pyrene	19.40	202	1305716	6.082	ng/ul	96
83) Benzo(a)anthracene	21.16	228	724761	3.516	ng/ul	98
85) Chrysene	21.21	228	668070	3.447	ng/ul	99
88) Benzo(b)fluoranthene	22.70	252	850604	4.923	ng/ul#	94
89) Benzo(k)fluoranthene	22.70	252	850604	4.962	ng/ul#	95
91) Benzo(a)pyrene	23.25	252	504545	3.287	ng/ul	97
92) Indeno(1,2,3-cd)pyrene	25.49	276	305405	1.768	ng/ul	93
94) Benzo(g,h,i)perylene	26.13	276	211208	1.477	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
Data File : BN010527.D
Acq On : 16 Apr 2020 21:34
Operator : CG/JU
Sample : L2191-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB7A0

Quant Time: Apr 17 01:07:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 10:21:51 2020
Response via : Initial Calibration

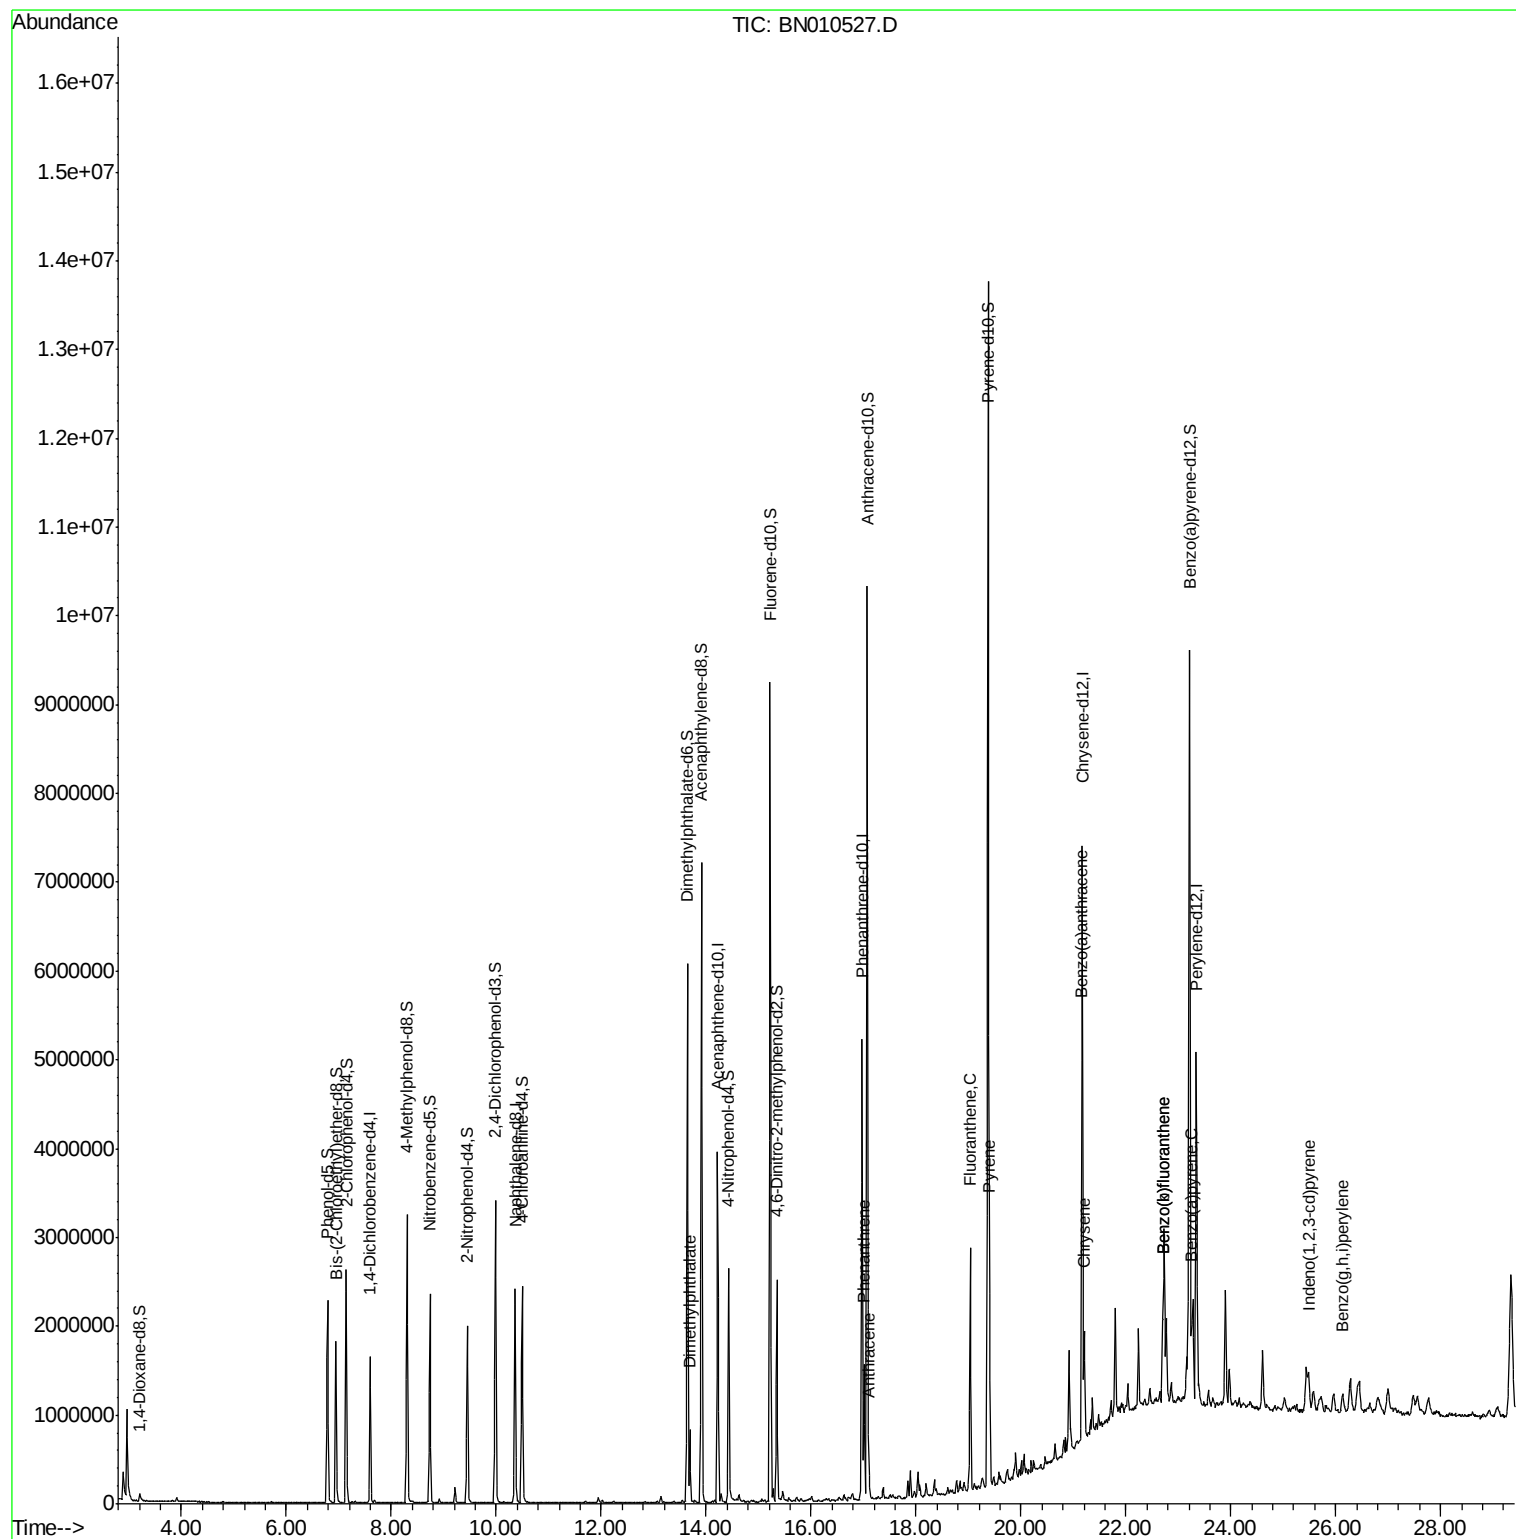

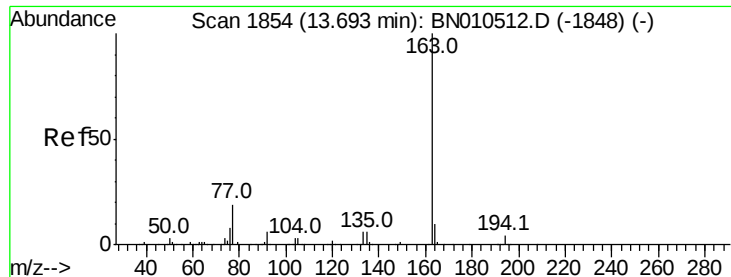

#45

Dimethylphthalate

Concen: 5.024 ng/ul

RT: 13.69 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BN010527.D

Acq: 16 Apr 2020 21:34

Instrument :

BNA_N

ClientSampleId :

CB7A0


Tot Ion:163 Resp: 511810

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9




164 10.3 8.0 12.0

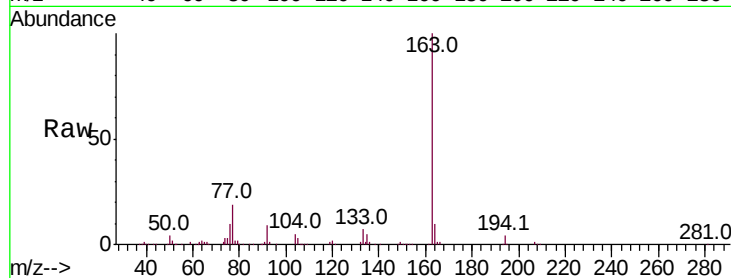

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

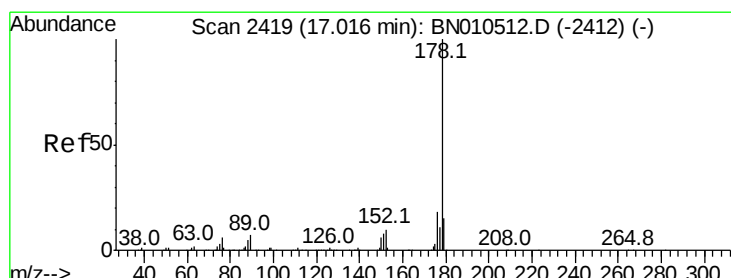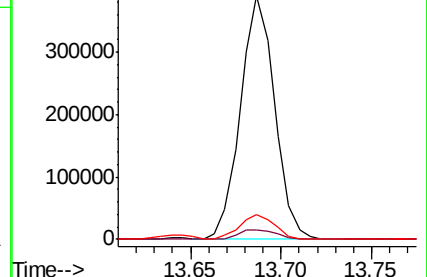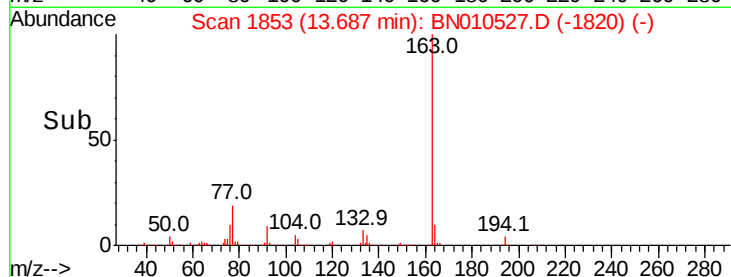

#70

Phenanthrene

Concen: 5.549 ng/ul

RT: 17.01 min Scan# 2418

Delta R.T. -0.01 min

Lab File: BN010527.D

Acq: 16 Apr 2020 21:34


Tgt Ion:178 Resp: 916498

Ion Ratio Lower Upper

178 100

179 14.8 11.4 17.2



176 18.3 15.3 22.9

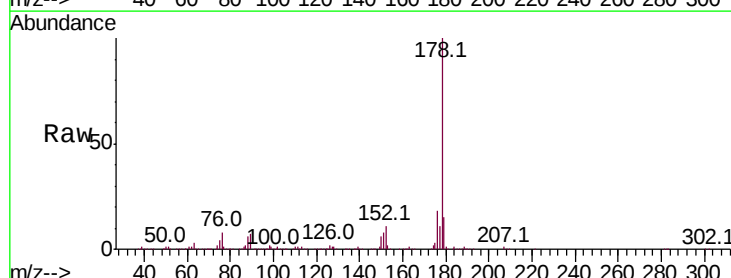


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

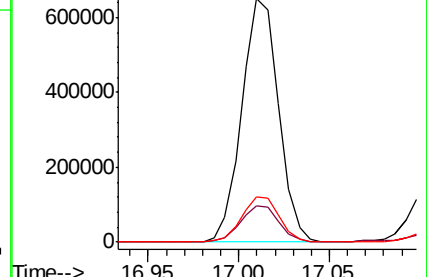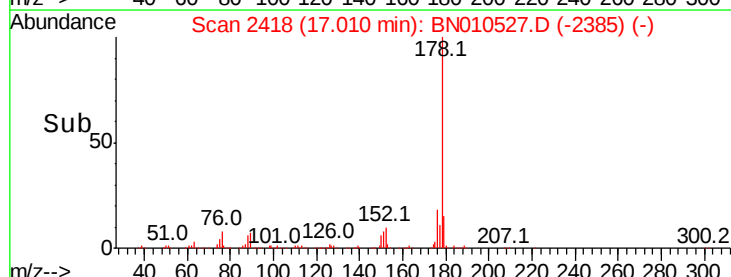

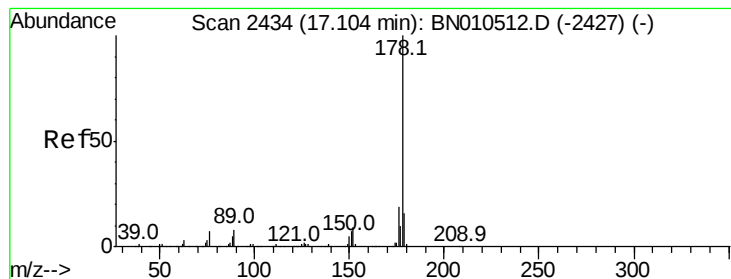

#72

Anthracene

Concen: 1.056 ng/ul

RT: 17.10 min Scan# 2434

Delta R.T. -0.00 min

Lab File: BN010527.D

Acq: 16 Apr 2020 21:34

Instrument :

BNA_N

ClientSampleId :

CB7A0


Tot Ion:178 Resp: 176813

Ion Ratio Lower Upper

178 100

179 15.3 12.3 18.5




176 19.7 14.2 21.4

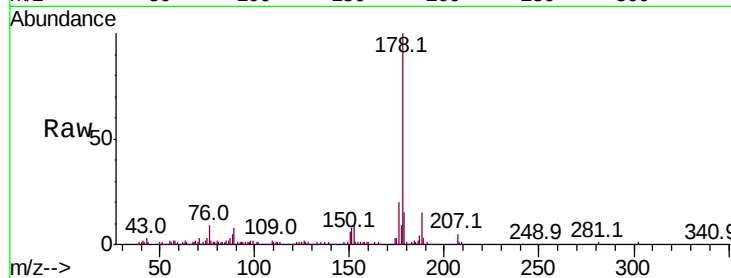

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

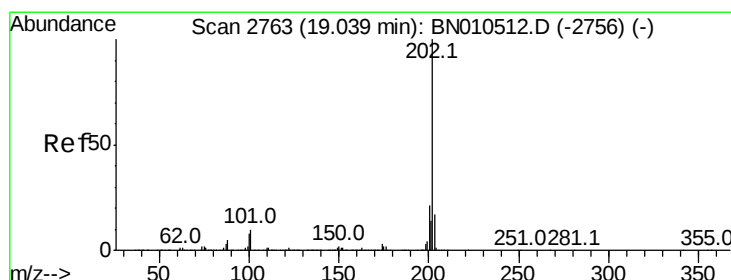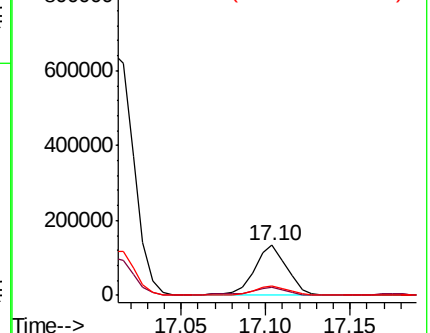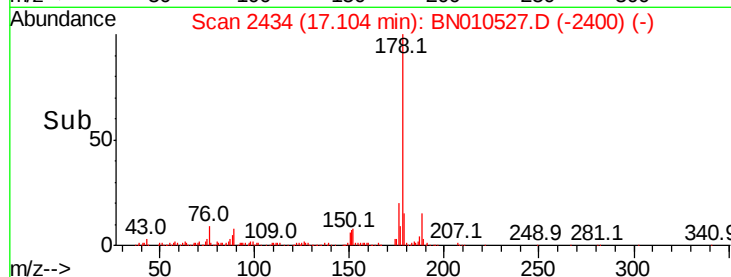

#77

Fluoranthene

Concen: 8.865 ng/ul

RT: 19.03 min Scan# 2762

Delta R.T. -0.01 min

Lab File: BN010527.D

Acq: 16 Apr 2020 21:34


Tgt Ion:202 Resp: 1590736

Ion Ratio Lower Upper

202 100

101 10.1 7.1 10.7



100 7.6 5.5 8.3

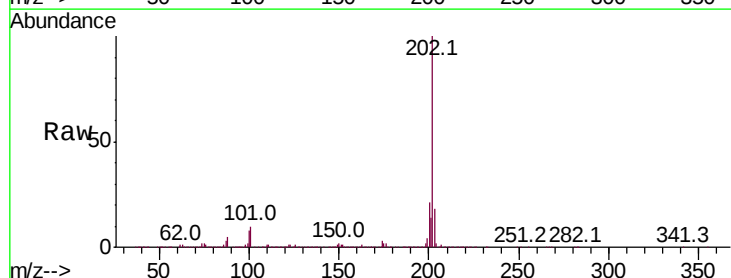


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

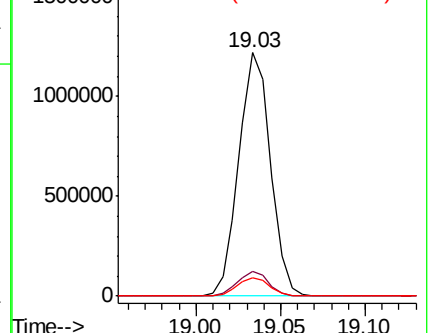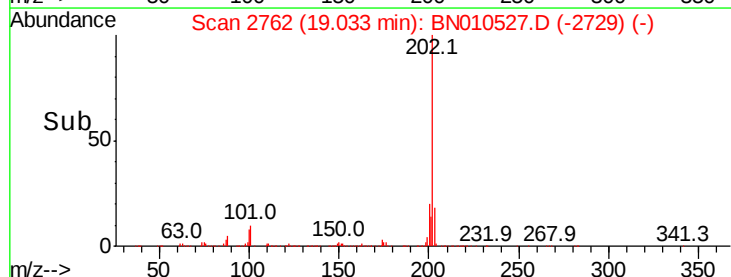


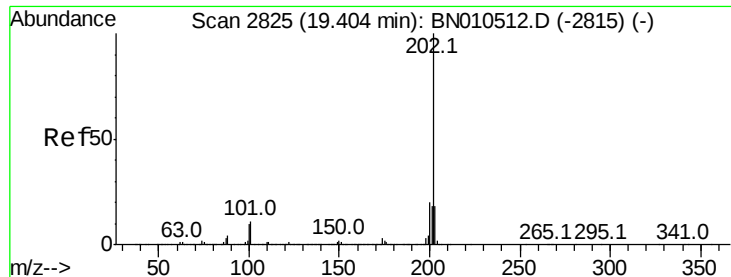




#80
Pvrene
Concen: 6.082 ng/ul
RT: 19.40 min Scan# 2824
Delta R.T. -0.01 min
Lab File: BN010527.D
Acq: 16 Apr 2020 21:34

Instrument :
BNA_N
ClientSampleId :
CB7A0

Tot Ion:202 Resp: 1305716
Ion Ratio Lower Upper
202 100
101 12.2 8.6 13.0
100 10.4 7.0 10.6

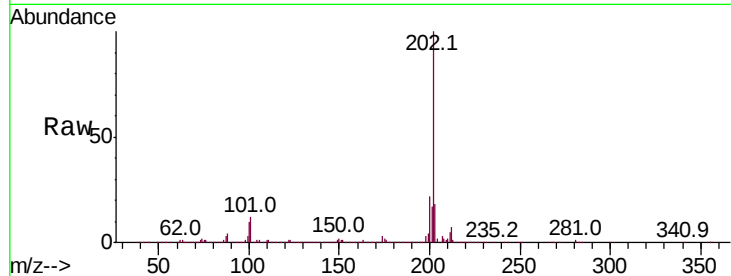


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

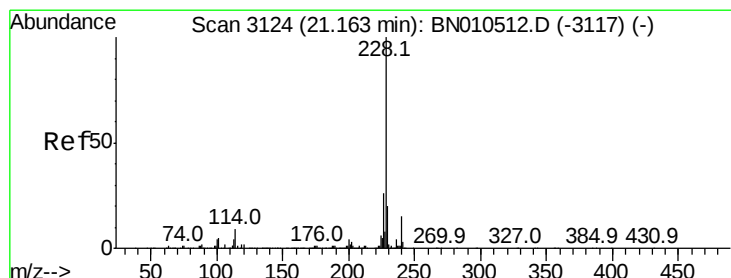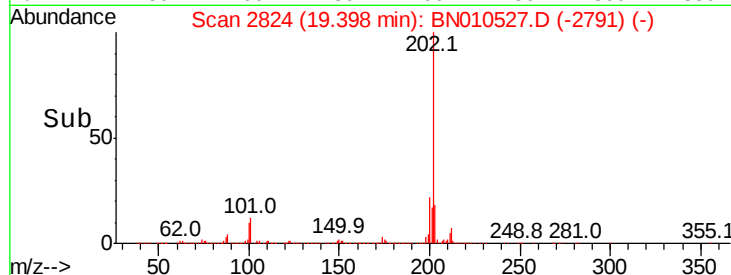
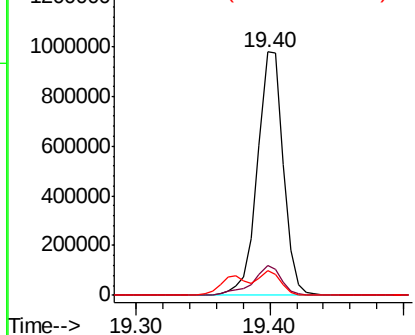



#83
Benzo(a)anthracene
Concen: 3.516 ng/ul
RT: 21.16 min Scan# 3123
Delta R.T. -0.01 min
Lab File: BN010527.D
Acq: 16 Apr 2020 21:34

Tgt Ion:228 Resp: 724761
Ion Ratio Lower Upper
228 100
229 19.5 16.0 24.0
226 27.8 21.4 32.2

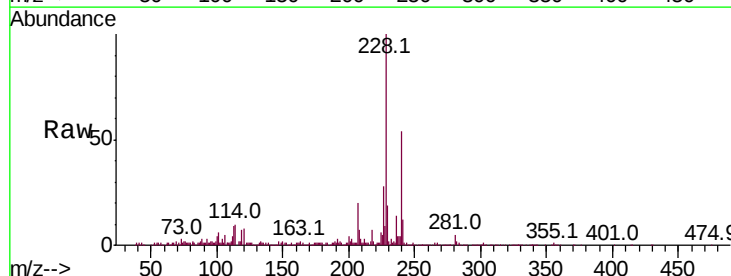

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E



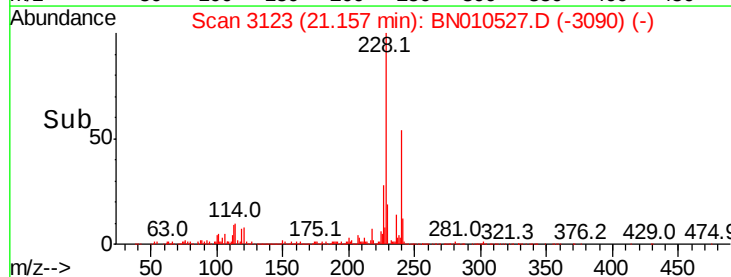
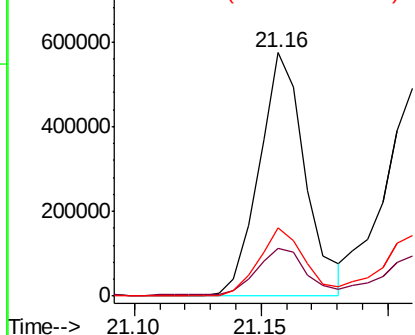


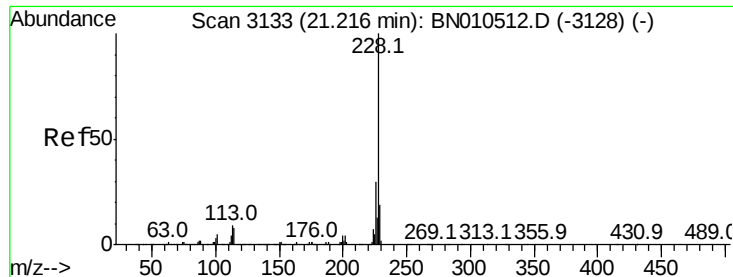

#85
 Chrysene
 Concen: 3.447 ng/ul
 RT: 21.21 min Scan# 3132
 Delta R.T. -0.01 min
 Lab File: BN010527.D
 Acq: 16 Apr 2020 21:34




Instrument :
 BNA_N
 ClientSampleId :
 CB7A0


Tot	Ion:228	Resp:	668070
Ion	Ratio	Lower	Upper
228	100		
226	29.0	23.0	34.6
229	19.1	15.0	22.4

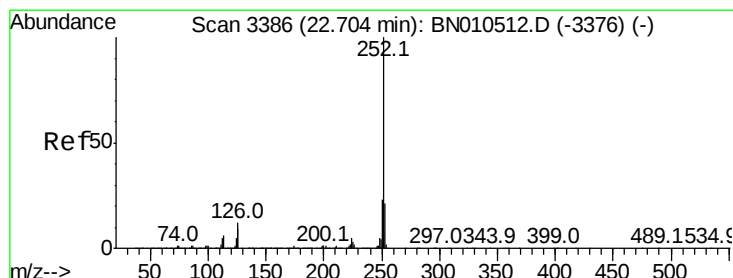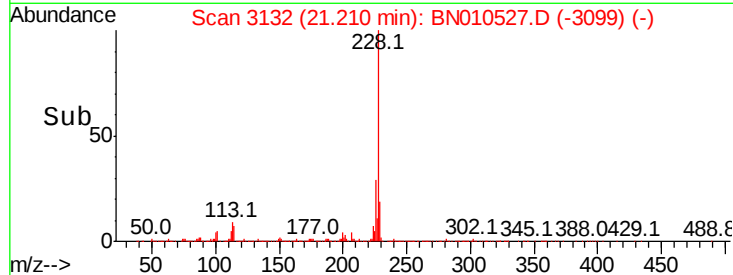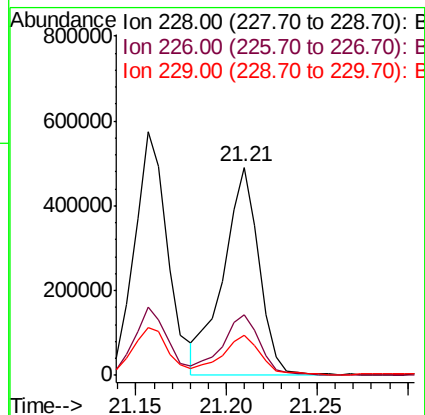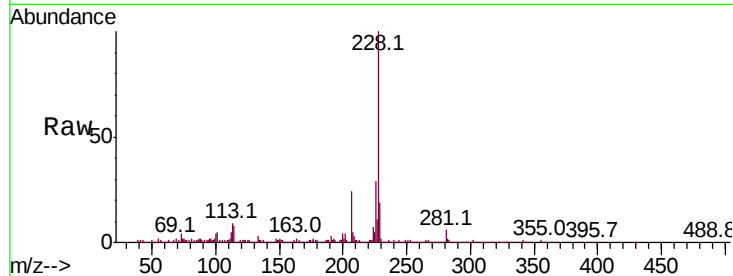

#88
 Benzo(b)fluoranthene
 Concen: 4.923 ng/ul
 RT: 22.70 min Scan# 3386
 Delta R.T. -0.00 min
 Lab File: BN010527.D
 Acq: 16 Apr 2020 21:34

Tgt	Ion:252	Resp:	850604
Ion	Ratio	Lower	Upper
252	100		
253	24.1	16.7	25.1
125	10.9	7.2	10.8#

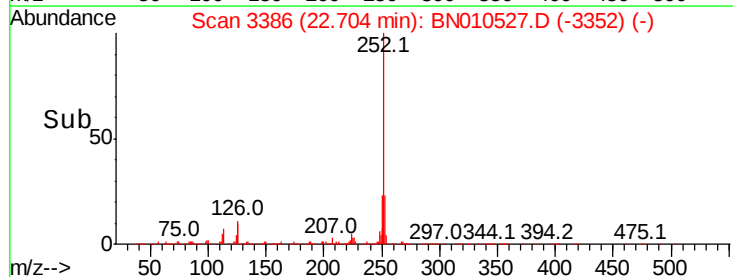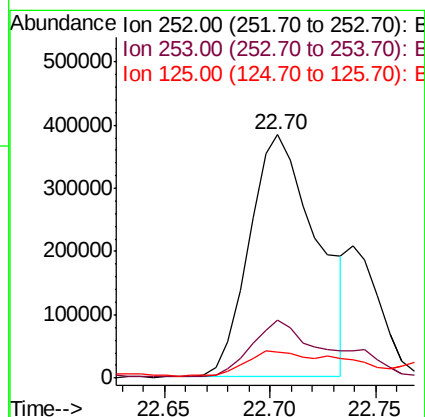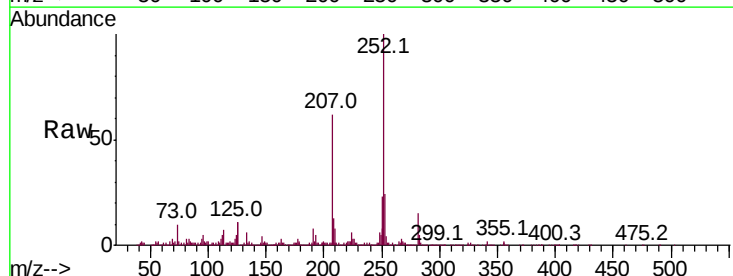

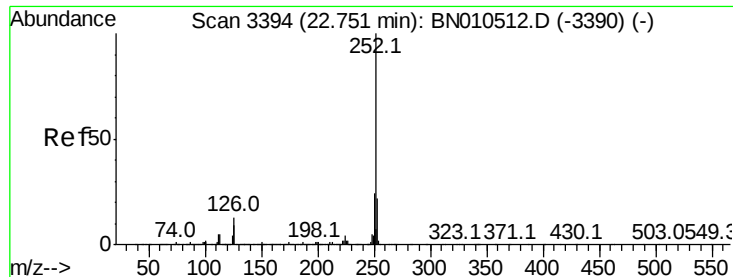

#89

Benzo(k)fluoranthene

Concen: 4.962 ng/ul

RT: 22.70 min Scan# 3386

Delta R.T. -0.05 min

Lab File: BN010527.D

Acq: 16 Apr 2020 21:34

Instrument :

BNA_N

ClientSampleId :

CB7A0





Tot Ion:252 Resp: 850604

Ion Ratio Lower Upper

252 100

253 24.1 17.4 26.2

125 10.9 6.9 10.3#

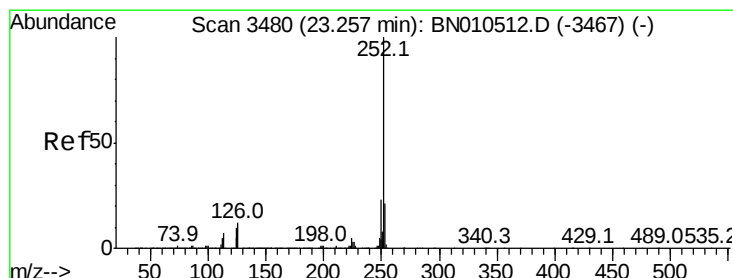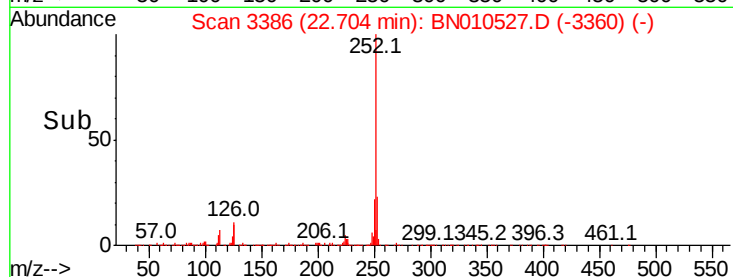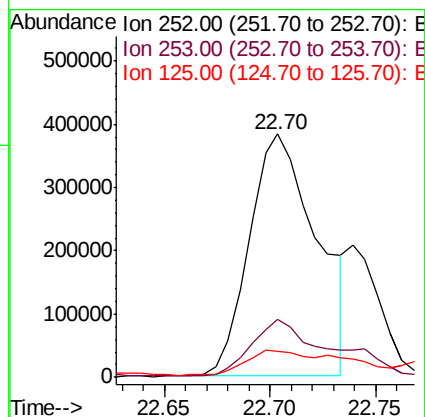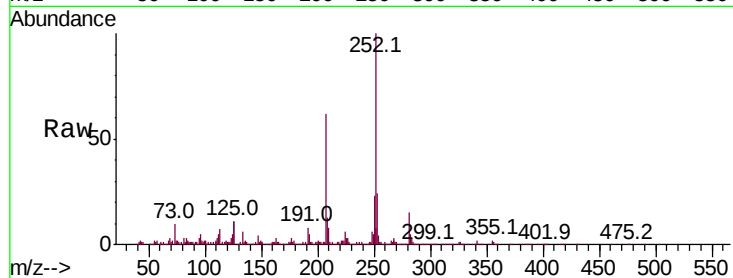

#91

Benzo(a)pyrene

Concen: 3.287 ng/ul

RT: 23.25 min Scan# 3479

Delta R.T. -0.01 min

Lab File: BN010527.D

Acq: 16 Apr 2020 21:34




Tgt Ion:252 Resp: 504545


Ion Ratio Lower Upper

252 100

253 23.7 17.8 26.8

125 11.2 7.8 11.6

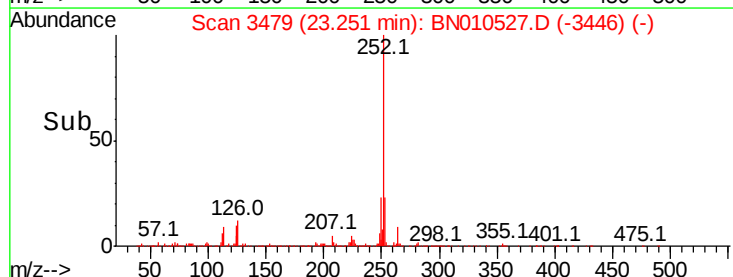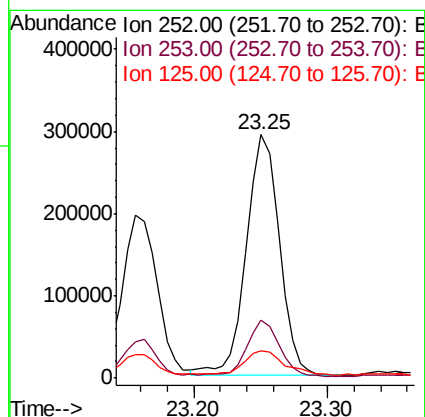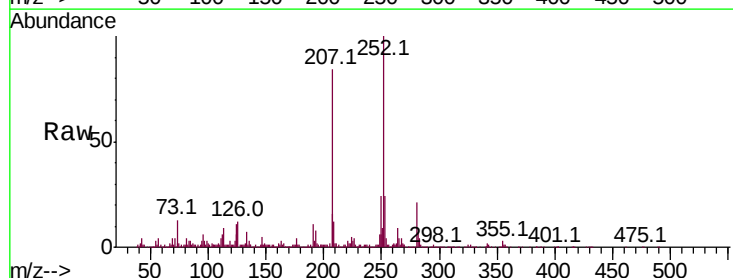




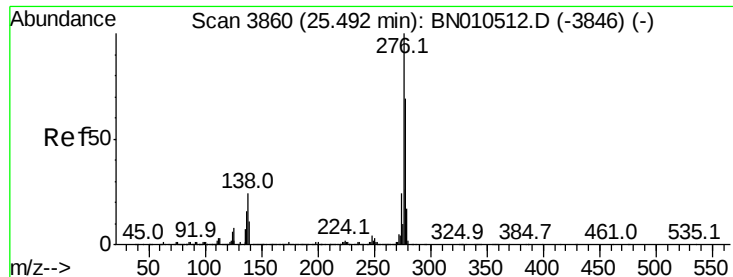


#92

Indeno(1,2,3-cd)pyrene
Concen: 1.768 ng/ul
RT: 25.49 min Scan# 3859
Delta R.T. -0.01 min
Lab File: BN010527.D
Acq: 16 Apr 2020 21:34

Instrument :
BNA_N
ClientSampleId :
CB7A0

Tot Ion	Ratio	Lower	Upper
276	100		
138	19.2	18.3	27.5
277	27.9	19.8	29.8

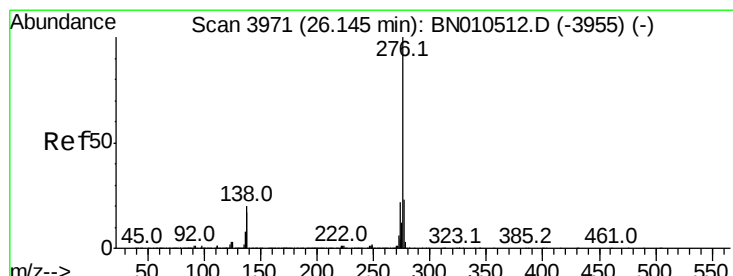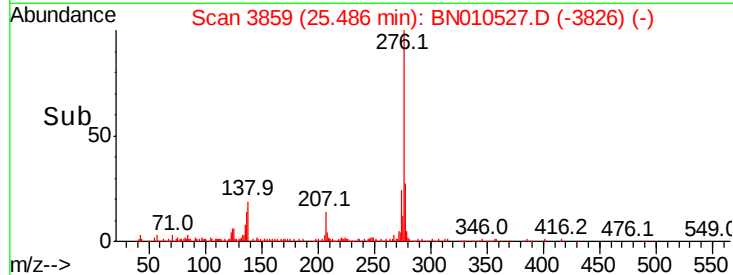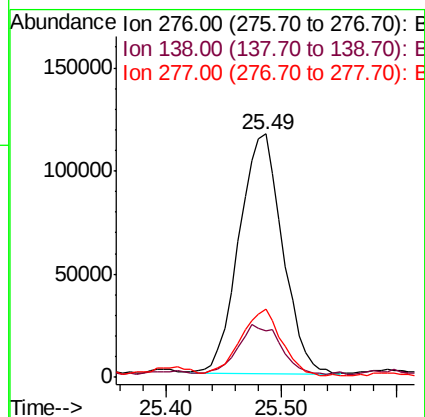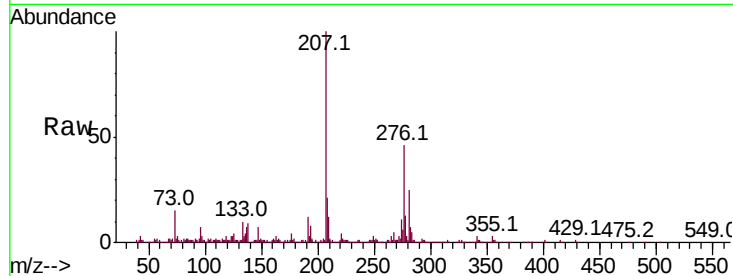

#94

Benzo(g,h,i)perylene
Concen: 1.477 ng/ul
RT: 26.13 min Scan# 3969
Delta R.T. -0.01 min
Lab File: BN010527.D
Acq: 16 Apr 2020 21:34

Tgt Ion	Ratio	Lower	Upper
276	100		
138	21.6	14.7	22.1
277	27.3	18.4	27.6

